

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030886.D
 Acq On : 13 Apr 2024 18:44
 Operator : MA/JU
 Sample : P2050-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R98

Quant Time: Apr 14 22:17:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 14 22:12:55 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.664	152	172085	20.000	ng/ul	0.00
20) Naphthalene-d8	10.446	136	748276	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.310	164	491261	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	1101696	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	1254809	20.000	ng/ul	0.00
88) Perylene-d12	24.222	264	1406709	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.176	96	14476	3.944	ng/uL	0.00
4) Pyridine-d5	3.587	84	79383	7.214	ng/ul	0.00
7) Phenol-d5	6.840	99	74665	5.364	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	253508	29.484	ng/ul	0.00
11) 2-Chlorophenol-d4	7.199	132	248164	23.499	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	154075	13.206	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	166295	32.037	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	157877	33.247	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	287161	27.623	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	435162	25.426	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	1091821	33.288	ng/ul	0.00
49) Acenaphthylene-d8	13.999	160	1249954	33.145	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	27662	4.409	ng/ul	0.00
60) Fluorene-d10	15.304	176	1002047	34.912	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.428	200	127941	26.310	ng/ul	0.00
73) Anthracene-d10	17.157	188	1759330	37.064	ng/ul	0.00
81) Pyrene-d10	19.457	212	2192603	32.501	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.022	264	2482210	38.295	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.728	165	6734	1.072	ng/ul#	Qvalue 42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030886.D
Acq On : 13 Apr 2024 18:44
Operator : MA/JU
Sample : P2050-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R98


Quant Time: Apr 14 22:17:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 14 22:12:55 2024
Response via : Initial Calibration

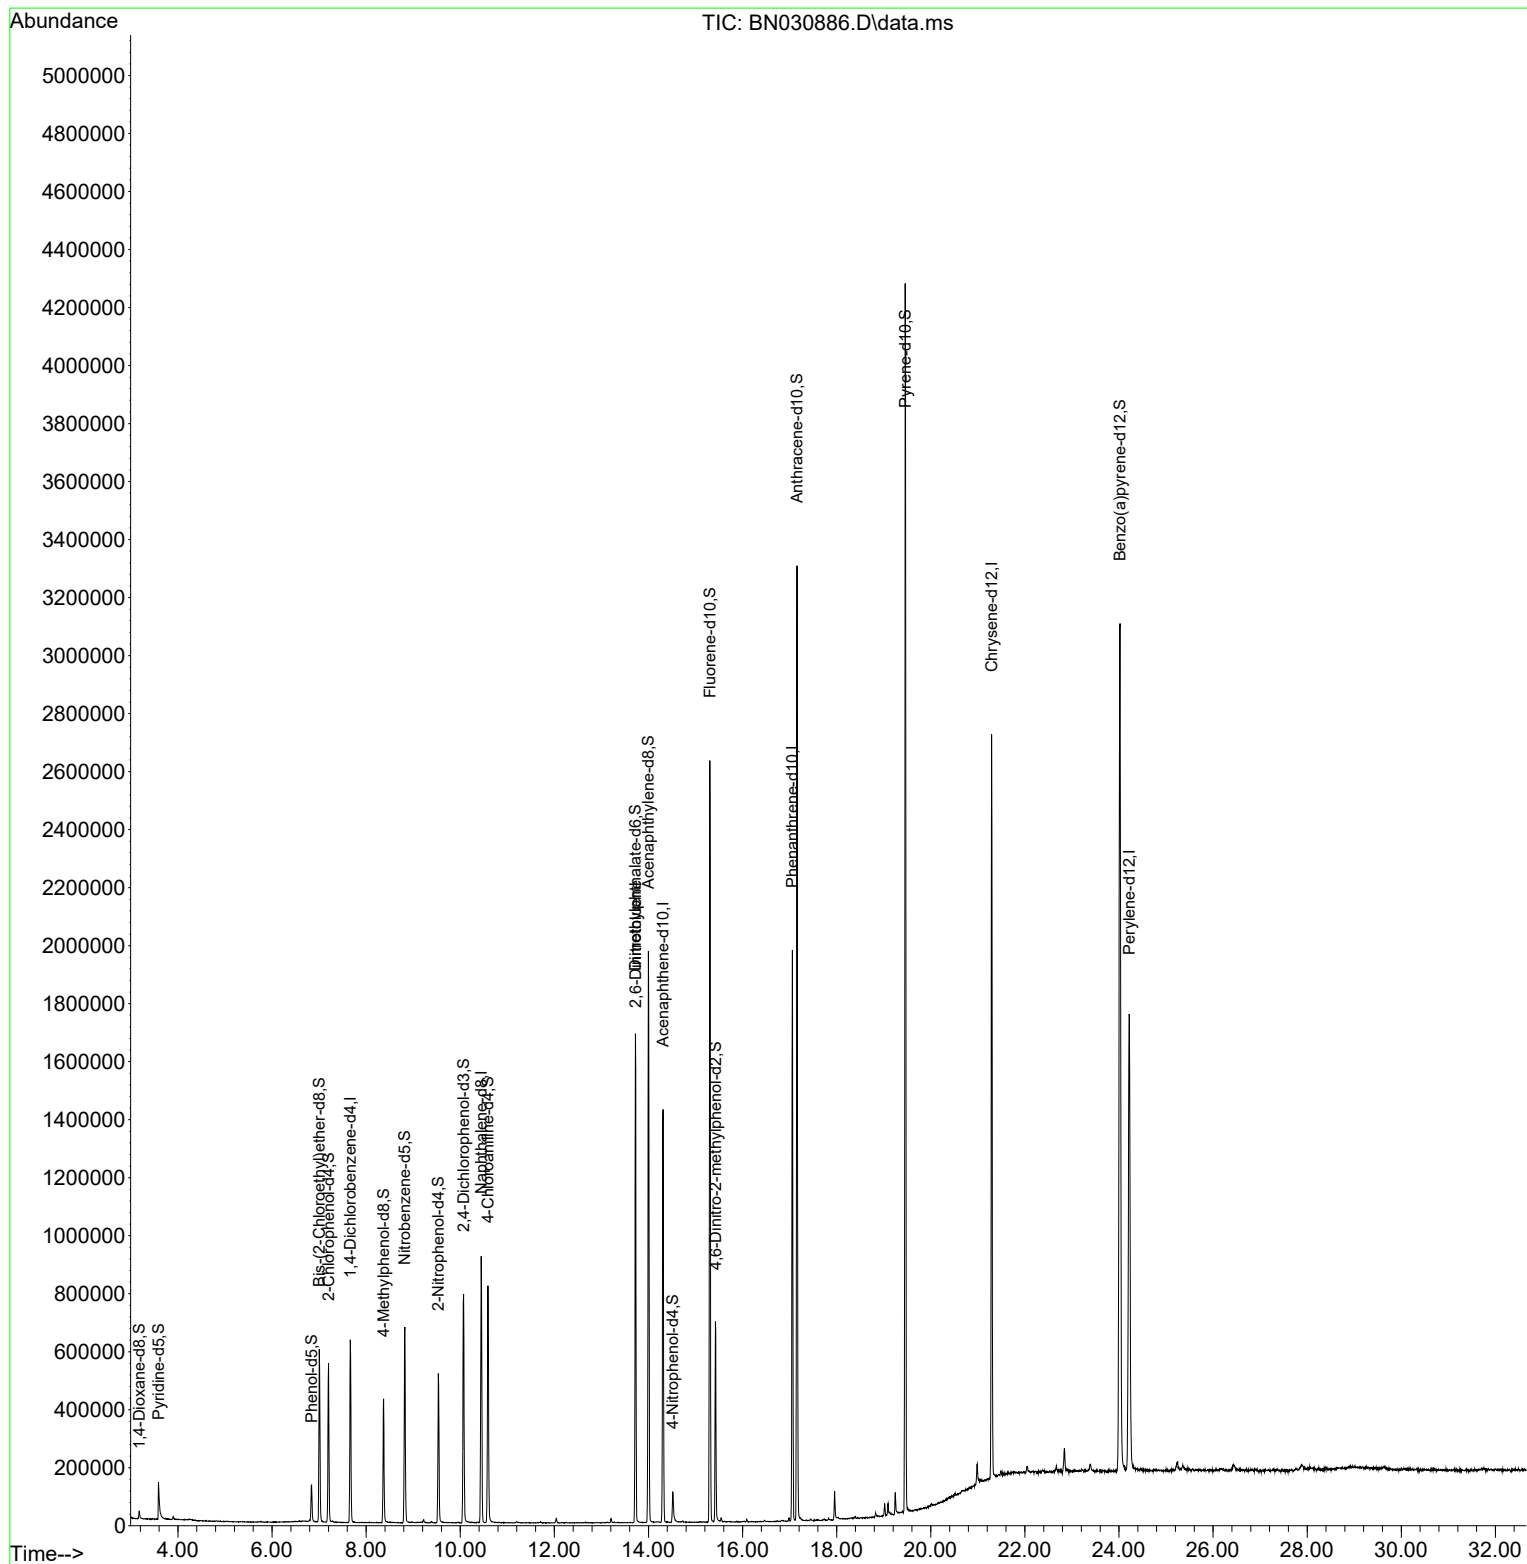

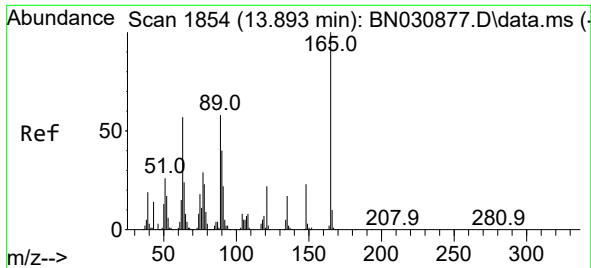

#48
 2,6-Dinitrotoluene
 Concen: 1.072 ng/ul
 RT: 13.728 min Scan# 11
 Delta R.T. -0.165 min
 Lab File: BN030886.D
 Acq: 13 Apr 2024 18:44

Instrument :
 BNA_N
 ClientSampleId :
 C0R98

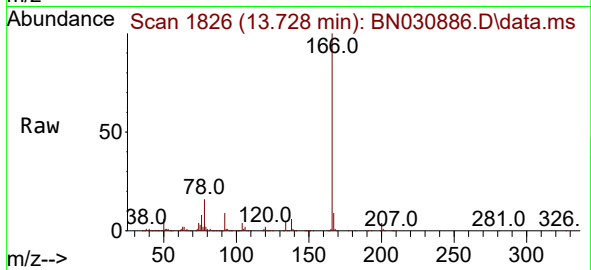

Tgt Ion:165 Resp: 6734
 Ion Ratio Lower Upper
 165 100
 89 2.6 43.5 65.3#
 121 28.7 15.7 23.5#

