

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030893.D
 Acq On : 13 Apr 2024 23:59
 Operator : MA/JU
 Sample : PB160192BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK192

Quant Time: Apr 14 22:19:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 14 22:12:55 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.664	152	156882	20.000	ng/ul	0.00
20) Naphthalene-d8	10.446	136	692353	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164	468578	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	1043152	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	1156514	20.000	ng/ul	0.00
88) Perylene-d12	24.210	264	1275964	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.176	96	21633	6.465	ng/uL	0.00
4) Pyridine-d5	3.581	84	343881	34.277	ng/ul	0.00
7) Phenol-d5	6.834	99	420290	33.117	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	257928	32.905	ng/ul	0.00
11) 2-Chlorophenol-d4	7.199	132	336914	34.995	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	339630	31.931	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	170499	35.500	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	170500	38.806	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	326123	33.905	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	550819	34.784	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	1105852	35.348	ng/ul	0.00
49) Acenaphthylene-d8	13.999	160	1239085	34.447	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	197685	33.035	ng/ul	0.00
60) Fluorene-d10	15.304	176	975299	35.625	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.422	200	122536	26.613	ng/ul	0.00
73) Anthracene-d10	17.157	188	1636856	36.419	ng/ul	0.00
81) Pyrene-d10	19.457	212	2073465	33.347	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.016	264	2250896	38.285	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.728	165	8108	1.353	ng/ul#	Qvalue 43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030893.D
Acq On : 13 Apr 2024 23:59
Operator : MA/JU
Sample : PB160192BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK192


Quant Time: Apr 14 22:19:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 14 22:12:55 2024
Response via : Initial Calibration

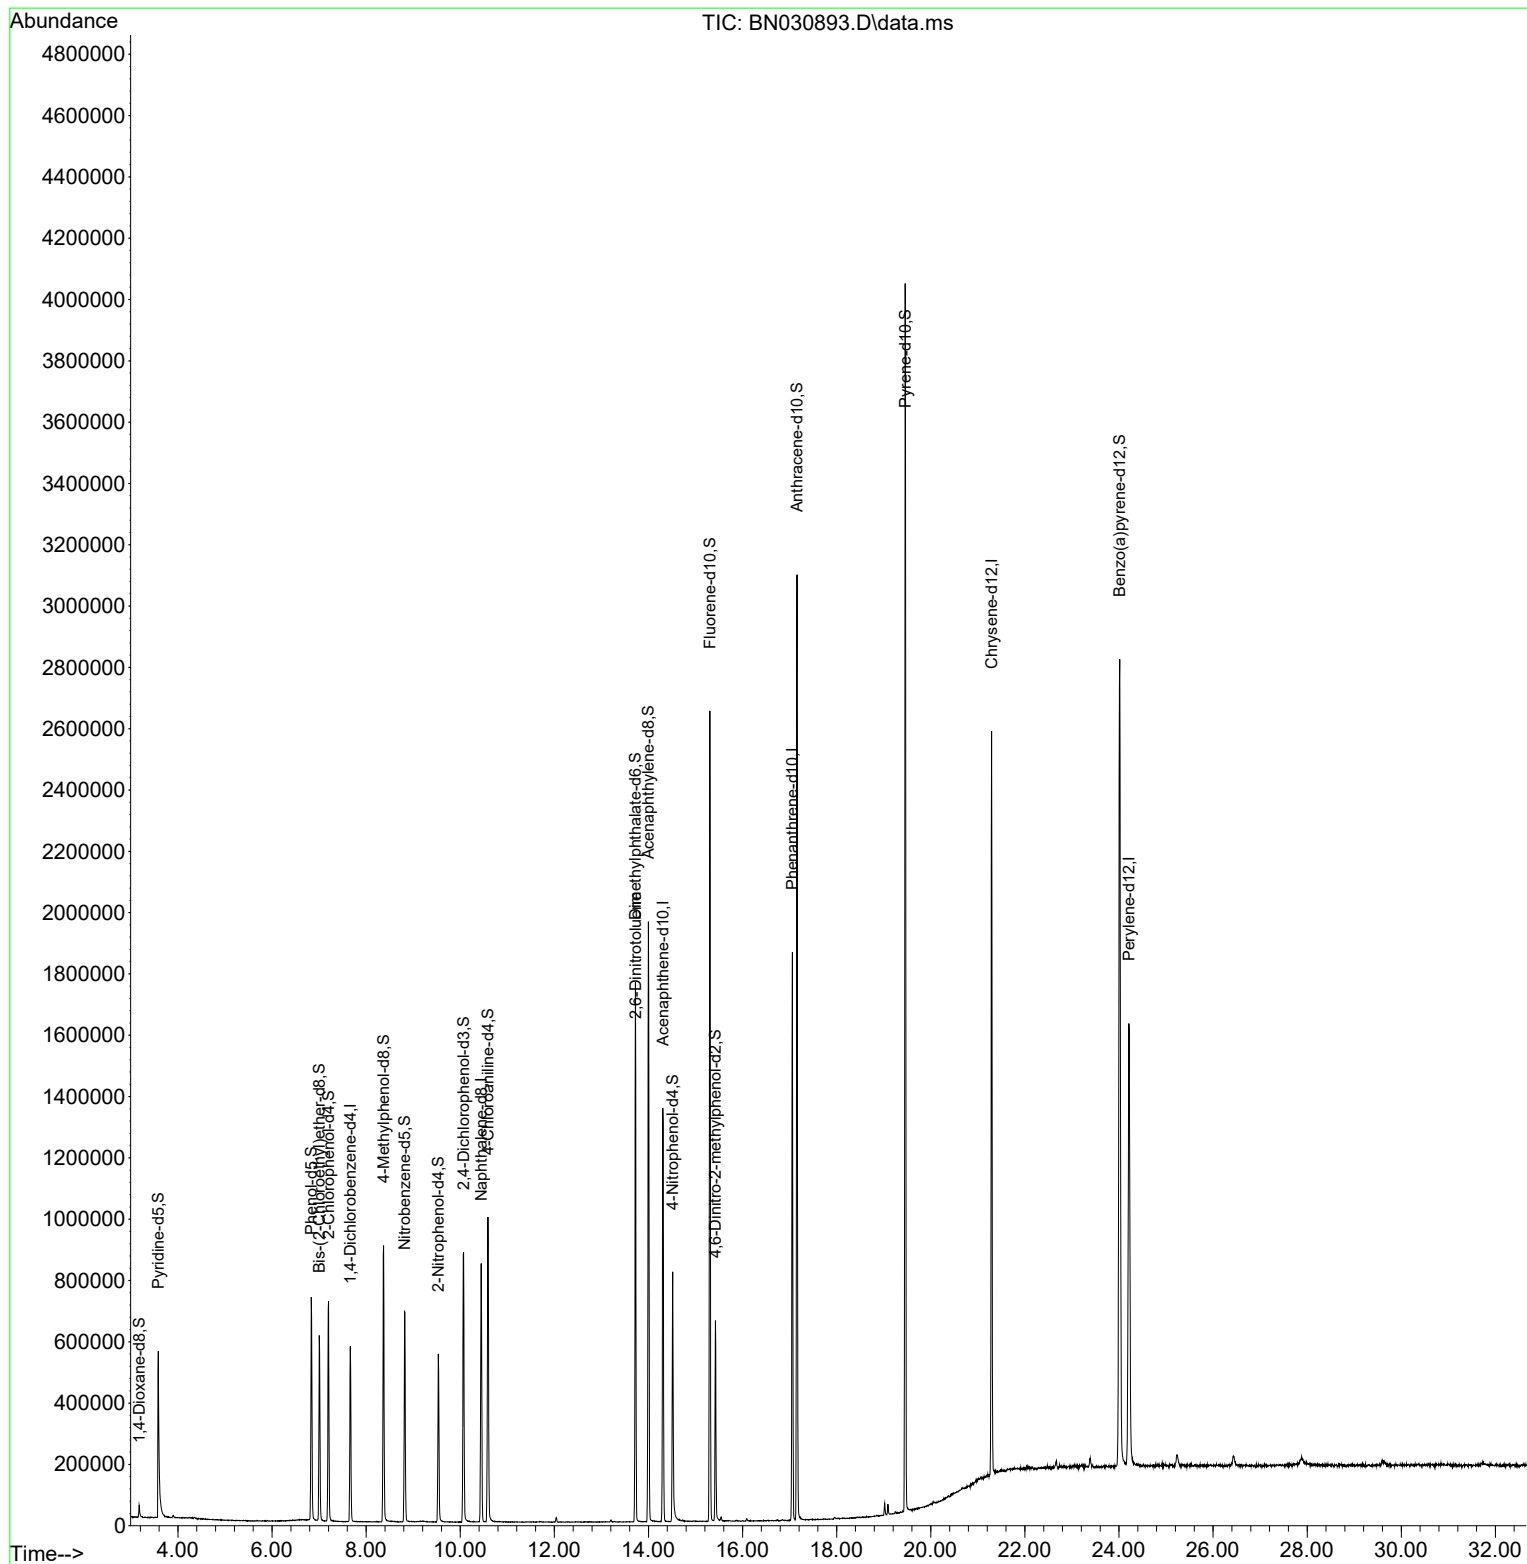

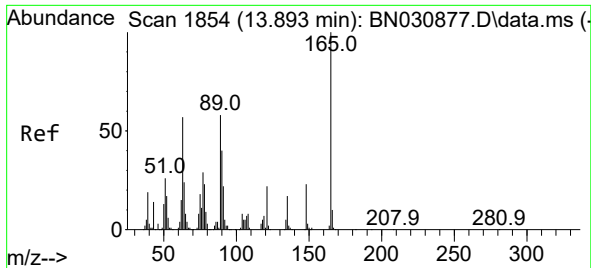

#48
 2,6-Dinitrotoluene
 Concen: 1.353 ng/ul
 RT: 13.728 min Scan# 11
 Delta R.T. -0.165 min
 Lab File: BN030893.D
 Acq: 13 Apr 2024 23:59

Instrument :
 BNA_N
 ClientSampleId :
 SBLK192

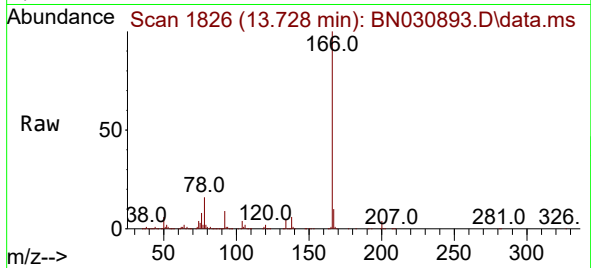

Tgt Ion:165 Resp: 8108
 Ion Ratio Lower Upper
 165 100
 89 2.7 43.5 65.3#
 121 27.4 15.7 23.5#

