

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030899.D
 Acq On : 14 Apr 2024 03:54
 Operator : MA/JU
 Sample : P2050-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R85

Quant Time: Apr 14 22:20:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 14 22:12:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	210724	20.000	ng/ul	0.00
20) Naphthalene-d8	10.445	136	934401	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.310	164	625448	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	1351148	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	1413432	20.000	ng/ul	0.00
88) Perylene-d12	24.215	264	1493773	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	15794	3.514	ng/uL	0.00
4) Pyridine-d5	3.587	84	122579	9.096	ng/ul	0.00
7) Phenol-d5	6.834	99	112307	6.588	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.004	67	364909	34.658	ng/ul	0.00
11) 2-Chlorophenol-d4	7.198	132	365347	28.252	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	227665	15.935	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	256595	39.587	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	246959	41.648	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	432932	33.350	ng/ul	0.00
31) 4-Chloroaniline-d4	10.586	131	638753	29.888	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	1512346	36.217	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	1810466	37.708	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	41027	5.136	ng/ul	0.00
60) Fluorene-d10	15.304	176	1357023	37.136	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.422	200	153779	25.785	ng/ul	0.00
73) Anthracene-d10	17.157	188	2266161	38.927	ng/ul	0.00
81) Pyrene-d10	19.457	212	2780356	36.588	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.015	264	2961241	43.023	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.733	107	56406	3.780	ng/ul	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030899.D
Acq On : 14 Apr 2024 03:54
Operator : MA/JU
Sample : P2050-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R85

Quant Time: Apr 14 22:20:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 14 22:12:55 2024
Response via : Initial Calibration

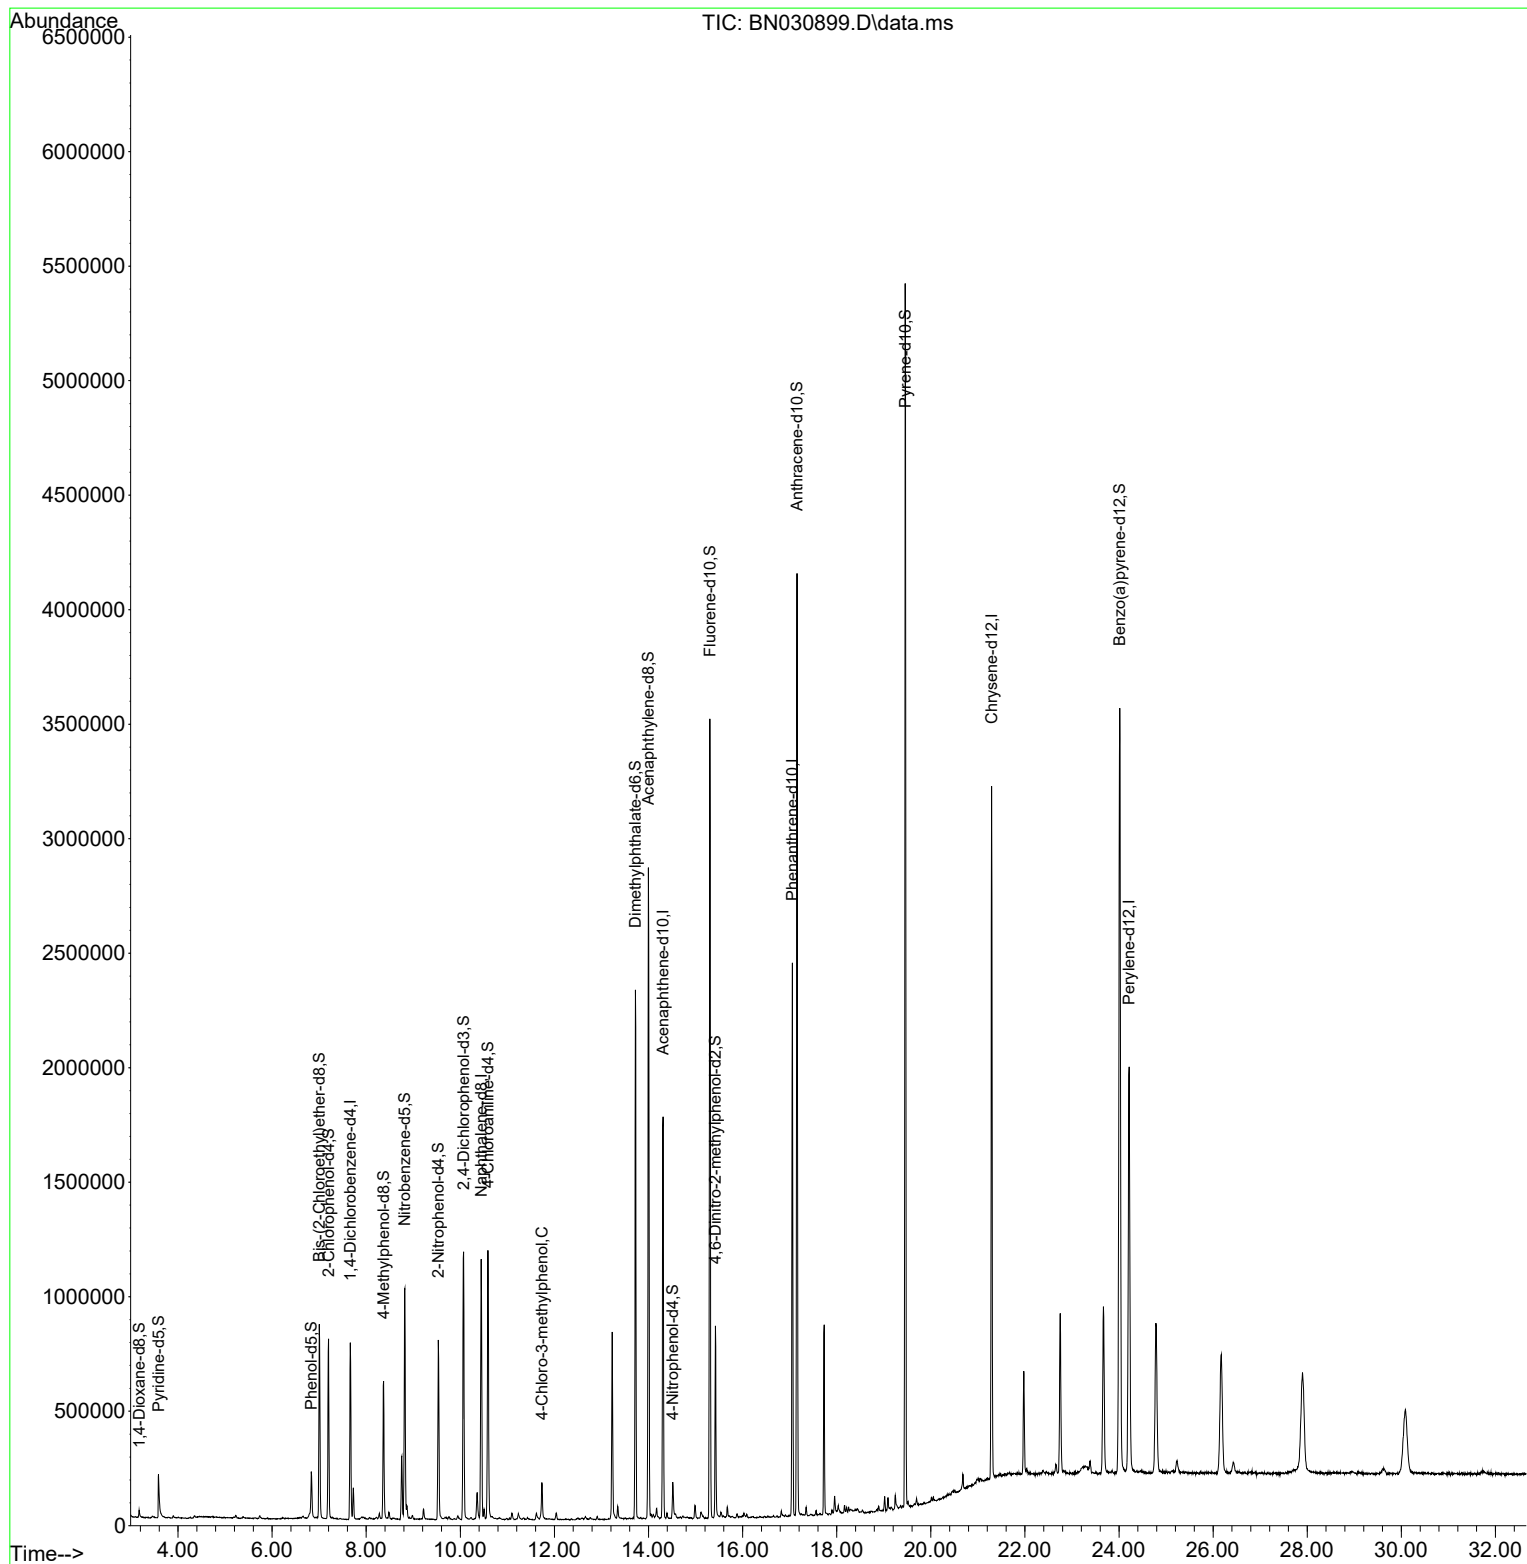

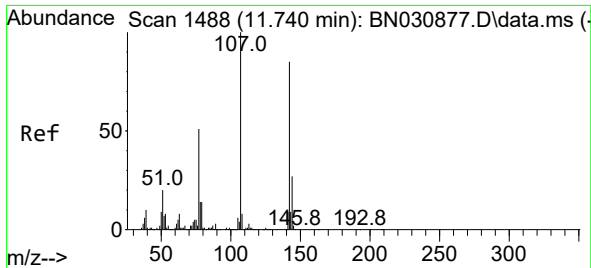

#35
 4-Chloro-3-methylphenol
 Concen: 3.780 ng/ul
 RT: 11.733 min Scan# 14
 Delta R.T. -0.006 min
 Lab File: BN030899.D
 Acq: 14 Apr 2024 03:54

Instrument :
 BNA_N
 ClientSampleId :
 C0R85

Tgt Ion:107 Resp: 56406
 Ion Ratio Lower Upper
 107 100
 144 25.6 21.4 32.0
 142 76.1 65.9 98.9

