

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030916.D
 Acq On : 14 Apr 2024 15:39
 Operator : MA/JU
 Sample : P2006-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R78

Quant Time: Apr 14 22:23:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 14 22:12:55 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	213630	20.000	ng/ul	0.00
20) Naphthalene-d8	10.446	136	953814	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.310	164	661827	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	1560336	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	1835767	20.000	ng/ul	0.00
88) Perylene-d12	24.216	264	1999626	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	18909	4.150	ng/uL	0.00
4) Pyridine-d5	3.587	84	122958	9.000	ng/ul	0.00
7) Phenol-d5	6.834	99	121615	7.037	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	388568	36.403	ng/ul	0.00
11) 2-Chlorophenol-d4	7.199	132	393498	30.015	ng/ul	0.00
15) 4-Methylphenol-d8	8.363	113	242906	16.771	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	277689	41.969	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	264169	43.643	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	469756	35.450	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	708712	32.486	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	1726355	39.069	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	2025678	39.872	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	55936	6.618	ng/ul	0.00
60) Fluorene-d10	15.304	176	1563133	40.425	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.428	200	222364	32.286	ng/ul	0.00
73) Anthracene-d10	17.157	188	2859859	42.539	ng/ul	0.00
81) Pyrene-d10	19.457	212	3655959	37.042	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.021	264	4221885	45.821	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.734	107	52841	3.469	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030916.D
Acq On : 14 Apr 2024 15:39
Operator : MA/JU
Sample : P2006-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R78

Quant Time: Apr 14 22:23:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 14 22:12:55 2024
Response via : Initial Calibration

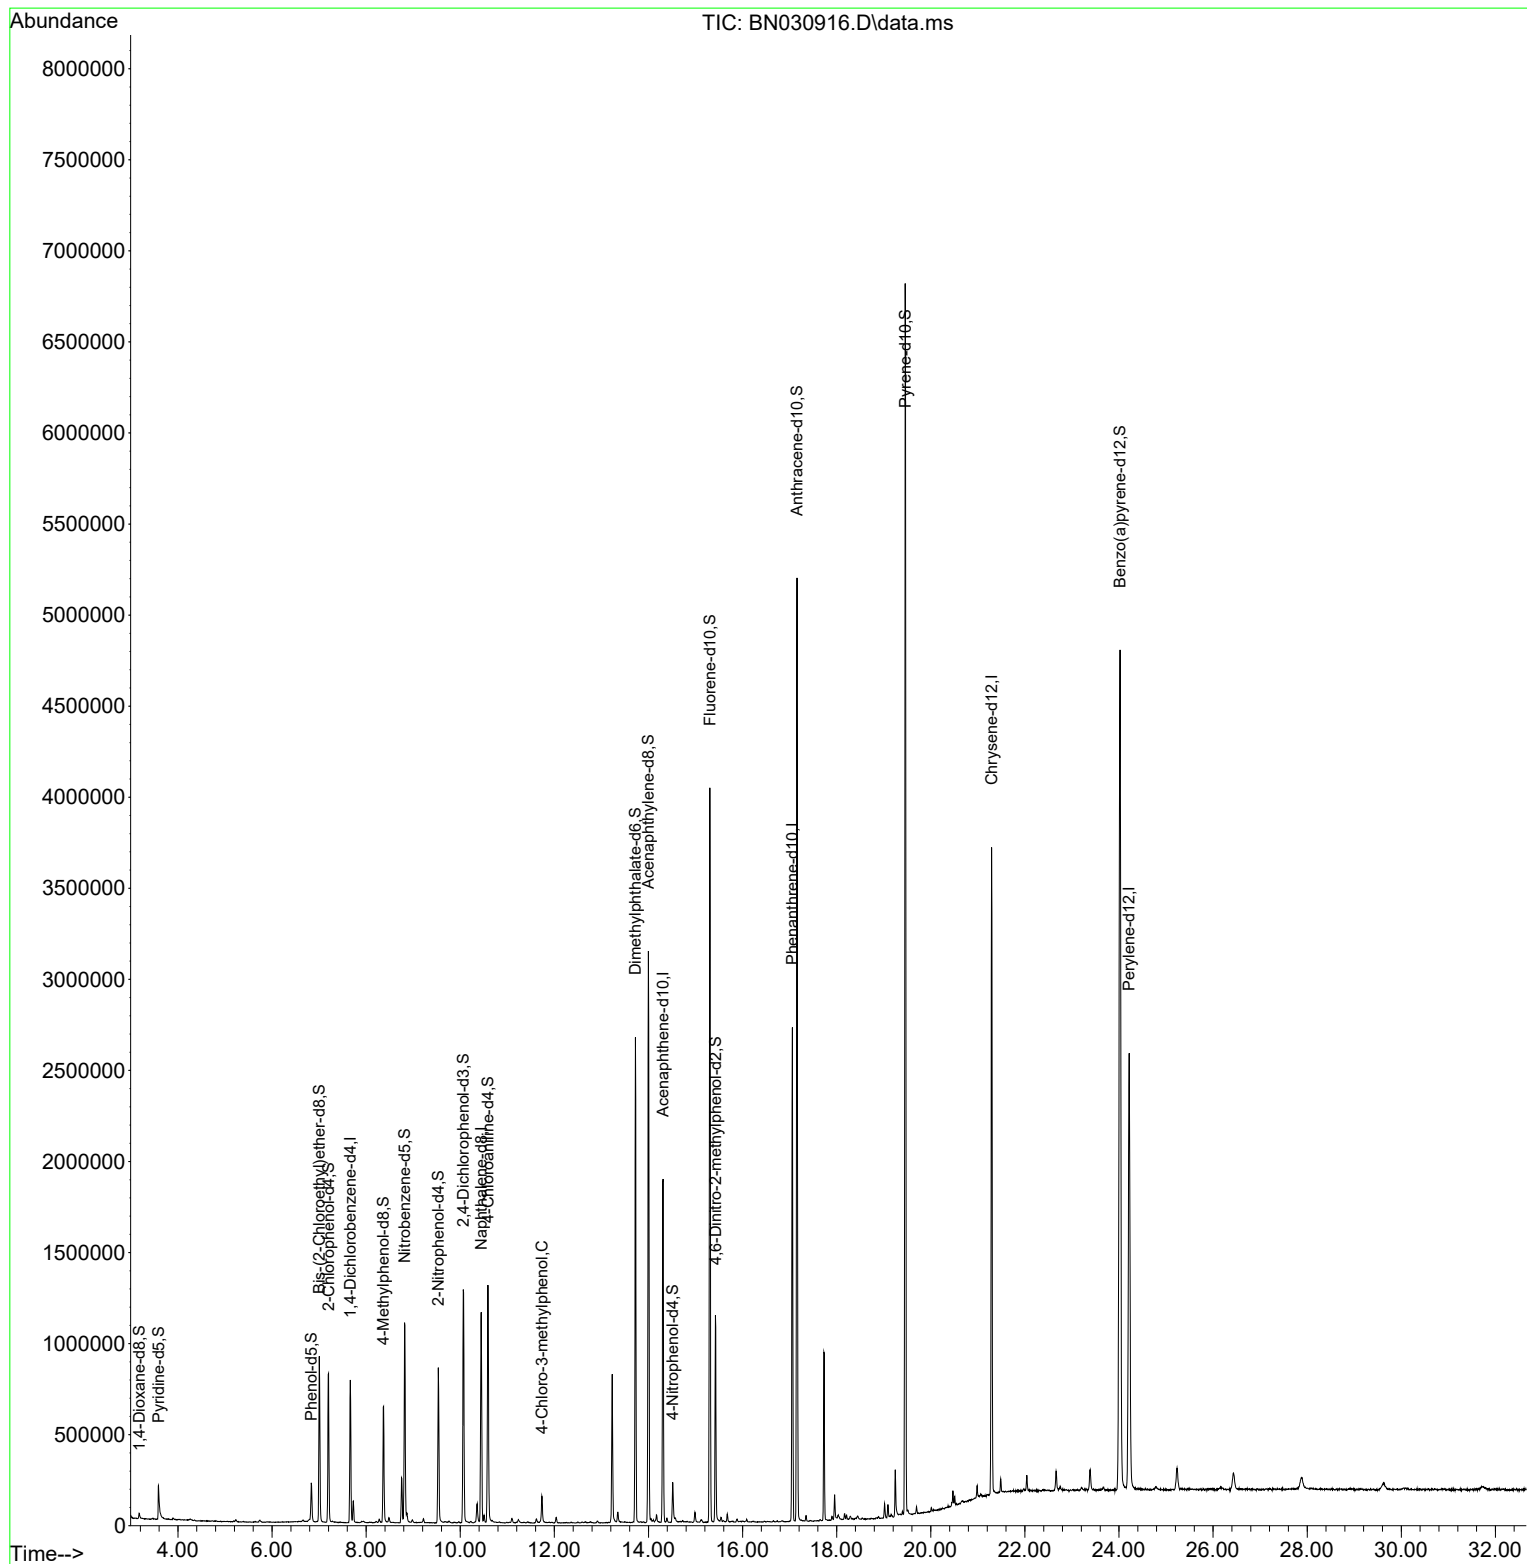

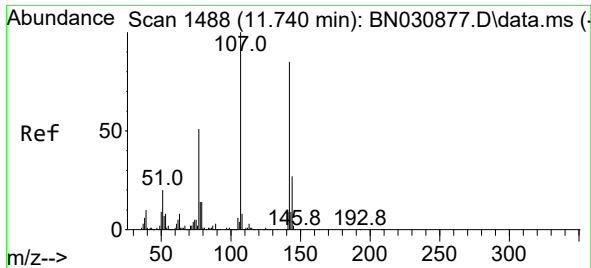

#35
 4-Chloro-3-methylphenol
 Concen: 3.469 ng/ul
 RT: 11.734 min Scan# 14
 Delta R.T. -0.006 min
 Lab File: BN030916.D
 Acq: 14 Apr 2024 15:39

Instrument :
 BNA_N
 ClientSampleId :
 MC0R78

Tgt Ion:107 Resp: 52841
 Ion Ratio Lower Upper
 107 100
 144 25.0 21.4 32.0
 142 79.2 65.9 98.9

