

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030913.D
Acq On : 14 Apr 2024 13:41
Operator : MA/JU
Sample : P2036-01
Misc :
ALS Vial : 40 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
YCSW7

Manual IntegrationsAPPROVED

Quant Time: Apr 14 22:23:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 14 22:12:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

04/16/2024
Supervised By :mohammad
ahmed

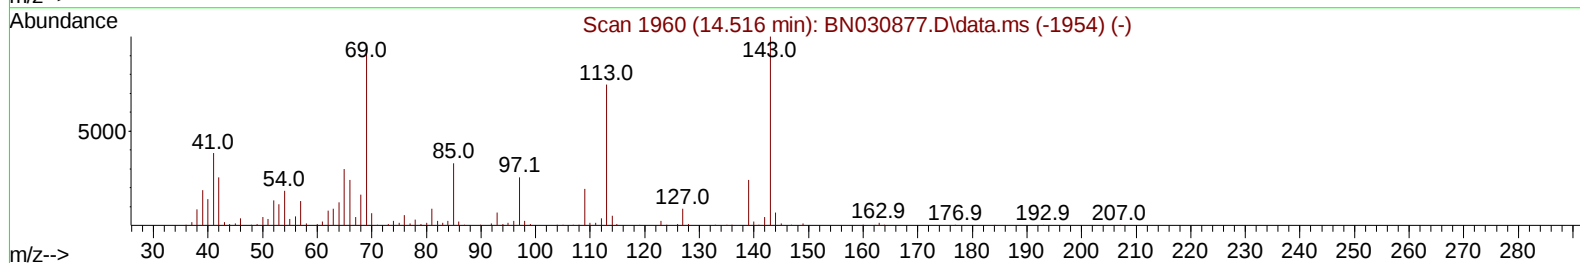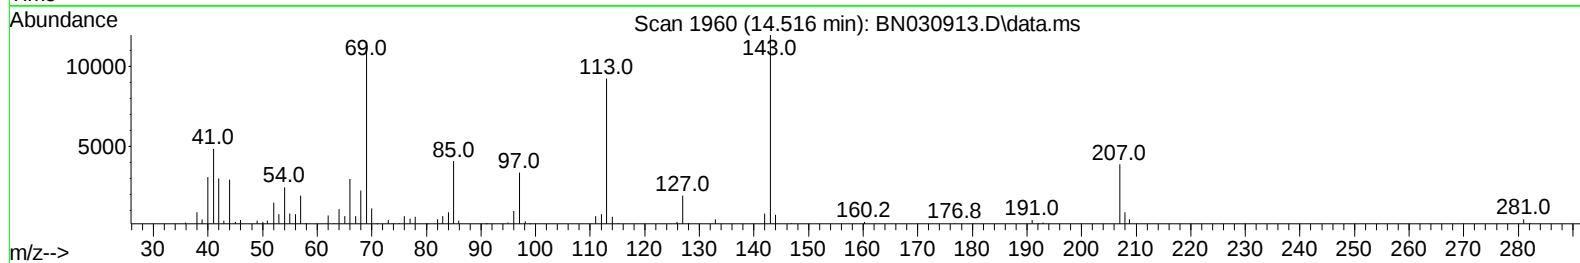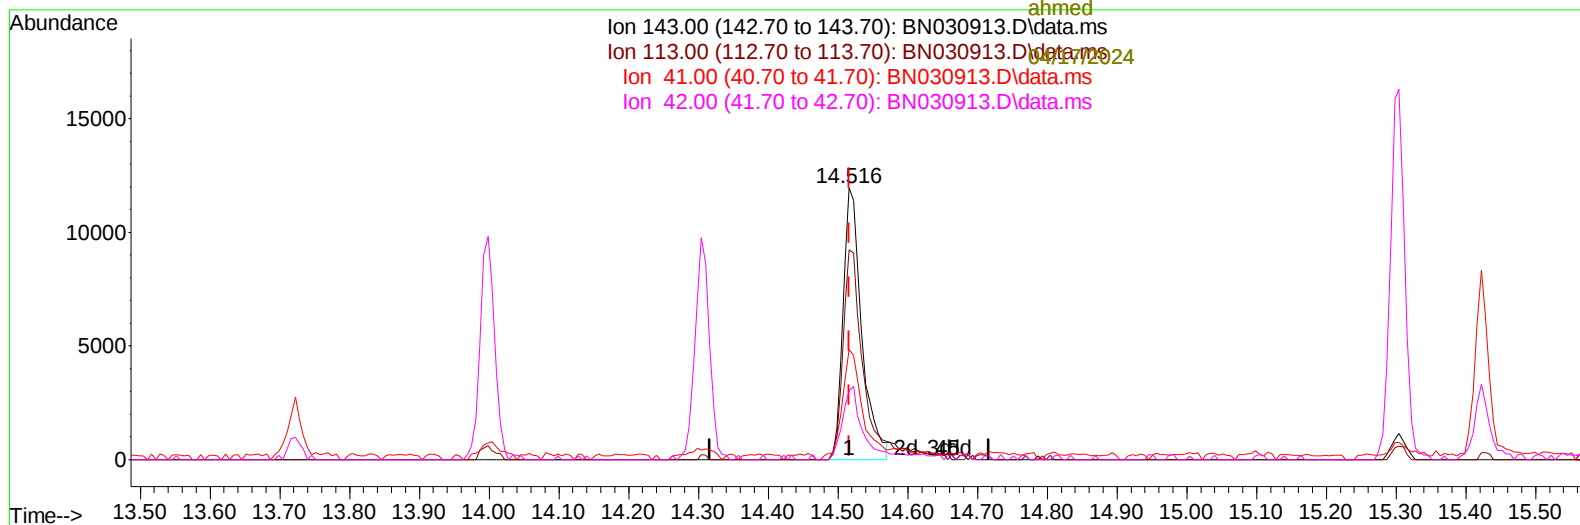

TIC: BN030913.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.516min (-0.000) 3.80 ng/u1

response 22192

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	72.10	77.13
41.00	38.20	40.48
42.00	26.70	25.10

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030913.D
Acq On : 14 Apr 2024 13:41
Operator : MA/JU
Sample : P2036-01
Misc :
ALS Vial : 40 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
YCSW7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh
Patel

04/16/2024
Supervised By :mohammad
ahmed

Quant Time: Apr 14 22:23:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 14 22:12:55 2024
Response via : Initial Calibration

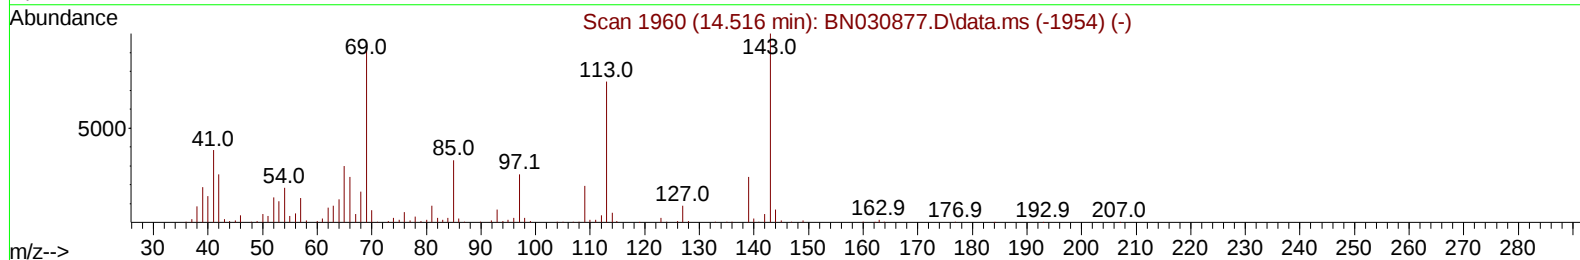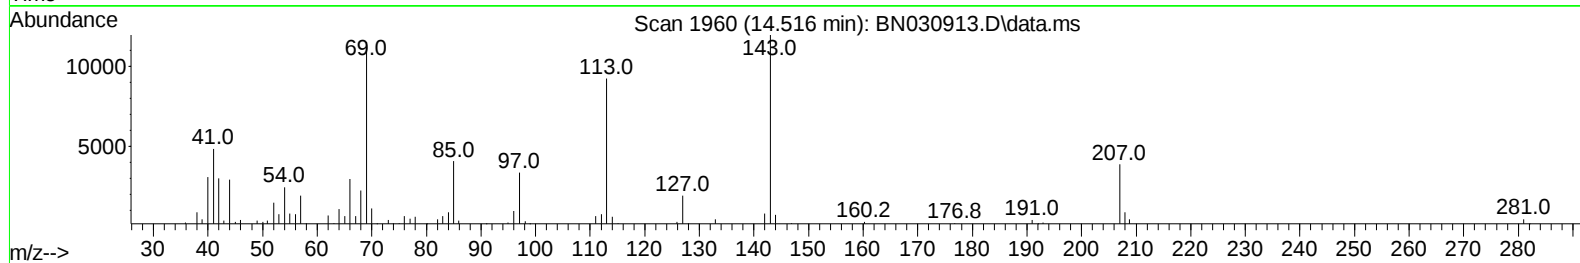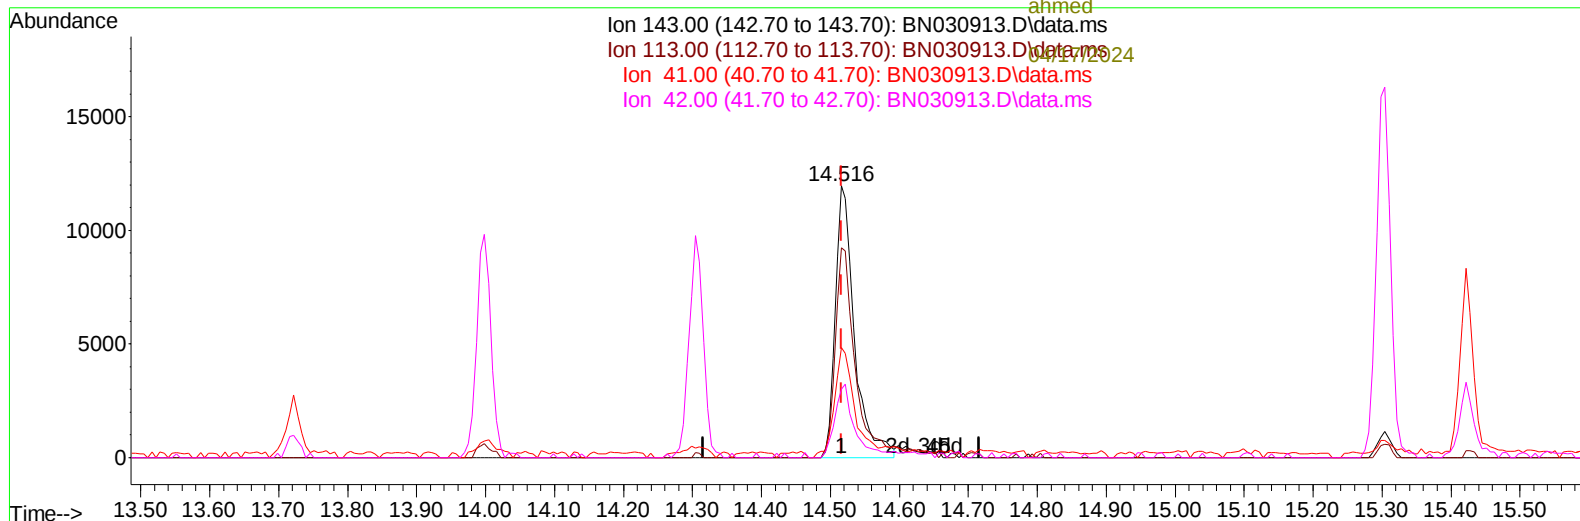

TIC: BN030913.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.516min (-0.000) 3.94 ng/ul m

response 23010

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	72.10	77.13
41.00	38.20	40.48
42.00	26.70	25.10

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030913.D
 Acq On : 14 Apr 2024 13:41
 Operator : MA/JU
 Sample : P2036-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSW7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh
 Patel

04/16/2024
 Supervised By :mohammad
 ahmed

Quant Time: Apr 14 23:37:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 14 22:12:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/17/2024						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	152423	20.000	ng/ul	0.00
20) Naphthalene-d8	10.446	136	675005	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.304	164	457389	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	1077357	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	1299520	20.000	ng/ul	0.00
88) Perylene-d12	24.216	264	1427584	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	10749	3.306	ng/uL	0.00
4) Pyridine-d5	3.593	84	46449	4.765	ng/ul	0.01
7) Phenol-d5	6.834	99	63572	5.156	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	227554	29.879	ng/ul	0.00
11) 2-Chlorophenol-d4	7.199	132	216036	23.096	ng/ul	0.00
15) 4-Methylphenol-d8	8.363	113	130633	12.641	ng/ul	0.00
21) Nitrobenzene-d5	8.816	128	152820	32.637	ng/ul	0.00
24) 2-Nitrophenol-d4	9.534	143	136810	31.938	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	254545	27.143	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	353285	22.883	ng/ul	0.00
46) Dimethylphthalate-d6	13.722	166	1014586	33.224	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	1196968	34.091	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	23010m	3.939	ng/ul	0.00
60) Fluorene-d10	15.304	176	959536	35.907	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.422	200	113789	23.928	ng/ul	0.00
73) Anthracene-d10	17.157	188	1835553	39.543	ng/ul	0.00
81) Pyrene-d10	19.457	212	2452695	35.105	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.016	264	2602098	39.558	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030913.D
Acq On : 14 Apr 2024 13:41
Operator : MA/JU
Sample : P2036-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSW7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh
Patel

04/16/2024
Supervised By :mohammad
ahmed

04/17/2024

