

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030884.D
 Acq On : 13 Apr 2024 17:26
 Operator : MA/JU
 Sample : P2050-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R79

Quant Time: Apr 14 22:17:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 14 22:12:55 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	130916	20.000	ng/u1	0.00
20) Naphthalene-d8	10.446	136	573702	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.310	164	386237	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.057	188	839774	20.000	ng/u1	0.00
79) Chrysene-d12	21.292	240	944436	20.000	ng/u1	0.00
88) Perylene-d12	24.215	264	1076434	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	12538	4.490	ng/uL	0.00
4) Pyridine-d5	3.587	84	72956	8.714	ng/u1	0.00
7) Phenol-d5	6.840	99	76280	7.203	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	267944	40.963	ng/u1	0.00
11) 2-Chlorophenol-d4	7.199	132	254758	31.710	ng/u1	0.00
15) 4-Methylphenol-d8	8.369	113	160701	18.105	ng/u1	0.00
21) Nitrobenzene-d5	8.822	128	180717	45.409	ng/u1	0.00
24) 2-Nitrophenol-d4	9.534	143	163384	44.877	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	306356	38.437	ng/u1	0.00
31) 4-Chloroaniline-d4	10.587	131	445813	33.975	ng/u1	0.00
46) Dimethylphthalate-d6	13.728	166	1177855	45.676	ng/u1	0.00
49) Acenaphthylene-d8	13.998	160	1316817	44.413	ng/u1	0.00
54) 4-Nitrophenol-d4	14.516	143	25655	5.201	ng/u1	0.00
60) Fluorene-d10	15.304	176	1043255	46.231	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.428	200	114965	31.015	ng/u1	0.00
73) Anthracene-d10	17.157	188	1772320	48.982	ng/u1	0.00
81) Pyrene-d10	19.457	212	2170360	42.743	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.021	264	2410317	48.596	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.740	107	37394	4.081	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030884.D
Acq On : 13 Apr 2024 17:26
Operator : MA/JU
Sample : P2050-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R79


Quant Time: Apr 14 22:17:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 14 22:12:55 2024
Response via : Initial Calibration

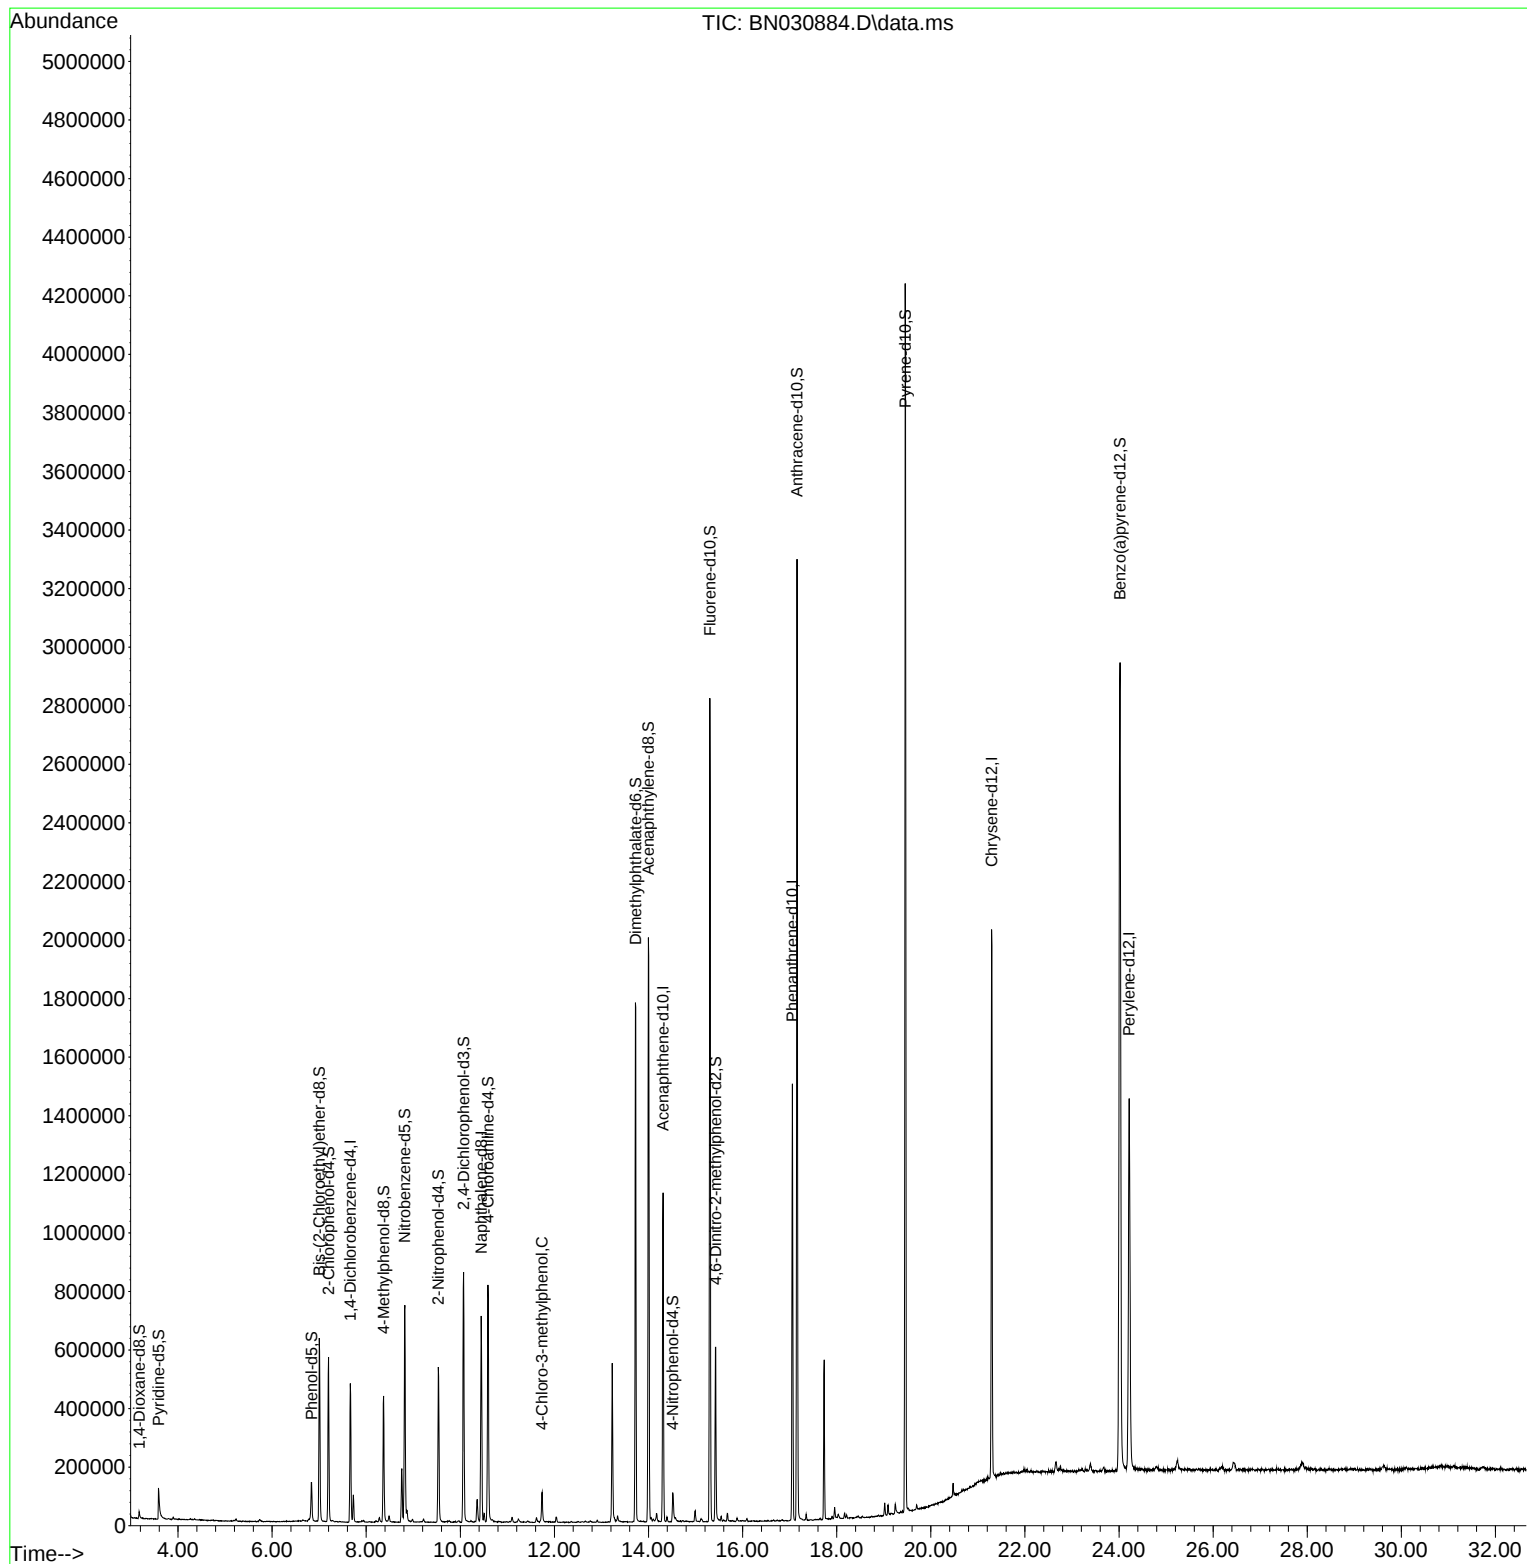

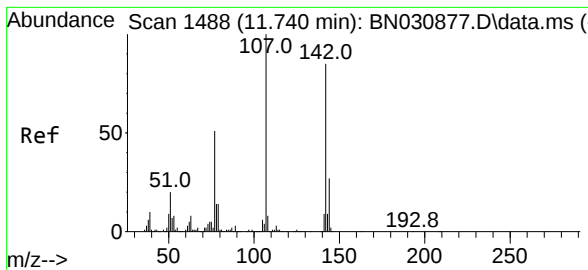

#35
 4-Chloro-3-methylphenol
 Concen: 4.081 ng/ul
 RT: 11.740 min Scan# 1488
 Delta R.T. -0.000 min
 Lab File: BN030884.D
 Acq: 13 Apr 2024 17:26

Instrument :
 BNA_N
 ClientSampleId :
 MC0R79

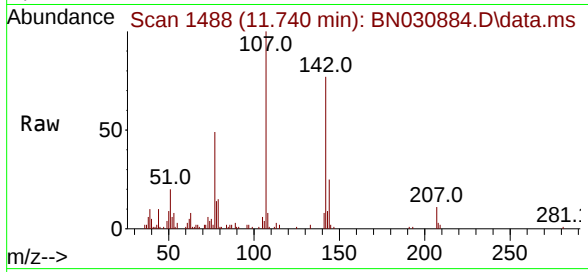

Tgt Ion:	107	Resp:	37394
Ion	Ratio	Lower	Upper
107	100		
144	25.3	21.4	32.0
142	77.4	65.9	98.9

