

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030909.D
 Acq On : 14 Apr 2024 11:04
 Operator : MA/JU
 Sample : P2036-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSY1

Quant Time: Apr 14 22:22:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 14 22:12:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	189157	20.000	ng/u1	0.00
20) Naphthalene-d8	10.446	136	829557	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.304	164	546729	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.057	188	1205219	20.000	ng/u1	0.00
79) Chrysene-d12	21.292	240	1304571	20.000	ng/u1	0.00
88) Perylene-d12	24.210	264	1371206	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	17863	4.428	ng/uL	0.00
4) Pyridine-d5	3.587	84	92760	7.668	ng/u1	0.00
7) Phenol-d5	6.834	99	124949	8.166	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	360043	38.095	ng/u1	0.00
11) 2-Chlorophenol-d4	7.199	132	377234	32.498	ng/u1	0.00
15) 4-Methylphenol-d8	8.369	113	236840	18.468	ng/u1	0.00
21) Nitrobenzene-d5	8.816	128	250851	43.592	ng/u1	0.00
24) 2-Nitrophenol-d4	9.534	143	239484	45.492	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	427493	37.093	ng/u1	0.00
31) 4-Chloroaniline-d4	10.587	131	571958	30.145	ng/u1	0.00
46) Dimethylphthalate-d6	13.722	166	1531912	41.967	ng/u1	0.00
49) Acenaphthylene-d8	13.998	160	1770231	42.179	ng/u1	0.00
54) 4-Nitrophenol-d4	14.516	143	44035	6.307	ng/u1	0.00
60) Fluorene-d10	15.304	176	1369084	42.861	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.422	200	180906	34.006	ng/u1	0.00
73) Anthracene-d10	17.157	188	2323584	44.746	ng/u1	0.00
81) Pyrene-d10	19.457	212	2845678	40.572	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.015	264	2983055	47.214	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.211	88	6913	1.600	ng/uL#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030909.D
Acq On : 14 Apr 2024 11:04
Operator : MA/JU
Sample : P2036-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY1

Quant Time: Apr 14 22:22:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 14 22:12:55 2024
Response via : Initial Calibration

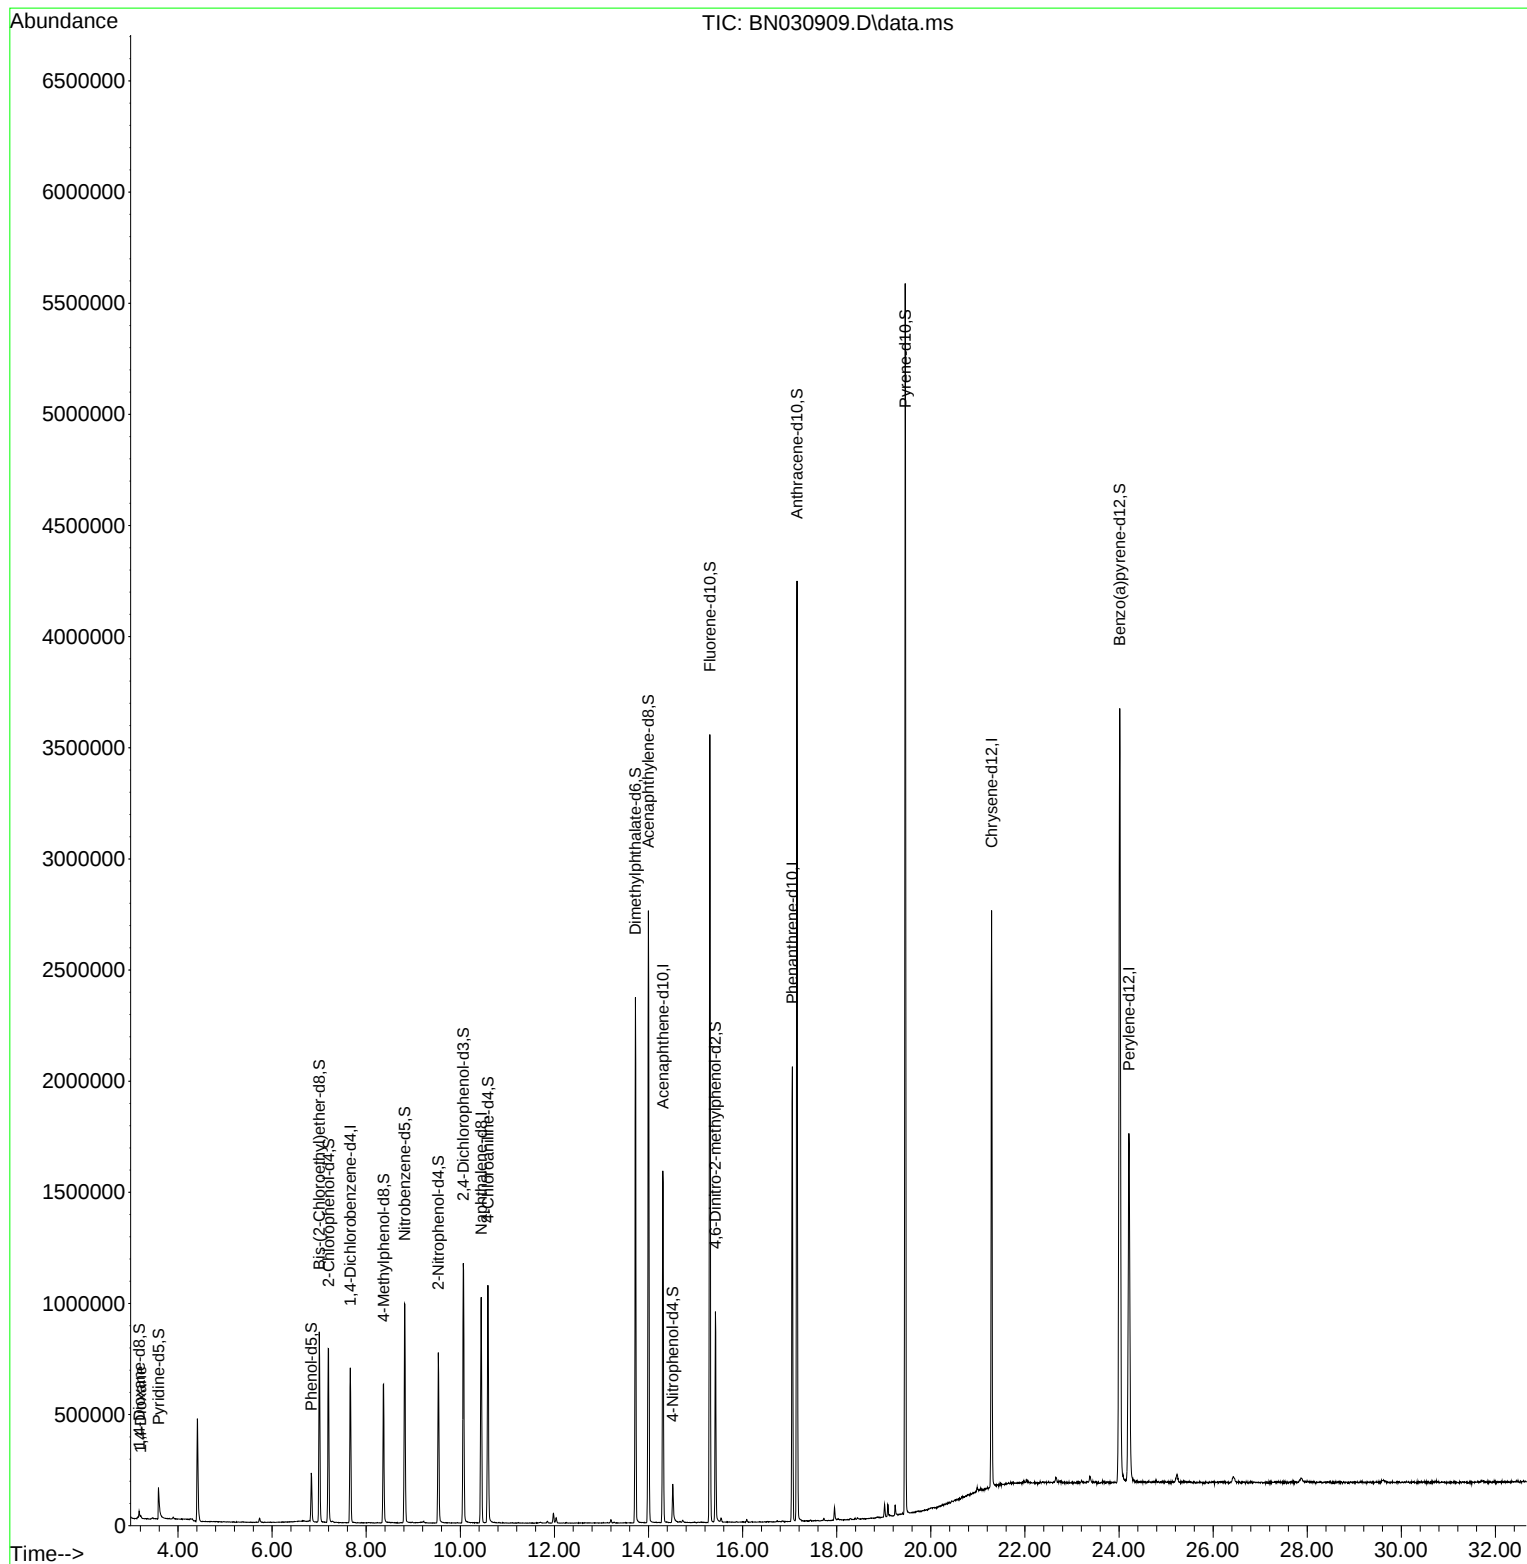

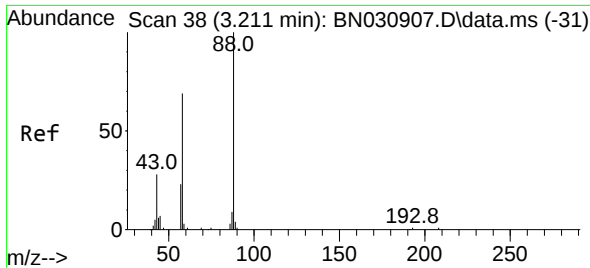

#2
 1,4-Dioxane
 Concen: 1.600 ng/uL
 RT: 3.211 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN030909.D
 Acq: 14 Apr 2024 11:04

Instrument :
 BNA_N
 ClientSampleId :
 YCSY1

Tgt Ion: 88 Resp: 6913
 Ion Ratio Lower Upper
 88 100
 43 41.8 23.8 35.8#
 58 63.5 56.6 84.8

