

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030879.D
 Acq On : 13 Apr 2024 14:09
 Operator : MA/JU
 Sample : PB160193BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK193

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030879.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	40	rBV	42614	63730	1.08%	0.121%
2	3.581	98	101	124	rBV	582807	1004771	17.08%	1.901%
3	3.899	152	155	161	rVB3	8463	12383	0.21%	0.023%
4	4.352	228	232	241	rVB4	5441	9237	0.16%	0.017%
5	6.834	645	654	667	rBV	758511	1212946	20.61%	2.295%
6	7.005	677	683	698	rVB	628619	1006031	17.10%	1.903%
7	7.199	709	716	729	rBV	774444	1200847	20.41%	2.272%
8	7.663	788	795	806	rBV	631051	1007677	17.13%	1.906%
9	8.369	908	915	929	rBV	963795	1526671	25.95%	2.888%
10	8.822	984	992	1006	rBV	740905	1191028	20.24%	2.253%
11	9.534	1106	1113	1130	rBV	562748	926564	15.75%	1.753%
12	10.069	1196	1204	1216	rBV	945560	1546010	26.28%	2.925%
13	10.446	1259	1268	1277	rBV	902870	1522356	25.87%	2.880%
14	10.587	1283	1292	1305	rBV	1061186	1811048	30.78%	3.426%
15	12.045	1532	1540	1544	rBV2	16693	27744	0.47%	0.052%
16	13.204	1731	1737	1742	rBV4	13855	20471	0.35%	0.039%
17	13.728	1819	1826	1837	rBV	1751793	2419528	41.12%	4.577%
18	14.004	1864	1873	1885	rBV	2025596	2963780	50.37%	5.607%
19	14.310	1918	1925	1932	rBV	1473128	2149084	36.52%	4.066%
20	14.516	1954	1960	1982	rBV	847064	1299645	22.09%	2.459%
21	15.304	2087	2094	2104	rBV	2576497	3743354	63.62%	7.082%
22	15.428	2109	2115	2125	rBV	651737	887466	15.08%	1.679%
23	15.545	2132	2135	2139	rVB3	12177	17255	0.29%	0.033%
24	16.092	2224	2228	2232	rBV5	8397	12361	0.21%	0.023%
25	16.539	2300	2304	2310	rVB8	4028	7678	0.13%	0.015%
26	16.845	2353	2356	2361	rVB5	5366	7956	0.14%	0.015%
27	17.057	2386	2392	2402	rBV	1948050	2701219	45.91%	5.110%
28	17.157	2402	2409	2425	rBV	3112286	4274563	72.65%	8.087%
29	17.957	2541	2545	2550	rBV5	27922	43733	0.74%	0.083%
30	19.022	2722	2726	2733	rVB2	38471	50459	0.86%	0.095%
31	19.092	2734	2738	2744	rBV	32059	44715	0.76%	0.085%
32	19.245	2761	2764	2769	rBV5	25512	41369	0.70%	0.078%
33	19.463	2794	2801	2808	rBV	3808762	5315304	90.34%	10.056%
34	21.298	3107	3113	3121	rBV	2330615	3360070	57.11%	6.357%
35	24.021	3566	3576	3592	rBV2	2461828	5883928	100.00%	11.131%
36	24.221	3601	3610	3626	rVB	1440631	3545930	60.26%	6.708%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030879.D
Acq On : 13 Apr 2024 14:09
Operator : MA/JU
Sample : PB160193BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK193

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 52858911

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030879.D
Acq On : 13 Apr 2024 14:09
Operator : MA/JU
Sample : PB160193BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

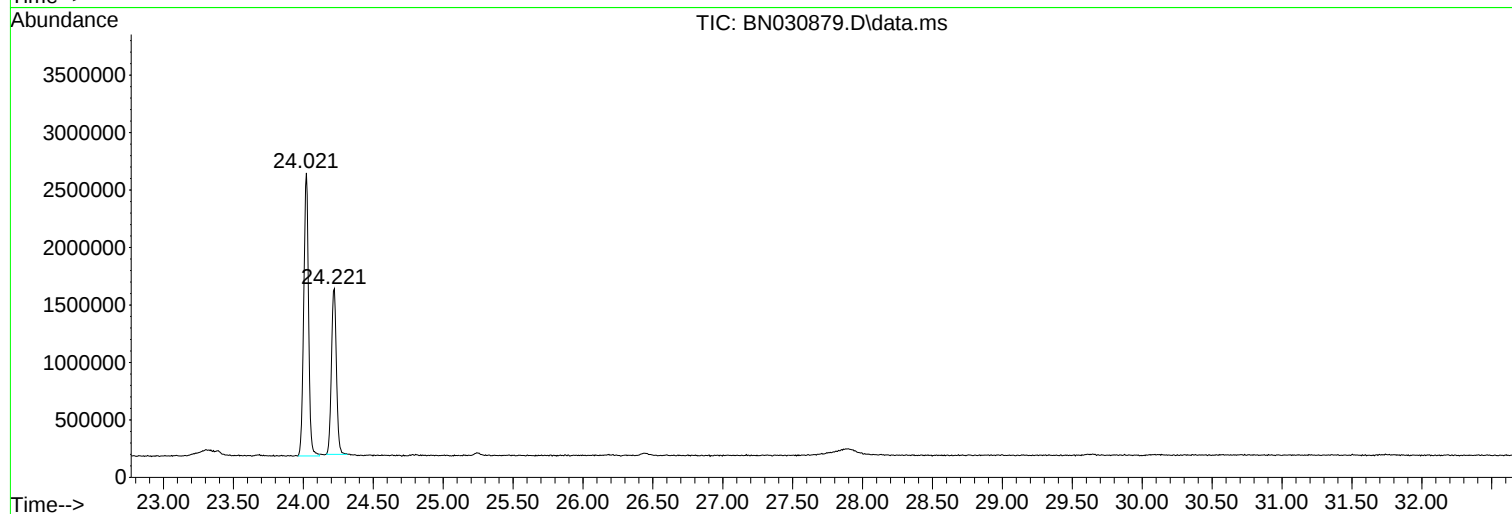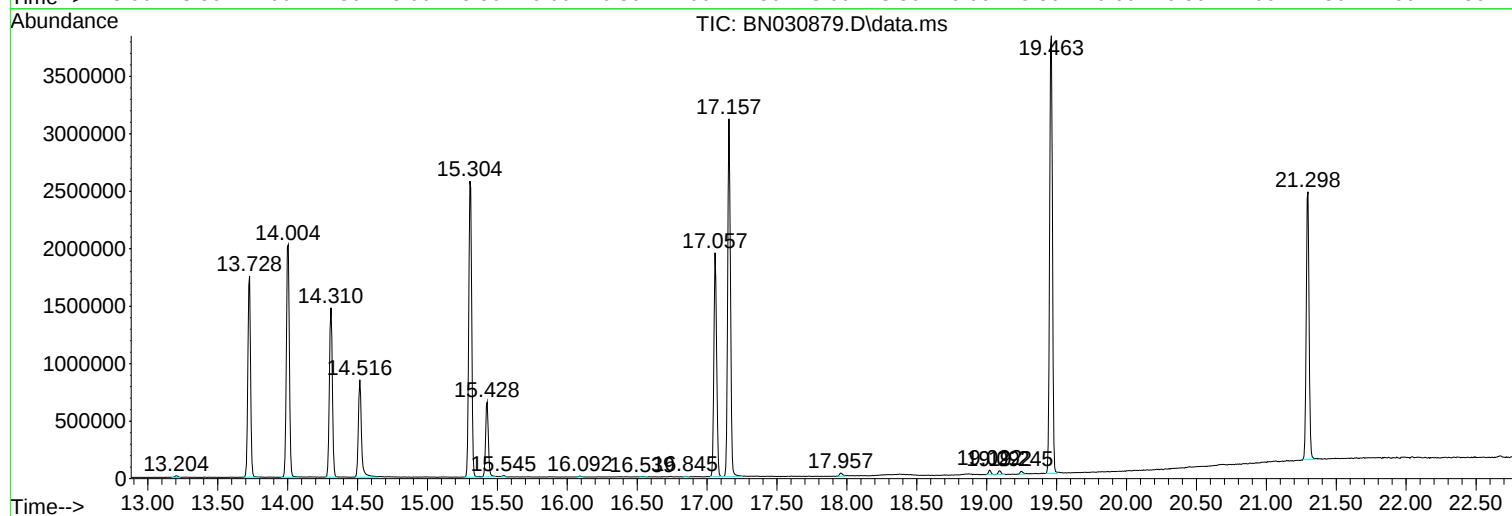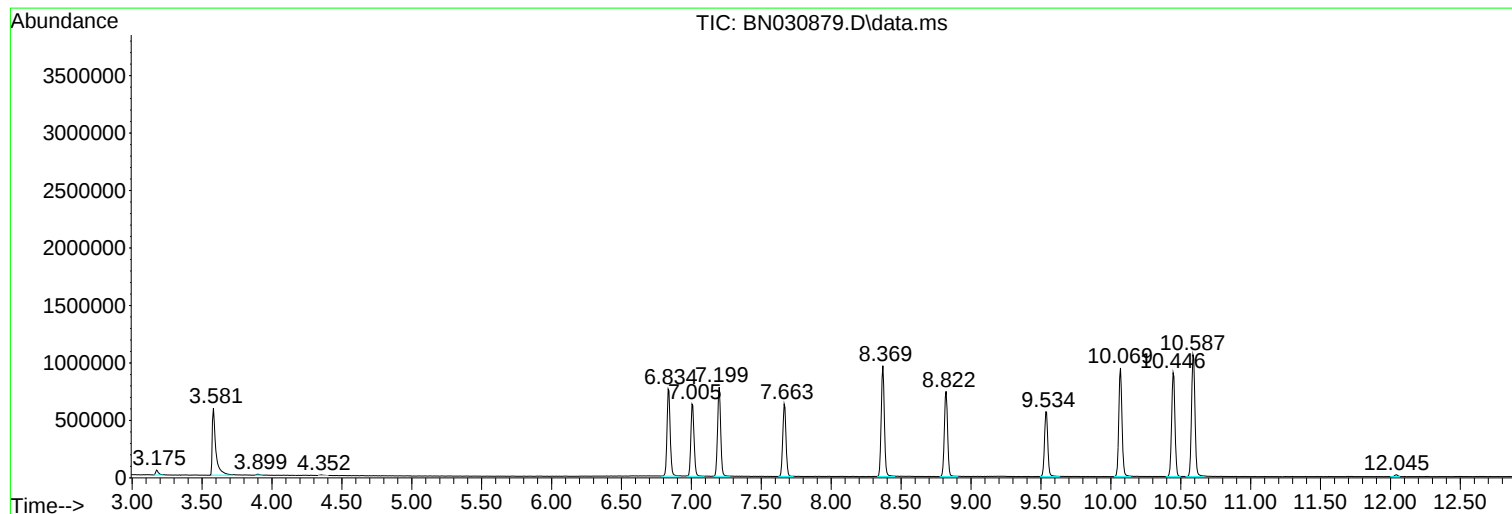

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030879.D
Acq On : 13 Apr 2024 14:09
Operator : MA/JU
Sample : PB160193BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030879.D
Acq On : 13 Apr 2024 14:09
Operator : MA/JU
Sample : PB160193BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK193

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc