

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030880.D
 Acq On : 13 Apr 2024 14:48
 Operator : MA/JU
 Sample : P2050-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	40	rVB	22625	33740	0.53%	0.071%
2	3.593	100	103	114	rBV	46755	86396	1.35%	0.181%
3	3.899	152	155	165	rVB2	8919	15178	0.24%	0.032%
4	6.840	649	655	663	rVB	131799	214997	3.37%	0.450%
5	7.005	676	683	692	rBV	618405	966700	15.16%	2.025%
6	7.199	709	716	726	rBV	563424	875495	13.73%	1.834%
7	7.399	746	750	756	rVB6	5397	8499	0.13%	0.018%
8	7.663	788	795	806	rBV	580526	930385	14.59%	1.949%
9	8.369	908	915	924	rBV	428134	675072	10.58%	1.414%
10	8.822	985	992	1002	rBV	705197	1156529	18.13%	2.423%
11	9.228	1054	1061	1066	rVB5	4348	9474	0.15%	0.020%
12	9.393	1085	1089	1094	rVB7	5303	8639	0.14%	0.018%
13	9.534	1106	1113	1123	rBV	519897	841906	13.20%	1.764%
14	10.069	1196	1204	1220	rBV	816636	1357821	21.29%	2.844%
15	10.446	1261	1268	1278	rBV	839272	1412136	22.14%	2.958%
16	10.587	1285	1292	1311	rVB	510981	867527	13.60%	1.817%
17	11.163	1385	1390	1393	rBV2	12688	22076	0.35%	0.046%
18	11.193	1393	1395	1401	rVB3	9546	13571	0.21%	0.028%
19	11.981	1523	1529	1535	rBV	19112	34313	0.54%	0.072%
20	12.040	1535	1539	1545	rVB	16762	25345	0.40%	0.053%
21	13.204	1731	1737	1742	rVB2	14149	23002	0.36%	0.048%
22	13.722	1819	1825	1836	rBV	1668469	2353412	36.90%	4.930%
23	13.998	1860	1872	1880	rBV	1975431	2924082	45.85%	6.125%
24	14.151	1893	1898	1905	rBV6	9702	15569	0.24%	0.033%
25	14.310	1918	1925	1933	rBV	1345006	1947688	30.54%	4.080%
26	14.428	1940	1945	1953	rVB6	10925	18218	0.29%	0.038%
27	14.522	1953	1961	1976	rBV2	115433	246429	3.86%	0.516%
28	14.734	1992	1997	2003	rVB9	4515	8888	0.14%	0.019%
29	15.057	2048	2052	2058	rBV	14684	21045	0.33%	0.044%
30	15.304	2087	2094	2105	rBV	2555132	3706022	58.11%	7.763%
31	15.422	2109	2114	2127	rVV	643662	907996	14.24%	1.902%
32	15.540	2130	2134	2141	rVB4	12061	22591	0.35%	0.047%
33	16.092	2222	2228	2232	rVB4	8656	12004	0.19%	0.025%
34	16.739	2334	2338	2343	rBV7	4989	6971	0.11%	0.015%
35	16.845	2349	2356	2358	rBV4	4203	7528	0.12%	0.016%
36	16.986	2375	2380	2385	rBV6	8168	11169	0.18%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030880.D
Acq On : 13 Apr 2024 14:48
Operator : MA/JU
Sample : P2050-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.057	2386	2392	2402	rVV	1769913	2463335	38.62%	5.160%
38	17.157	2402	2409	2428	rVV	3189120	4453932	69.84%	9.330%
39	17.733	2502	2507	2511	rVB6	11645	18748	0.29%	0.039%
40	17.834	2519	2524	2528	rBV6	4395	7178	0.11%	0.015%
41	17.957	2540	2545	2551	rBV	89262	129498	2.03%	0.271%
42	18.392	2615	2619	2623	rBV6	8790	13921	0.22%	0.029%
43	18.828	2690	2693	2698	rBV6	6677	12227	0.19%	0.026%
44	19.022	2722	2726	2732	rVB2	41509	55475	0.87%	0.116%
45	19.092	2734	2738	2742	rBV	37275	49544	0.78%	0.104%
46	19.245	2760	2764	2775	rBV3	66922	111574	1.75%	0.234%
47	19.457	2794	2800	2809	rBV	4041815	5601254	87.82%	11.733%
48	21.292	3107	3112	3124	rBV	2215051	3172572	49.74%	6.646%
49	24.021	3566	3576	3592	rBV2	2661644	6377762	100.00%	13.360%
50	24.216	3600	3609	3623	rBV	1392713	3483213	54.61%	7.296%




Sum of corrected areas: 47738646

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030880.D
Acq On : 13 Apr 2024 14:48
Operator : MA/JU
Sample : P2050-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R57

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

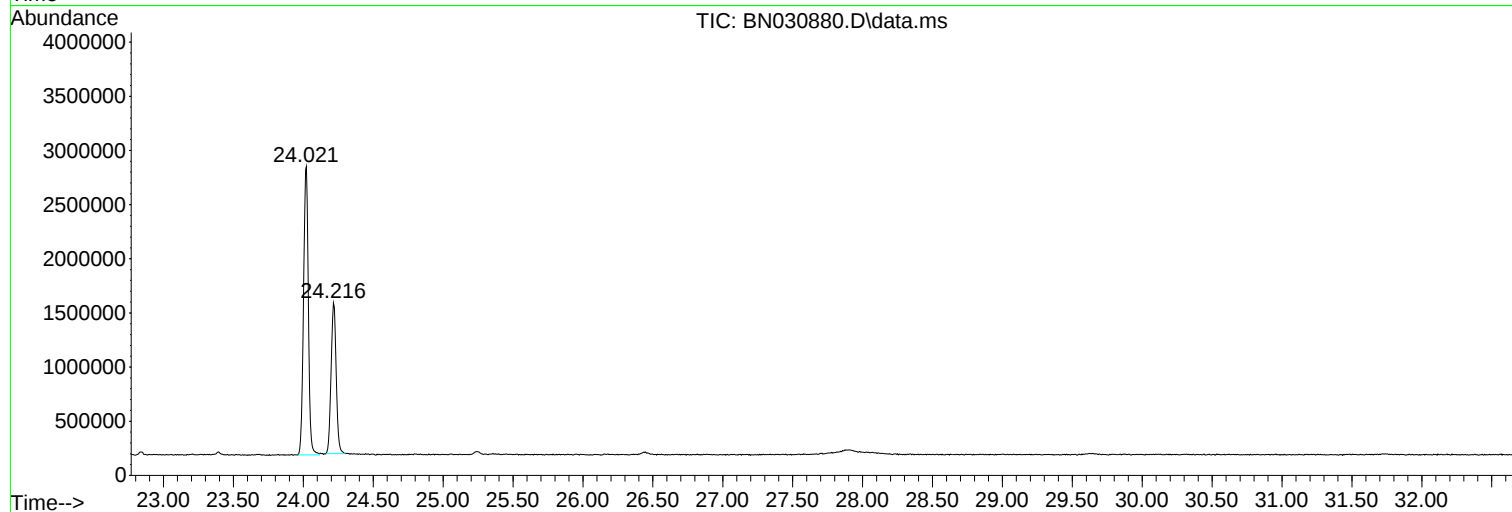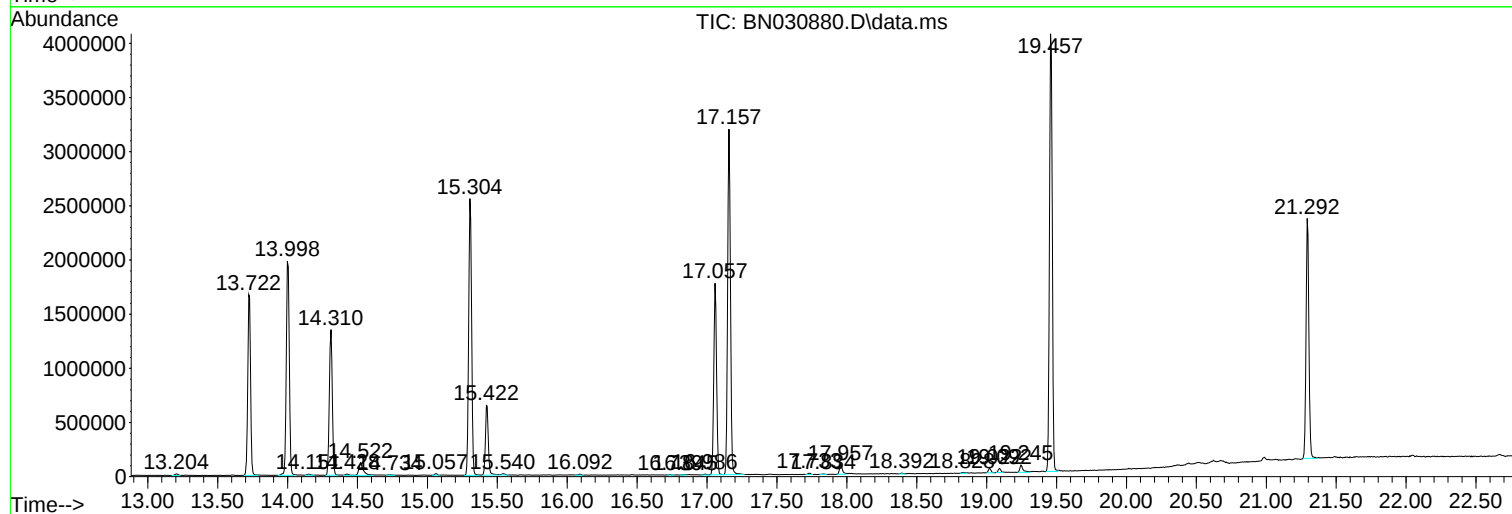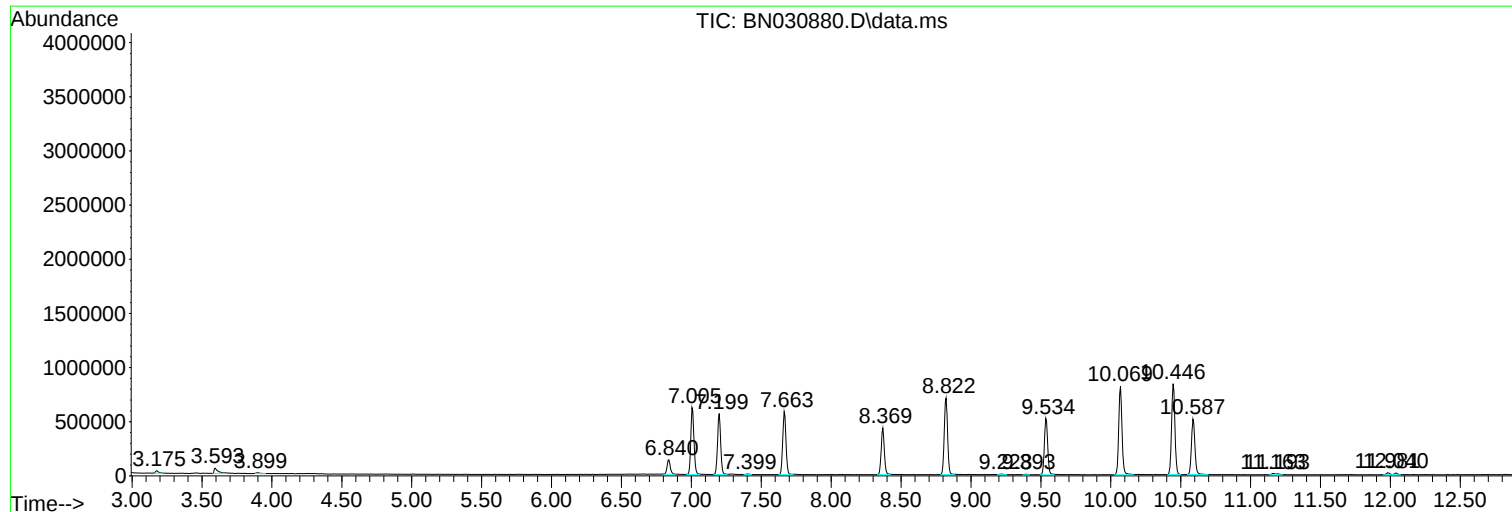

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030880.D
Acq On : 13 Apr 2024 14:48
Operator : MA/JU
Sample : P2050-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R57

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030880.D
Acq On : 13 Apr 2024 14:48
Operator : MA/JU
Sample : P2050-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R57

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc