

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030881.D
 Acq On : 13 Apr 2024 15:27
 Operator : MA/JU
 Sample : P2050-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	29	32	40	rVB2	20118	30097	0.50%	0.071%
2	3.452	75	79	85	rBV	6975	13876	0.23%	0.033%
3	3.593	100	103	118	rBV	57191	113694	1.90%	0.267%
4	3.899	152	155	161	rVB4	5171	8195	0.14%	0.019%
5	4.981	333	339	348	rVB	33229	55612	0.93%	0.130%
6	6.840	643	655	667	rVB	109050	192813	3.23%	0.452%
7	7.005	677	683	692	rBV	544678	854323	14.30%	2.003%
8	7.199	709	716	726	rBV	479606	747401	12.51%	1.752%
9	7.287	728	731	739	rVB8	5813	9506	0.16%	0.022%
10	7.664	789	795	805	rBV	446421	707889	11.85%	1.659%
11	8.369	908	915	927	rBV	360291	571465	9.57%	1.340%
12	8.822	983	992	1005	rBV	638004	1051402	17.60%	2.465%
13	9.222	1054	1060	1065	rVB4	7465	14421	0.24%	0.034%
14	9.387	1084	1088	1093	rBV6	4893	8077	0.14%	0.019%
15	9.534	1104	1113	1120	rBV	453799	743119	12.44%	1.742%
16	9.587	1120	1122	1131	rVB7	9247	15162	0.25%	0.036%
17	10.069	1195	1204	1218	rBV	712178	1189247	19.91%	2.788%
18	10.322	1244	1247	1253	rVB5	4801	8475	0.14%	0.020%
19	10.446	1260	1268	1277	rVB	667219	1083397	18.13%	2.540%
20	10.587	1286	1292	1309	rBV	517297	901686	15.09%	2.114%
21	11.199	1390	1396	1400	rBV3	11023	20820	0.35%	0.049%
22	12.040	1532	1539	1544	rBV	13971	25796	0.43%	0.060%
23	12.087	1544	1547	1550	rVV5	5692	8235	0.14%	0.019%
24	12.128	1550	1554	1559	rVB3	13092	22431	0.38%	0.053%
25	13.122	1717	1723	1728	rVB6	6281	11426	0.19%	0.027%
26	13.204	1733	1737	1744	rVB5	13314	20505	0.34%	0.048%
27	13.728	1818	1826	1832	rBV	1519383	2147939	35.95%	5.035%
28	13.999	1861	1872	1889	rBV	1776647	2663773	44.59%	6.245%
29	14.310	1918	1925	1935	rBV	1052765	1528084	25.58%	3.582%
30	14.516	1955	1960	1972	rBV2	112905	242199	4.05%	0.568%
31	14.675	1983	1987	1992	rVB5	8298	13082	0.22%	0.031%
32	14.734	1992	1997	2002	rVB8	5744	9659	0.16%	0.023%
33	14.869	2015	2020	2028	rVB2	8713	17792	0.30%	0.042%
34	15.304	2087	2094	2104	rBV	2475855	3461524	57.94%	8.115%
35	15.422	2108	2114	2127	rVV	544520	774856	12.97%	1.816%
36	15.546	2131	2135	2139	rVB3	11336	15977	0.27%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030881.D
 Acq On : 13 Apr 2024 15:27
 Operator : MA/JU
 Sample : P2050-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	16.093	2224	2228	2233	rVB5	8144	10754	0.18%	0.025%
38	16.469	2289	2292	2297	rVB7	6521	8629	0.14%	0.020%
39	16.534	2299	2303	2306	rBV4	5989	8993	0.15%	0.021%
40	16.651	2320	2323	2331	rVB7	5392	7595	0.13%	0.018%
41	16.987	2377	2380	2384	rVB4	11965	13478	0.23%	0.032%
42	17.057	2386	2392	2399	rBV	1435014	1958437	32.78%	4.591%
43	17.157	2402	2409	2421	rBV2	3035777	4161737	69.66%	9.756%
44	17.445	2455	2458	2462	rBV5	5381	7811	0.13%	0.018%
45	17.740	2504	2508	2514	rVB4	15483	24073	0.40%	0.056%
46	17.828	2520	2523	2532	rVB10	5085	10388	0.17%	0.024%
47	17.957	2540	2545	2553	rBV2	114525	164494	2.75%	0.386%
48	18.045	2556	2560	2567	rVB2	23684	37102	0.62%	0.087%
49	18.392	2617	2619	2624	rVB4	9369	10761	0.18%	0.025%
50	18.445	2624	2628	2632	rBV6	8656	15129	0.25%	0.035%
51	18.828	2690	2693	2698	rBV6	8035	12547	0.21%	0.029%
52	19.022	2722	2726	2732	rVB3	41338	55658	0.93%	0.130%
53	19.092	2734	2738	2742	rBV2	37861	53948	0.90%	0.126%
54	19.245	2760	2764	2773	rBV2	79009	125917	2.11%	0.295%
55	19.457	2794	2800	2807	rBV	3774327	5320359	89.05%	12.472%
56	21.292	3107	3112	3120	rBV2	1754257	2547570	42.64%	5.972%
57	24.016	3567	3575	3589	rVB2	2522404	5974335	100.00%	14.005%
58	24.216	3601	3609	3626	rVB2	1173743	2824162	47.27%	6.621%




Sum of corrected areas: 42657832

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030881.D
Acq On : 13 Apr 2024 15:27
Operator : MA/JU
Sample : P2050-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CORA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

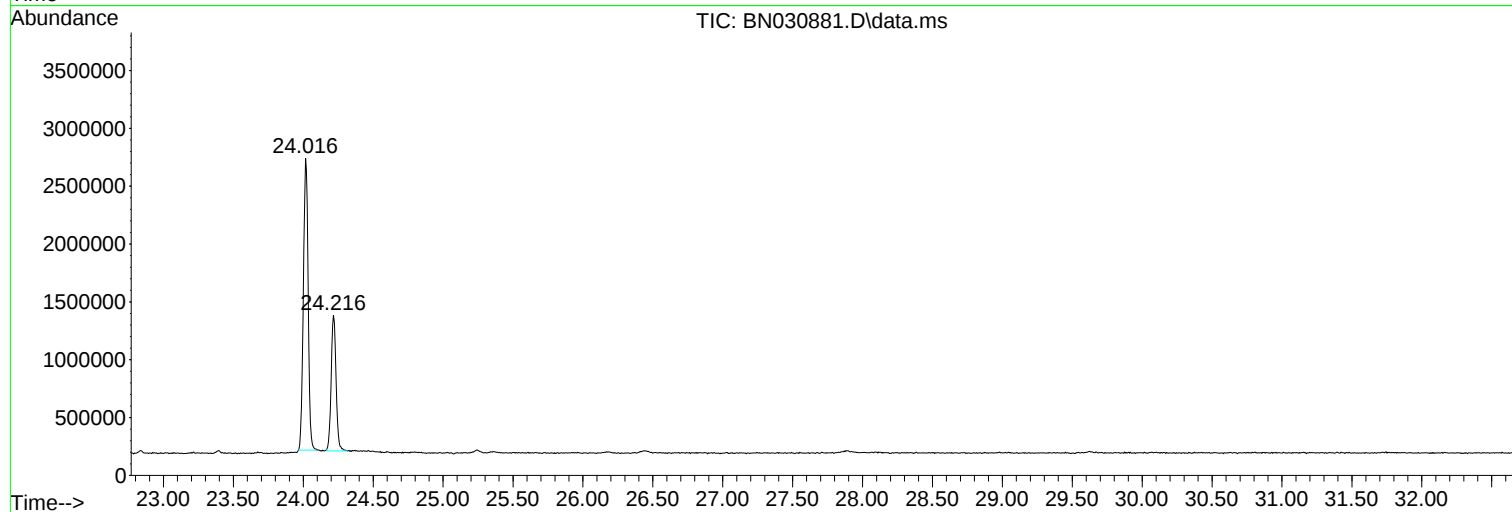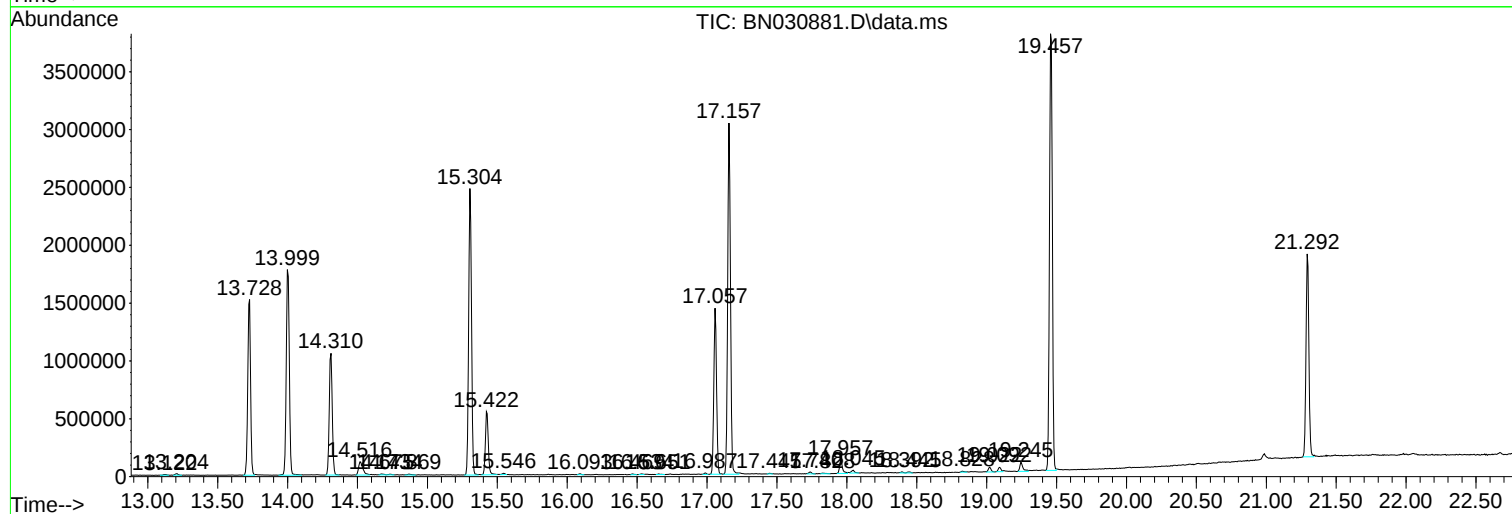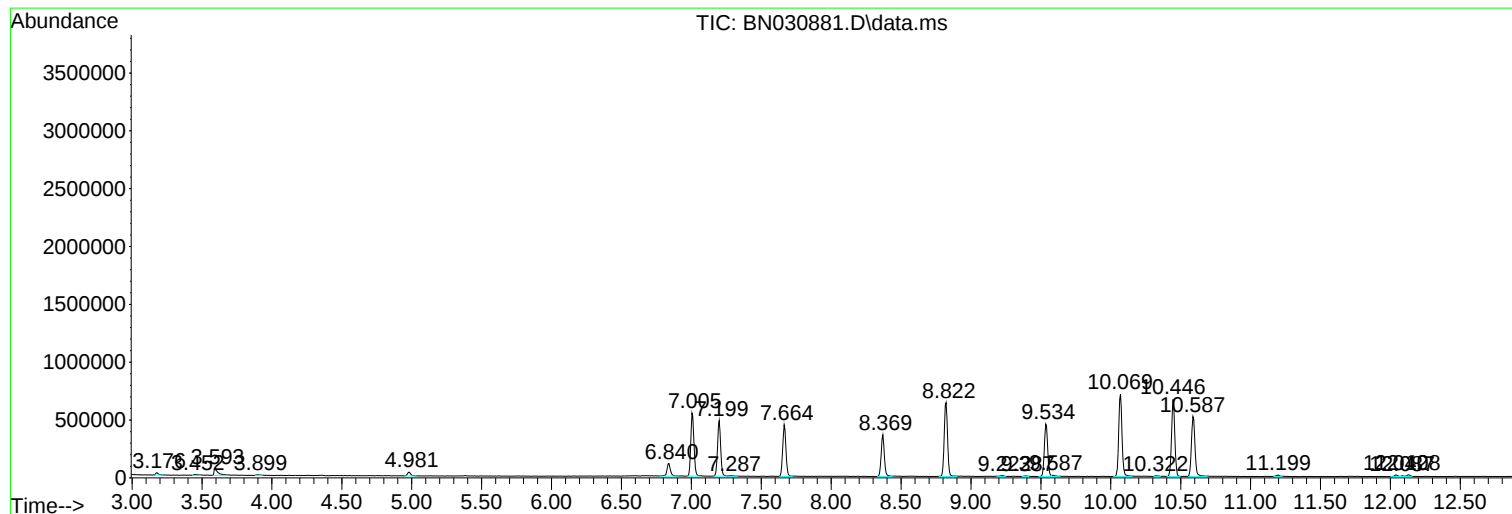

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030881.D
Acq On : 13 Apr 2024 15:27
Operator : MA/JU
Sample : P2050-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030881.D
Acq On : 13 Apr 2024 15:27
Operator : MA/JU
Sample : P2050-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc