

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030886.D
 Acq On : 13 Apr 2024 18:44
 Operator : MA/JU
 Sample : P2050-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	28	32	37	rBV	25100	37500	0.54%	0.074%
2	3.587	100	102	118	rBV	126617	229341	3.31%	0.454%
3	3.899	151	155	159	rBV2	9589	12393	0.18%	0.025%
4	6.840	649	655	664	rVB	125741	209244	3.02%	0.414%
5	7.005	676	683	692	rBV	596247	928383	13.39%	1.837%
6	7.199	709	716	726	rBV	546471	847062	12.22%	1.676%
7	7.664	787	795	805	rBV	630515	998480	14.40%	1.976%
8	8.369	908	915	925	rBV	426682	663755	9.58%	1.313%
9	8.822	984	992	1003	rBV	675708	1124743	16.23%	2.226%
10	9.222	1056	1060	1065	rVB	9316	13139	0.19%	0.026%
11	9.387	1084	1088	1093	rBV6	4308	7531	0.11%	0.015%
12	9.534	1104	1113	1126	rBV	515237	833208	12.02%	1.649%
13	9.952	1178	1184	1188	rBV6	3396	7443	0.11%	0.015%
14	10.069	1197	1204	1219	rBV	788804	1327187	19.15%	2.626%
15	10.446	1261	1268	1276	rBV	918147	1514110	21.84%	2.996%
16	10.587	1285	1292	1308	rBV	815938	1367338	19.73%	2.706%
17	11.199	1391	1396	1401	rBV7	4455	8459	0.12%	0.017%
18	11.705	1474	1482	1487	rVB10	4131	8362	0.12%	0.017%
19	12.040	1528	1539	1544	rBV2	15342	27697	0.40%	0.055%
20	13.204	1732	1737	1745	rBV3	14698	22788	0.33%	0.045%
21	13.722	1819	1825	1836	rBV	1685679	2331880	33.64%	4.614%
22	13.999	1865	1872	1884	rBV	1968448	2847910	41.08%	5.636%
23	14.310	1918	1925	1932	rBV	1422712	2118075	30.56%	4.191%
24	14.516	1954	1960	1978	rBV2	106723	216449	3.12%	0.428%
25	15.304	2086	2094	2105	rBV	2626490	3738606	53.93%	7.398%
26	15.422	2108	2114	2126	rBV	690561	957651	13.82%	1.895%
27	15.546	2131	2135	2140	rVB4	13472	20860	0.30%	0.041%
28	16.087	2223	2227	2234	rVB6	10147	14436	0.21%	0.029%
29	16.463	2287	2291	2297	rBV7	5065	8695	0.13%	0.017%
30	16.987	2376	2380	2383	rVB5	11380	13075	0.19%	0.026%
31	17.057	2386	2392	2400	rBV	1967314	2704366	39.01%	5.351%
32	17.157	2402	2409	2420	rBV	3291095	4574112	65.99%	9.051%
33	17.440	2455	2457	2465	rVB6	5603	9107	0.13%	0.018%
34	17.828	2519	2523	2529	rBV9	7300	9223	0.13%	0.018%
35	17.957	2540	2545	2554	rBV	98896	144420	2.08%	0.286%
36	18.392	2616	2619	2624	rVB6	8128	10098	0.15%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030886.D
Acq On : 13 Apr 2024 18:44
Operator : MA/JU
Sample : P2050-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	18.828	2689	2693	2697	rBV4	13780	18457	0.27%	0.037%
38	19.022	2721	2726	2730	rBV2	42419	55739	0.80%	0.110%
39	19.092	2733	2738	2742	rBV	41331	58525	0.84%	0.116%
40	19.245	2760	2764	2770	rBV3	76399	106303	1.53%	0.210%
41	19.457	2794	2800	2807	rBV	4234796	5790048	83.53%	11.458%
42	20.986	3056	3060	3065	rBV4	63704	98940	1.43%	0.196%
43	21.292	3107	3112	3119	rBV	2555881	3558309	51.33%	7.041%
44	24.022	3566	3576	3591	rBV2	2916871	6931868	100.00%	13.717%
45	24.216	3600	3609	3622	rBV2	1565717	4009566	57.84%	7.934%




Sum of corrected areas: 50534881

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030886.D
Acq On : 13 Apr 2024 18:44
Operator : MA/JU
Sample : P2050-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

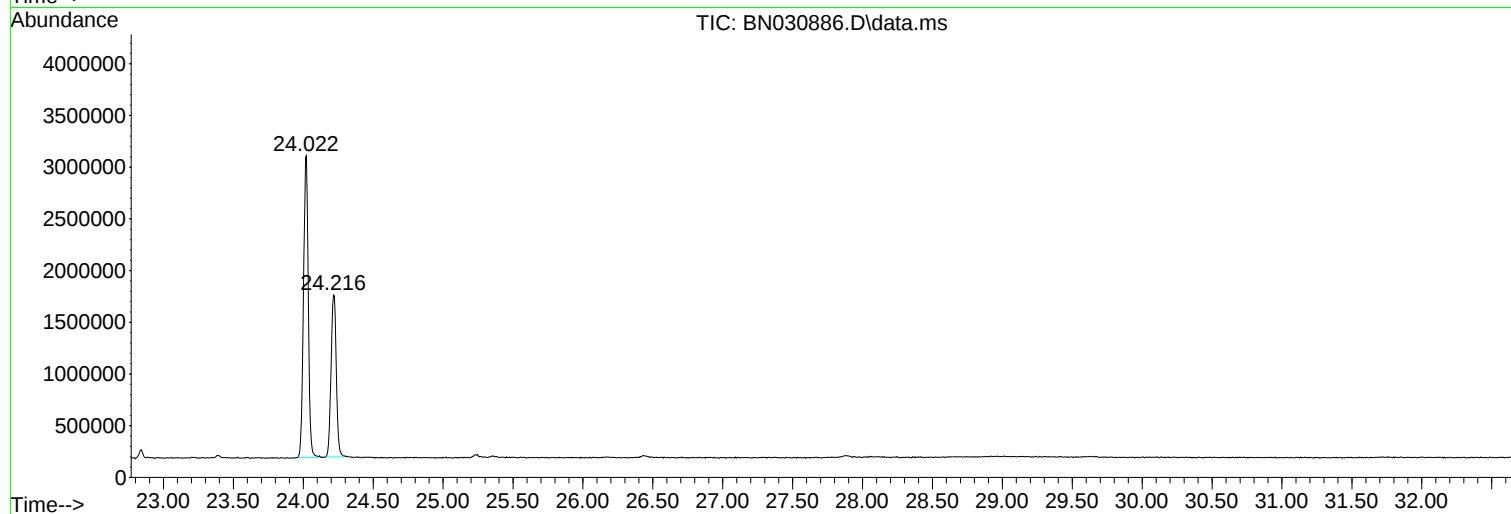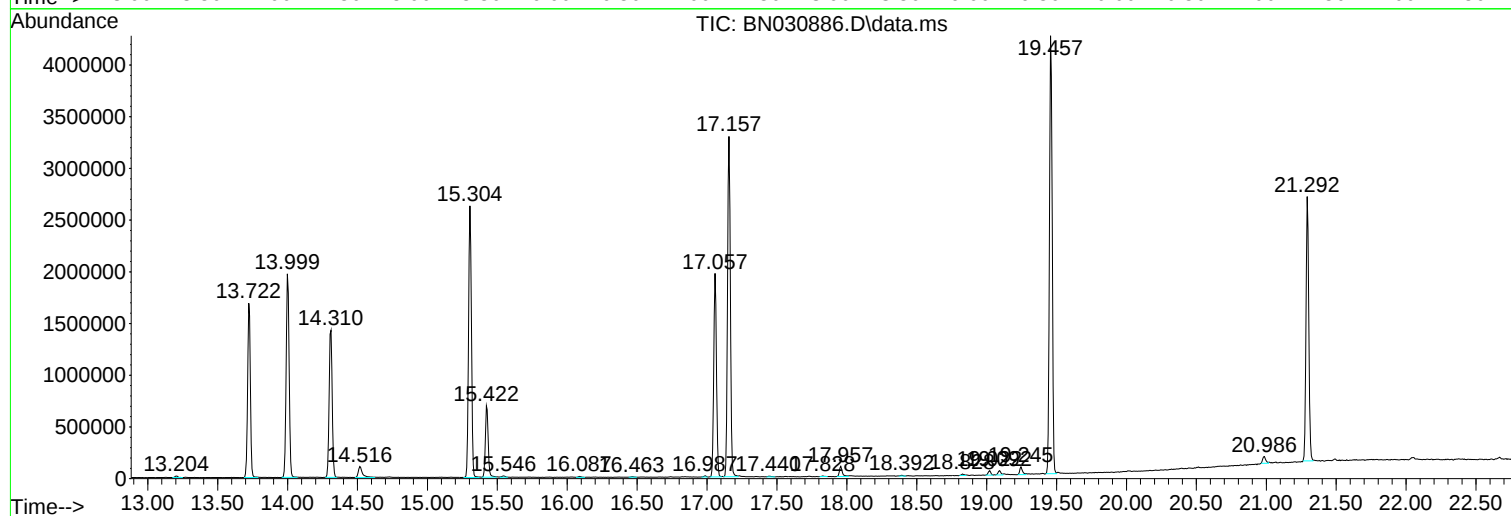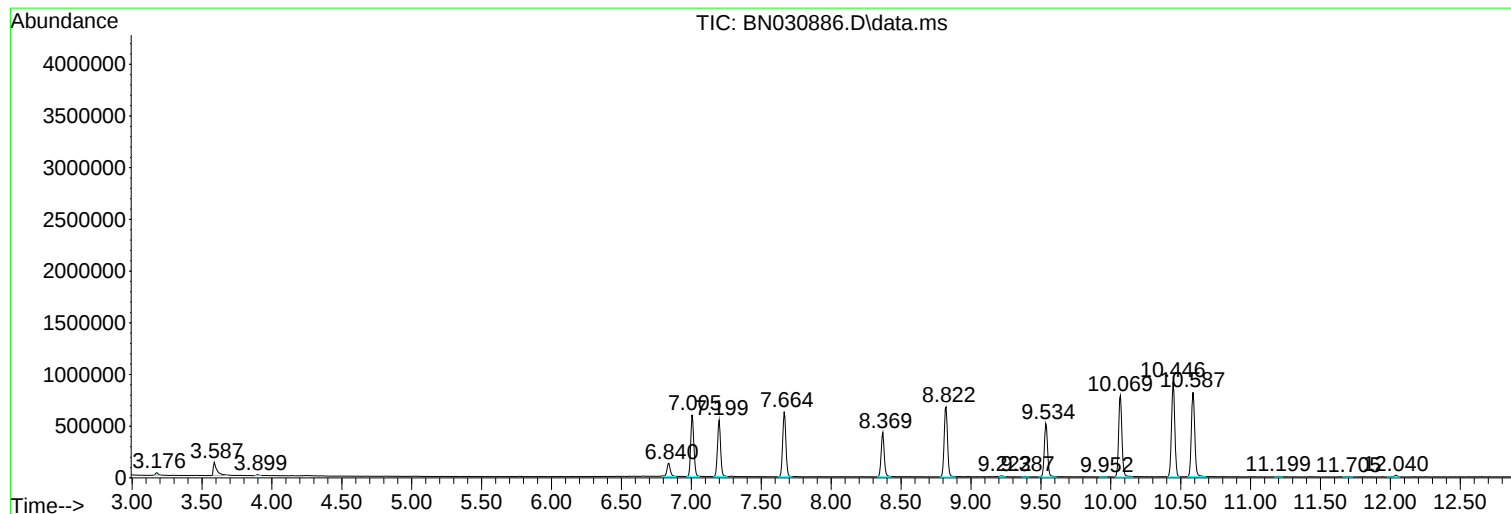

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030886.D
Acq On : 13 Apr 2024 18:44
Operator : MA/JU
Sample : P2050-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030886.D
Acq On : 13 Apr 2024 18:44
Operator : MA/JU
Sample : P2050-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc