

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030887.D
 Acq On : 13 Apr 2024 19:24
 Operator : MA/JU
 Sample : P2050-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CORB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	41	rVB	24563	39364	0.54%	0.073%
2	3.587	100	102	118	rBV	165222	297599	4.10%	0.551%
3	3.899	152	155	159	rVB2	7289	8873	0.12%	0.016%
4	5.011	339	344	353	rVB	13062	22793	0.31%	0.042%
5	6.799	643	648	649	rBV2	6354	8326	0.11%	0.015%
6	6.834	649	654	662	rVB	136366	220685	3.04%	0.408%
7	7.005	674	683	694	rBV	617177	979005	13.48%	1.812%
8	7.199	709	716	728	rBV	569776	902951	12.43%	1.671%
9	7.552	770	776	784	rVB	25751	44346	0.61%	0.082%
10	7.663	788	795	809	rVV	638138	1107260	15.24%	2.049%
11	7.752	809	810	816	rVB4	4973	7406	0.10%	0.014%
12	8.010	849	854	861	rBV	57070	90801	1.25%	0.168%
13	8.369	908	915	926	rBV	453649	724133	9.97%	1.340%
14	8.822	984	992	1004	rBV	726109	1194470	16.44%	2.211%
15	9.222	1053	1060	1064	rVB2	12313	18410	0.25%	0.034%
16	9.387	1084	1088	1095	rVB7	7796	13687	0.19%	0.025%
17	9.534	1106	1113	1126	rBV	535463	872482	12.01%	1.615%
18	10.069	1197	1204	1215	rBV	885023	1456881	20.05%	2.696%
19	10.310	1239	1245	1253	rBV	124386	202256	2.78%	0.374%
20	10.446	1260	1268	1276	rBV	922438	1514579	20.85%	2.803%
21	10.587	1284	1292	1314	rBV	827797	1448098	19.93%	2.680%
22	10.822	1327	1332	1337	rBV6	5939	10399	0.14%	0.019%
23	11.193	1390	1395	1401	rBV5	7576	13892	0.19%	0.026%
24	12.040	1533	1539	1547	rVV	16624	30150	0.42%	0.056%
25	13.210	1731	1738	1745	rBV3	16456	31070	0.43%	0.058%
26	13.722	1819	1825	1835	rBV	1910141	2650988	36.49%	4.906%
27	13.998	1863	1872	1884	rBV	2063050	3125213	43.02%	5.784%
28	14.310	1918	1925	1932	rBV	1452956	2121975	29.21%	3.927%
29	14.516	1955	1960	1971	rBV	128404	236896	3.26%	0.438%
30	14.675	1982	1987	1993	rBV8	6931	12646	0.17%	0.023%
31	14.734	1993	1997	2003	rVB9	6443	9098	0.13%	0.017%
32	15.304	2087	2094	2101	rBV	2934979	4167328	57.36%	7.713%
33	15.422	2109	2114	2129	rBV	764191	1065197	14.66%	1.971%
34	15.545	2131	2135	2139	rVB3	13418	19088	0.26%	0.035%
35	16.092	2224	2228	2232	rBV4	9965	14318	0.20%	0.026%
36	16.463	2288	2291	2297	rVB5	6970	8805	0.12%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030887.D
 Acq On : 13 Apr 2024 19:24
 Operator : MA/JU
 Sample : P2050-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	16.733	2333	2337	2342	rVB7	5114	8394	0.12%	0.016%
38	16.845	2348	2356	2358	rBV7	4317	11019	0.15%	0.020%
39	16.986	2376	2380	2384	rBV4	22003	26691	0.37%	0.049%
40	17.057	2386	2392	2402	rBV	1913115	2714282	37.36%	5.024%
41	17.157	2402	2409	2419	rBV2	3371698	4832477	66.52%	8.944%
42	17.451	2455	2459	2466	rBV8	7380	13562	0.19%	0.025%
43	17.728	2503	2506	2510	rVB5	13266	16358	0.23%	0.030%
44	17.828	2519	2523	2526	rBV5	8657	11681	0.16%	0.022%
45	17.957	2539	2545	2553	rBV	124573	186757	2.57%	0.346%
46	18.169	2576	2581	2590	rBV	61722	88720	1.22%	0.164%
47	18.286	2598	2601	2605	rBV3	10835	17337	0.24%	0.032%
48	18.392	2616	2619	2623	rVB5	13915	17579	0.24%	0.033%
49	18.445	2623	2628	2632	rBV7	11928	21240	0.29%	0.039%
50	18.628	2656	2659	2664	rBV7	6659	11398	0.16%	0.021%
51	18.828	2690	2693	2697	rBV5	17936	26523	0.37%	0.049%
52	19.022	2721	2726	2732	rBV2	51065	69489	0.96%	0.129%
53	19.092	2733	2738	2741	rBV	51961	74897	1.03%	0.139%
54	19.245	2760	2764	2773	rBV2	73972	108781	1.50%	0.201%
55	19.457	2794	2800	2815	rBV	4528892	6362880	87.59%	11.776%
56	20.986	3056	3060	3065	rBV3	72555	112596	1.55%	0.208%
57	21.292	3107	3112	3122	rVB	2446891	3496240	48.13%	6.471%
58	24.021	3566	3576	3591	rBV	3033239	7264608	100.00%	13.445%
59	24.215	3601	3609	3621	rVB	1575204	3845526	52.94%	7.117%




Sum of corrected areas: 54030503

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030887.D
Acq On : 13 Apr 2024 19:24
Operator : MA/JU
Sample : P2050-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

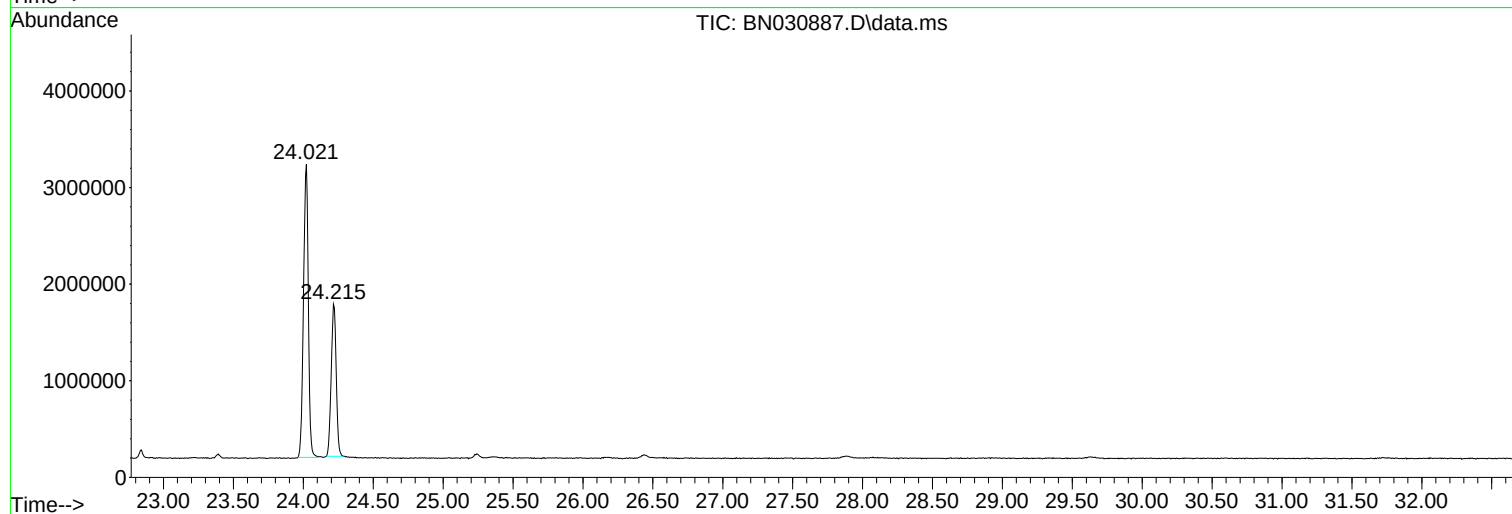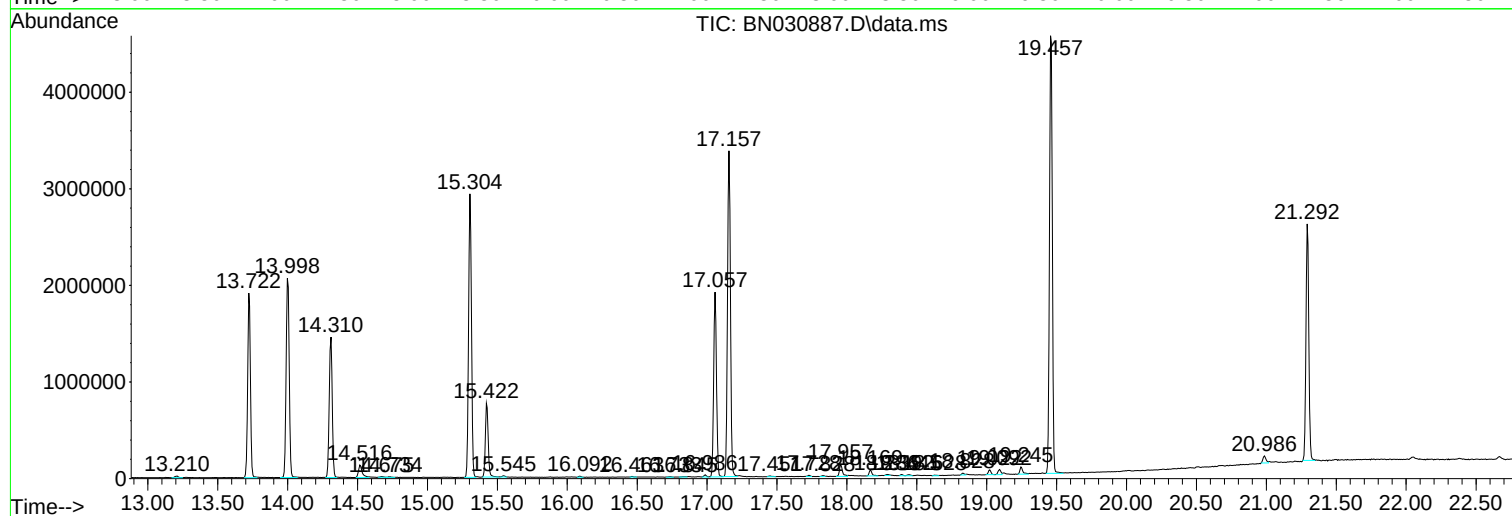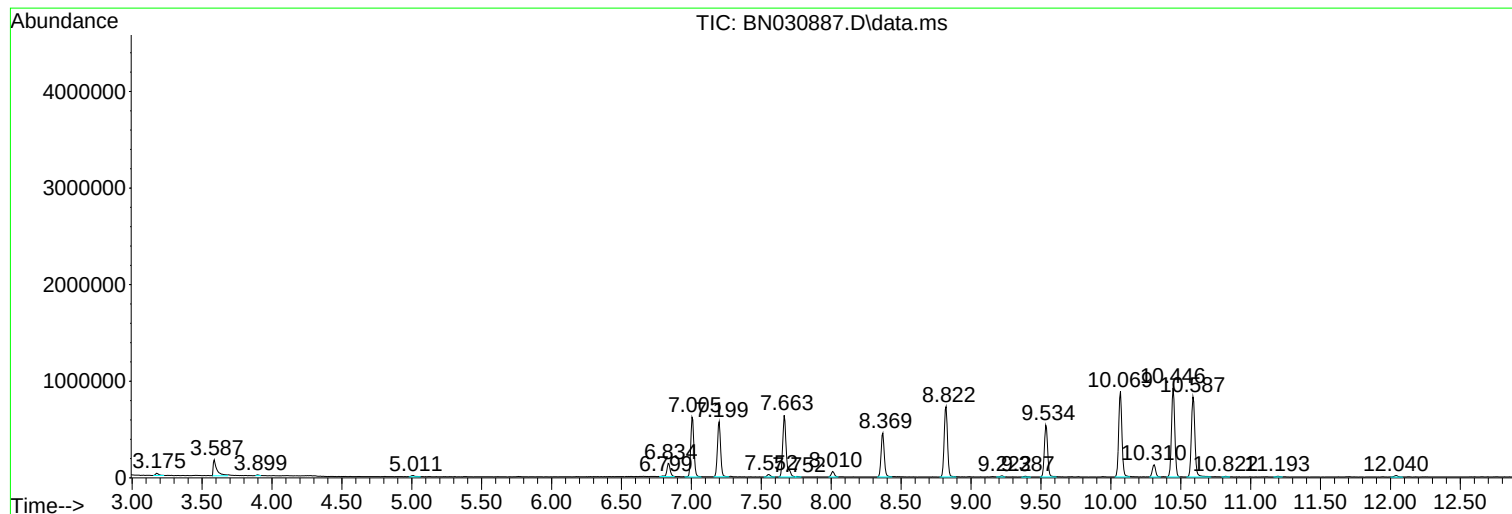

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030887.D
Acq On : 13 Apr 2024 19:24
Operator : MA/JU
Sample : P2050-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RB2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,3,5-trichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.310	2.67 ng/ul	202256	Naphthalene-d8	10.446

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
2			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
3			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
4			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	97
5			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	96

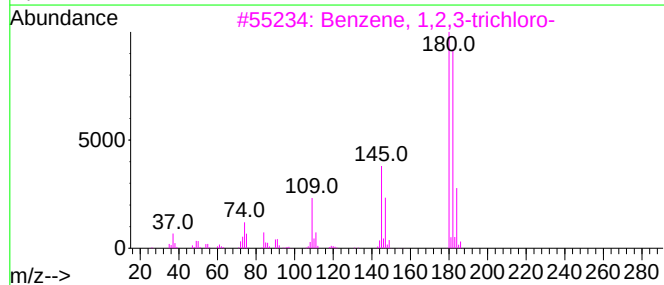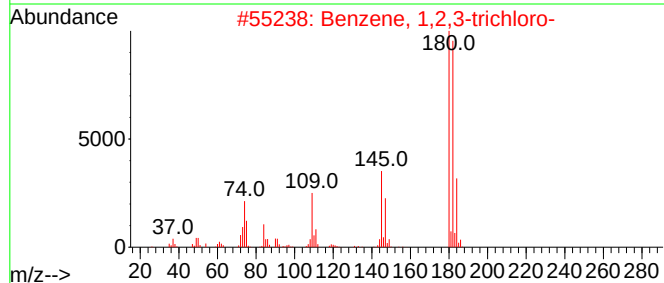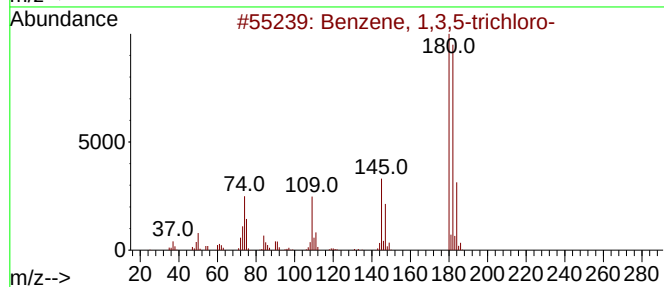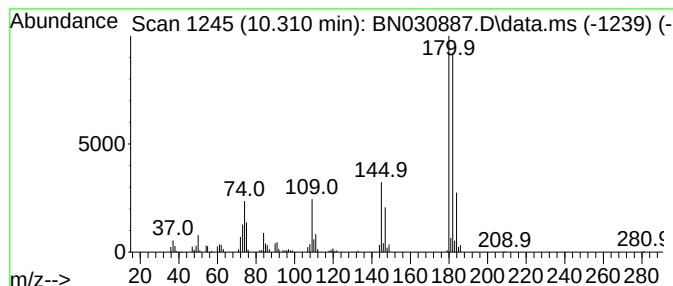

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030887.D
Acq On : 13 Apr 2024 19:24
Operator : MA/JU
Sample : P2050-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3,5-...	10.310	2.7	ng/u1	202256	2	10.446	1514580	20.0