

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030894.D
 Acq On : 14 Apr 2024 00:38
 Operator : MA/JU
 Sample : PB160206BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK206

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	42	rBV	42640	63361	1.07%	0.121%
2	3.581	98	101	122	rBV	603444	1077436	18.19%	2.060%
3	3.899	151	155	160	rVB2	8950	13478	0.23%	0.026%
4	4.352	228	232	238	rBV2	7031	13602	0.23%	0.026%
5	6.834	644	654	669	rVB	764157	1200194	20.26%	2.295%
6	7.005	677	683	693	rVB	617287	967671	16.33%	1.851%
7	7.199	709	716	728	rBV	749355	1193825	20.15%	2.283%
8	7.663	788	795	808	rVB	591156	925220	15.62%	1.769%
9	8.369	908	915	930	rBV	946951	1512878	25.54%	2.893%
10	8.822	983	992	1002	rBV	711720	1174833	19.83%	2.247%
11	9.534	1103	1113	1126	rBV	564367	910154	15.36%	1.741%
12	10.069	1196	1204	1216	rBV	924582	1542562	26.04%	2.950%
13	10.446	1260	1268	1276	rBV	844999	1399865	23.63%	2.677%
14	10.587	1285	1292	1310	rBV	1158462	1958185	33.06%	3.745%
15	12.040	1534	1539	1545	rVB	15795	25561	0.43%	0.049%
16	13.204	1731	1737	1741	rBV3	16685	26447	0.45%	0.051%
17	13.722	1819	1825	1837	rBV	1732670	2376850	40.12%	4.545%
18	13.998	1865	1872	1888	rBV	2039716	2972372	50.18%	5.684%
19	14.304	1916	1924	1934	rBV	1303826	1981289	33.45%	3.789%
20	14.516	1953	1960	1977	rBV	824706	1273212	21.49%	2.435%
21	15.304	2085	2094	2103	rBV	2740727	3740361	63.14%	7.153%
22	15.422	2108	2114	2130	rVV	640279	897117	15.14%	1.716%
23	15.539	2130	2134	2141	rVB4	12859	20691	0.35%	0.040%
24	16.087	2223	2227	2232	rVB5	7811	11947	0.20%	0.023%
25	17.057	2386	2392	2402	rBV	1815113	2545418	42.97%	4.868%
26	17.157	2402	2409	2421	rBV2	3014990	4222224	71.27%	8.074%
27	17.733	2504	2507	2512	rVB5	3851	6401	0.11%	0.012%
28	17.957	2541	2545	2550	rVB6	8563	13882	0.23%	0.027%
29	19.022	2721	2726	2731	rVB	37752	51222	0.86%	0.098%
30	19.092	2733	2738	2744	rBV	34429	50596	0.85%	0.097%
31	19.245	2761	2764	2768	rBV5	7249	11297	0.19%	0.022%
32	19.457	2794	2800	2808	rBV2	3895413	5378556	90.79%	10.286%
33	21.292	3106	3112	3121	rBV2	2290152	3274059	55.27%	6.261%
34	24.015	3566	3575	3587	rBV2	2538402	5923917	100.00%	11.329%
35	24.216	3600	3609	3622	rVB	1454440	3535065	59.67%	6.760%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030894.D
Acq On : 14 Apr 2024 00:38
Operator : MA/JU
Sample : PB160206BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK206

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 52291748

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030894.D
Acq On : 14 Apr 2024 00:38
Operator : MA/JU
Sample : PB160206BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

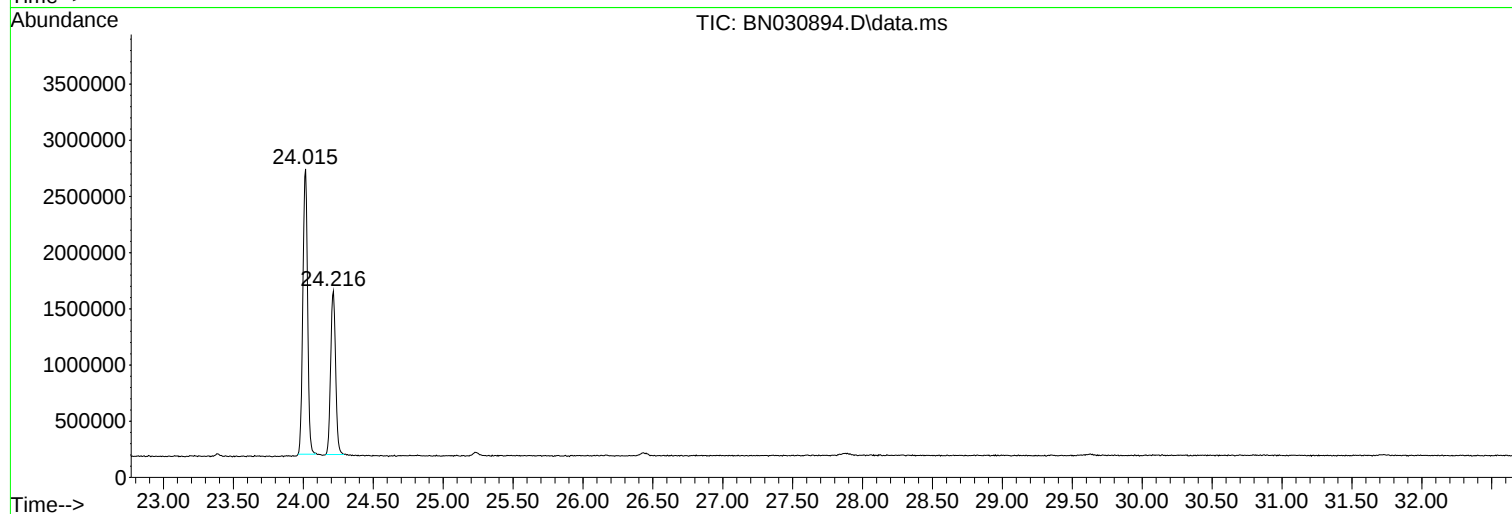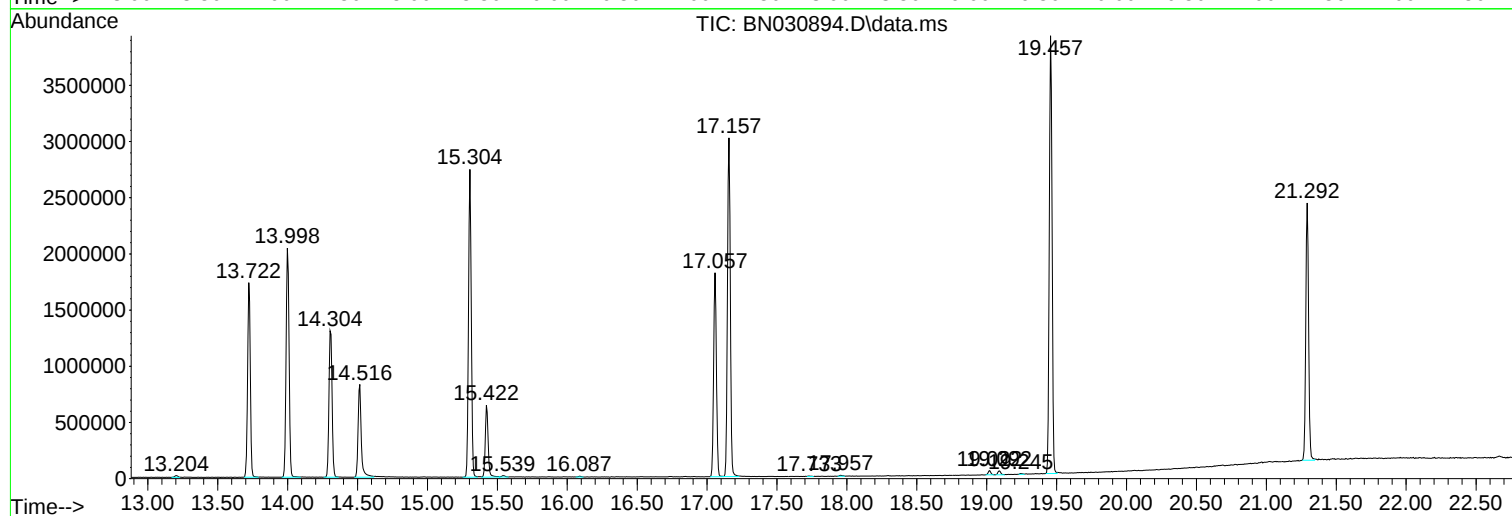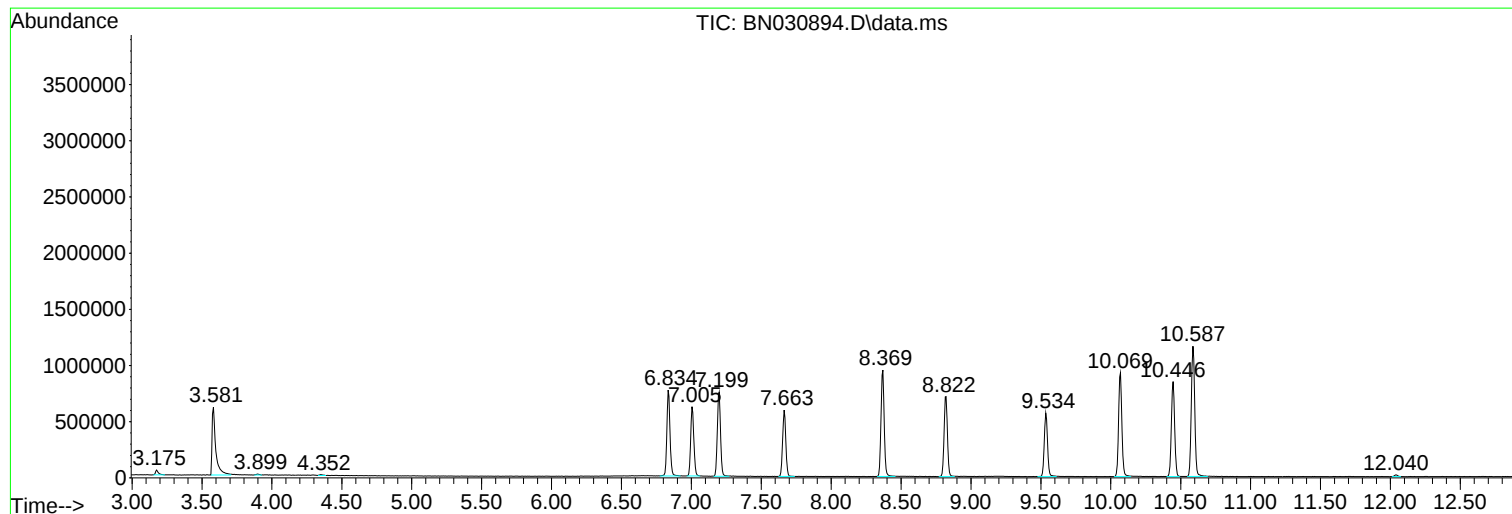

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030894.D
Acq On : 14 Apr 2024 00:38
Operator : MA/JU
Sample : PB160206BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030894.D
Acq On : 14 Apr 2024 00:38
Operator : MA/JU
Sample : PB160206BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK206

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------