

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030904.D
 Acq On : 14 Apr 2024 07:09
 Operator : MA/JU
 Sample : P2036-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	22	27	46	rBV2	278596	559272	7.49%	0.921%
2	3.587	99	102	115	rBV	227185	421983	5.65%	0.695%
3	3.899	151	155	161	rVB2	15313	22367	0.30%	0.037%
4	4.411	237	242	256	rVB	169899	284502	3.81%	0.469%
5	5.734	460	467	475	rBV	50636	79657	1.07%	0.131%
6	6.834	649	654	662	rVB	176084	275027	3.69%	0.453%
7	7.005	677	683	696	rVB	768730	1192207	15.97%	1.964%
8	7.199	708	716	725	rBV	697958	1118924	14.99%	1.843%
9	7.275	728	729	738	rVB8	5222	9723	0.13%	0.016%
10	7.663	788	795	804	rBV	783982	1213922	16.27%	1.999%
11	8.369	908	915	925	rBV	542647	884186	11.85%	1.456%
12	8.816	984	991	1002	rBV	885626	1456269	19.51%	2.398%
13	8.981	1013	1019	1023	rBV7	11119	16811	0.23%	0.028%
14	9.534	1105	1113	1125	rBV	661549	1072503	14.37%	1.766%
15	10.063	1196	1203	1219	rBV	1040973	1765778	23.66%	2.908%
16	10.446	1261	1268	1282	rBV	1160124	1880497	25.20%	3.097%
17	10.587	1285	1292	1309	rBV	1037688	1755731	23.53%	2.892%
18	12.040	1532	1539	1545	rVB2	20263	34004	0.46%	0.056%
19	13.198	1732	1736	1743	rVB	15306	24051	0.32%	0.040%
20	13.275	1743	1749	1754	rBV6	7012	11589	0.16%	0.019%
21	13.722	1818	1825	1835	rBV	2076024	2821451	37.81%	4.647%
22	13.998	1865	1872	1884	rBV2	2480363	3617138	48.47%	5.957%
23	14.304	1918	1924	1935	rBV	1701283	2594714	34.77%	4.273%
24	14.516	1954	1960	1974	rBV	120322	237618	3.18%	0.391%
25	14.675	1983	1987	1992	rVB7	6015	9675	0.13%	0.016%
26	14.722	1992	1995	2002	rVB7	8394	14513	0.19%	0.024%
27	15.304	2087	2094	2101	rBV	3214188	4546568	60.92%	7.488%
28	15.422	2109	2114	2128	rBV	751297	1021832	13.69%	1.683%
29	15.539	2130	2134	2141	rVB4	15345	26510	0.36%	0.044%
30	16.086	2223	2227	2232	rVB6	9677	12395	0.17%	0.020%
31	16.733	2334	2337	2341	rBV5	4998	7508	0.10%	0.012%
32	16.822	2349	2352	2354	rBV3	8302	10255	0.14%	0.017%
33	17.057	2385	2392	2402	rBV	2385870	3283940	44.00%	5.409%
34	17.157	2402	2409	2424	rVV	3664954	5268651	70.60%	8.677%
35	17.563	2474	2478	2482	rBV7	5704	8194	0.11%	0.013%
36	17.728	2501	2506	2510	rBV8	14788	20616	0.28%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030904.D
Acq On : 14 Apr 2024 07:09
Operator : MA/JU
Sample : P2036-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.957	2540	2545	2546	rBV2	56340	72929	0.98%	0.120%
38	17.975	2546	2548	2554	rVB	55158	72956	0.98%	0.120%
39	19.022	2721	2726	2730	rBV	51676	69564	0.93%	0.115%
40	19.092	2733	2738	2741	rBV	52709	77256	1.04%	0.127%
41	19.122	2741	2743	2748	rVB3	35439	44328	0.59%	0.073%
42	19.245	2760	2764	2772	rVB4	36976	51784	0.69%	0.085%
43	19.457	2794	2800	2813	rBV	5142747	6722870	90.08%	11.072%
44	21.292	3106	3112	3123	rBV2	2917126	4129207	55.33%	6.801%
45	24.015	3565	3575	3592	rBV2	3063291	7463018	100.00%	12.291%
46	24.210	3599	3608	3622	rVB2	1745263	4433134	59.40%	7.301%




Sum of corrected areas: 60717627

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030904.D
Acq On : 14 Apr 2024 07:09
Operator : MA/JU
Sample : P2036-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

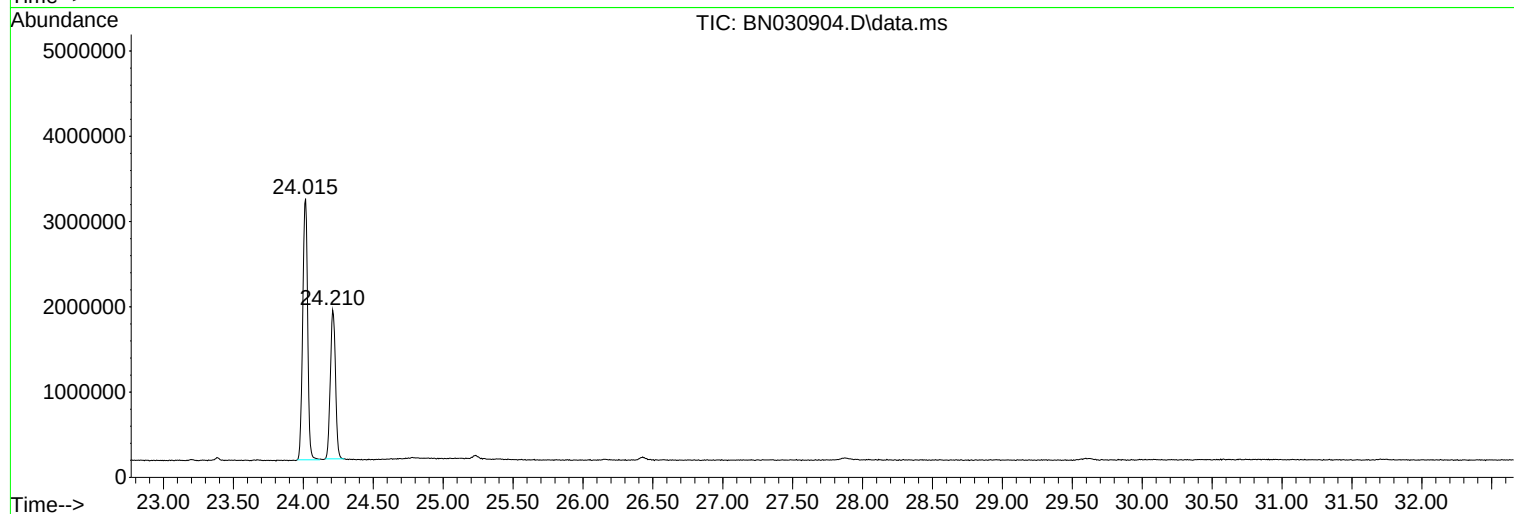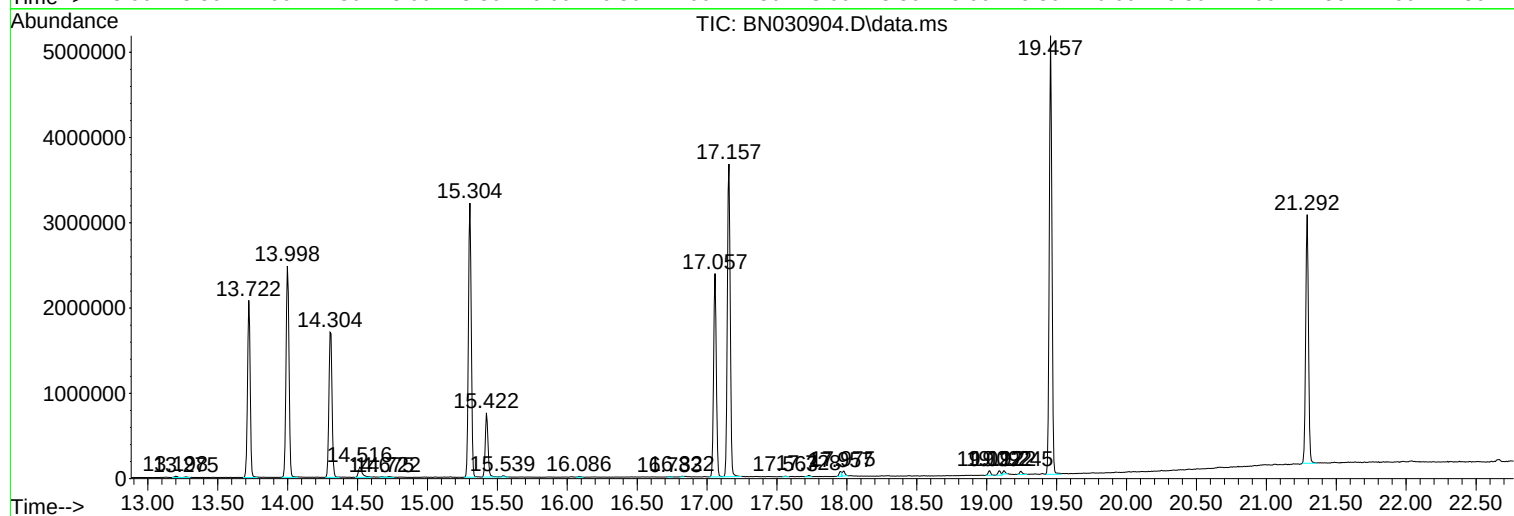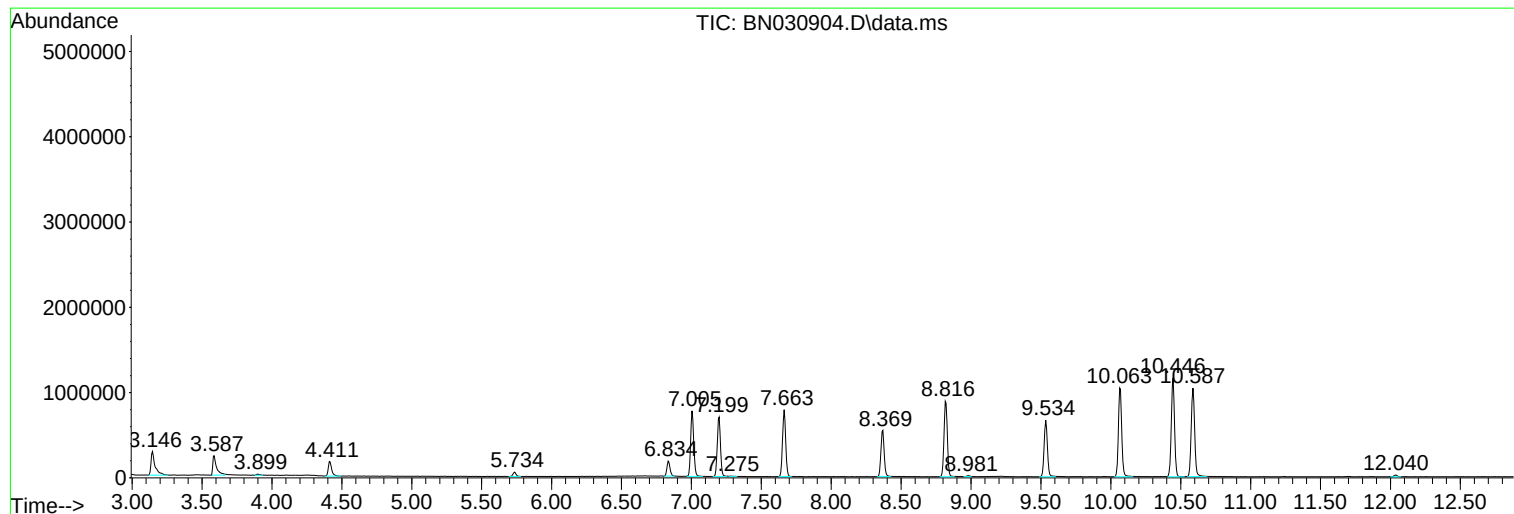

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030904.D
Acq On : 14 Apr 2024 07:09
Operator : MA/JU
Sample : P2036-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX3









Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.411	4.69 ng/ul	284502	1,4-Dichlorobenzene-d4	7.663

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

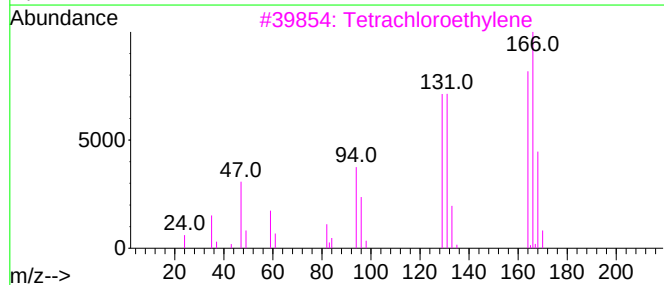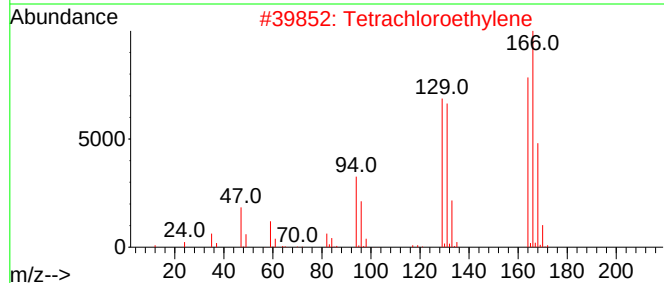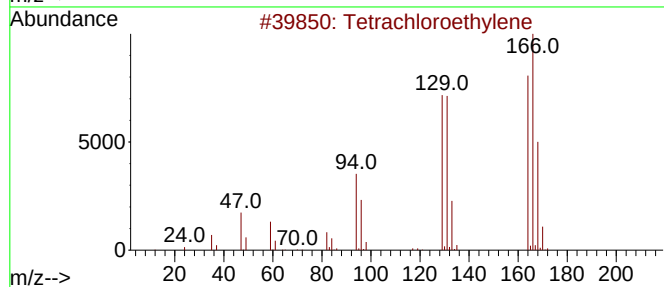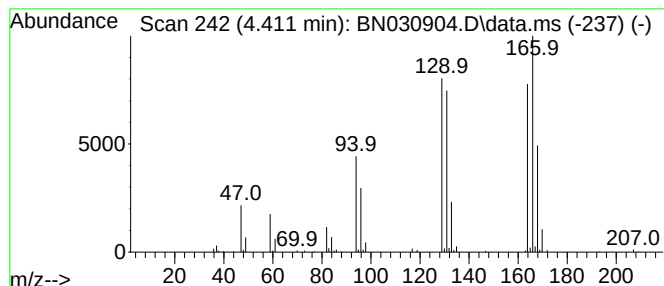

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030904.D
Acq On : 14 Apr 2024 07:09
Operator : MA/JU
Sample : P2036-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.411	4.7	ng/u1	284502	1	7.663	1213920	20.0