

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030910.D
 Acq On : 14 Apr 2024 11:43
 Operator : MA/JU
 Sample : P2036-08
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	22	27	45	rBV2	225352	439963	5.39%	0.784%
2	3.587	99	102	119	rBV	136490	262702	3.22%	0.468%
3	4.411	237	242	253	rVB	199899	338817	4.15%	0.604%
4	5.734	462	467	472	rBV	18512	27308	0.33%	0.049%
5	6.834	648	654	663	rVB	173615	278533	3.41%	0.497%
6	7.005	674	683	692	rBV	700465	1092013	13.38%	1.947%
7	7.199	709	716	727	rBV	648855	1058549	12.97%	1.887%
8	7.663	788	795	804	rBV	517011	819930	10.05%	1.462%
9	8.363	908	914	930	rBV	521358	837159	10.26%	1.493%
10	8.816	984	991	1006	rBV	844889	1373983	16.83%	2.450%
11	9.534	1104	1113	1133	rBV	624301	1023081	12.53%	1.824%
12	10.063	1196	1203	1219	rBV	977540	1635726	20.04%	2.916%
13	10.446	1260	1268	1276	rVB	763945	1254070	15.36%	2.236%
14	10.587	1284	1292	1315	rBV	923065	1593696	19.52%	2.841%
15	11.981	1522	1529	1533	rBV	33006	53927	0.66%	0.096%
16	12.034	1533	1538	1545	rVB	20411	34873	0.43%	0.062%
17	13.198	1732	1736	1741	rVB4	9078	11864	0.15%	0.021%
18	13.722	1818	1825	1841	rBV	1999721	2754727	33.75%	4.911%
19	13.998	1864	1872	1882	rBV2	2411776	3525550	43.19%	6.286%
20	14.304	1916	1924	1935	rBV	1242340	1816874	22.26%	3.239%
21	14.516	1954	1960	1977	rBV	138482	261989	3.21%	0.467%
22	15.304	2087	2094	2107	rBV	3156043	4505374	55.20%	8.033%
23	15.422	2108	2114	2124	rBV	805851	1069915	13.11%	1.908%
24	15.545	2131	2135	2138	rVB3	13614	20097	0.25%	0.036%
25	16.087	2223	2227	2233	rBV5	9883	14036	0.17%	0.025%
26	17.057	2384	2392	2401	rBV	1749620	2391396	29.30%	4.264%
27	17.157	2402	2409	2427	rVV	3768635	5397893	66.13%	9.624%
28	17.728	2502	2506	2511	rVB6	7765	9736	0.12%	0.017%
29	17.951	2538	2544	2550	rBV4	38741	59660	0.73%	0.106%
30	19.016	2721	2725	2731	rBV2	50336	70936	0.87%	0.126%
31	19.092	2733	2738	2742	rBV	45017	62823	0.77%	0.112%
32	19.245	2760	2764	2769	rBV4	24110	33926	0.42%	0.060%
33	19.457	2794	2800	2808	rBV	5286753	6988494	85.62%	12.460%
34	21.292	3106	3112	3122	rBV2	2287271	3250831	39.83%	5.796%
35	24.016	3565	3575	3592	rBV2	3488444	8162410	100.00%	14.553%
36	24.216	3600	3609	3630	rVB2	1388330	3555156	43.56%	6.339%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030910.D
Acq On : 14 Apr 2024 11:43
Operator : MA/JU
Sample : P2036-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 56088017

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030910.D
Acq On : 14 Apr 2024 11:43
Operator : MA/JU
Sample : P2036-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

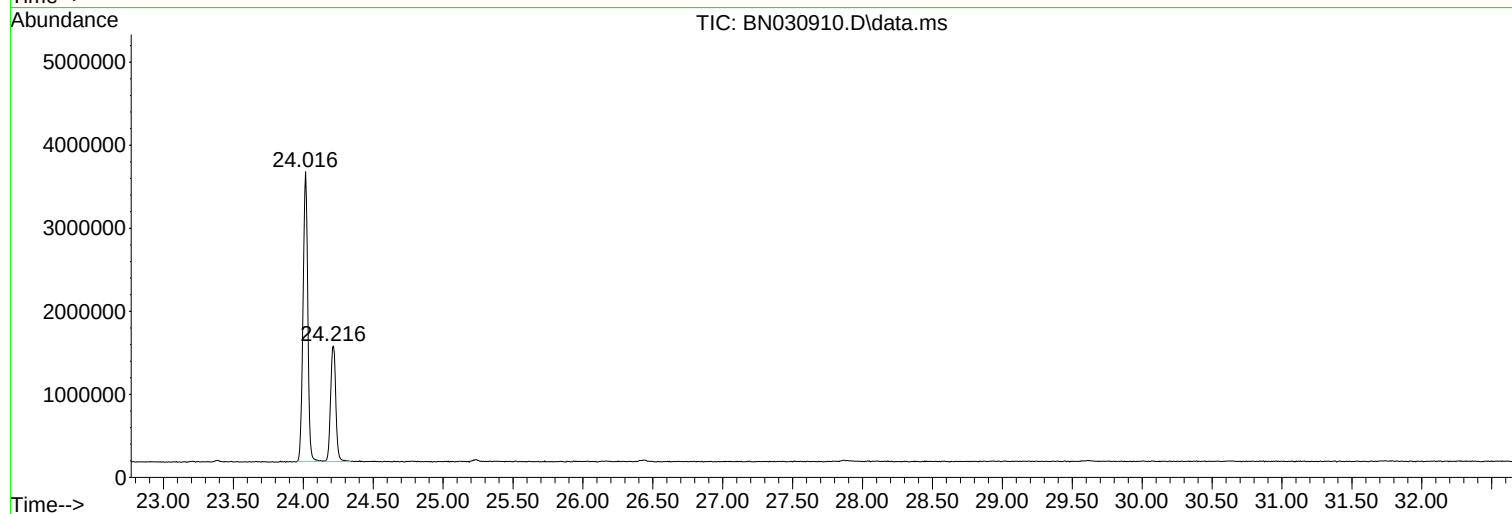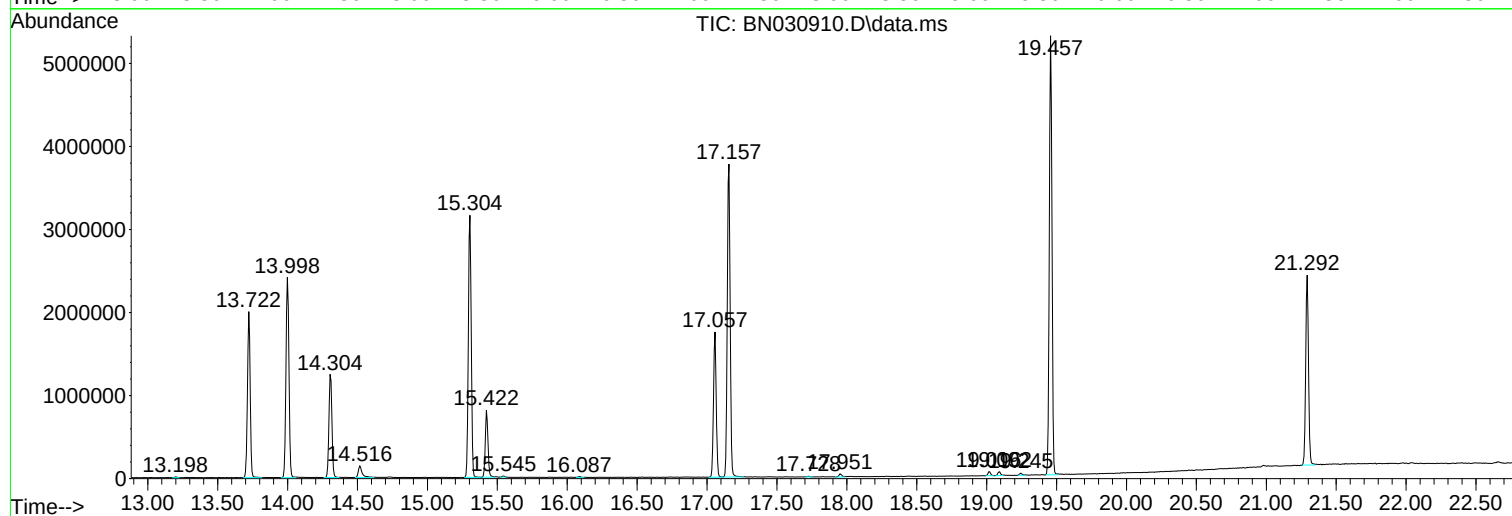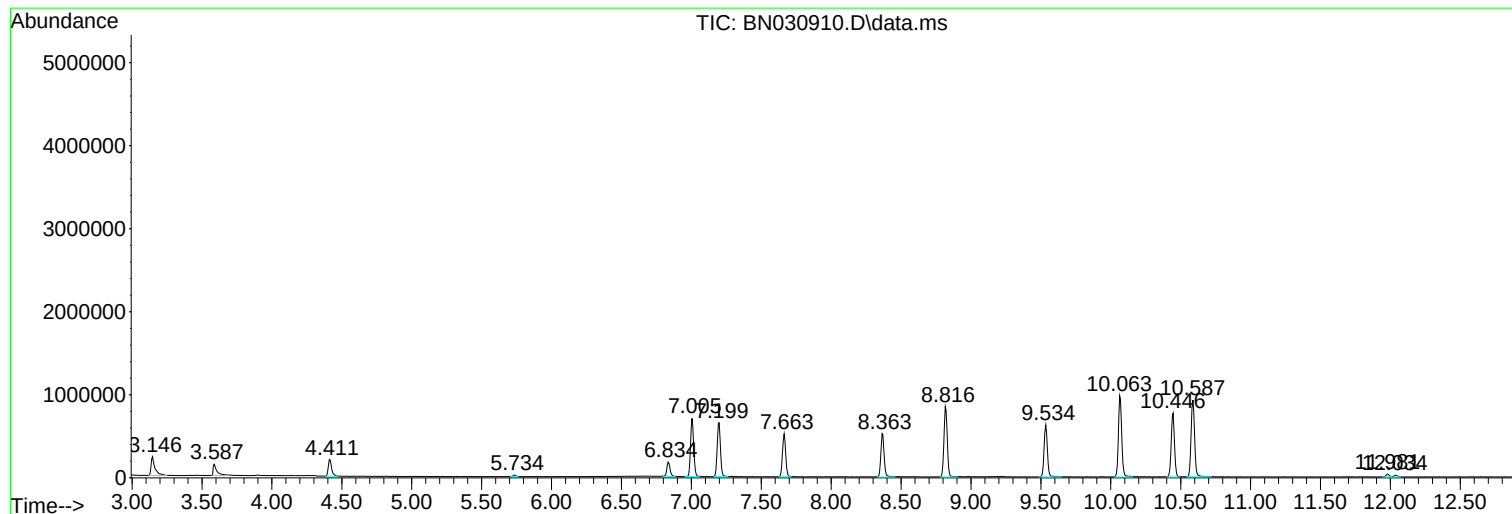

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030910.D
Acq On : 14 Apr 2024 11:43
Operator : MA/JU
Sample : P2036-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.411	8.26 ng/ul	338817	1,4-Dichlorobenzene-d4	7.663

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	25

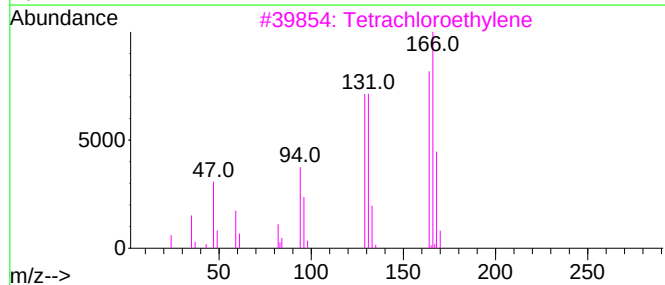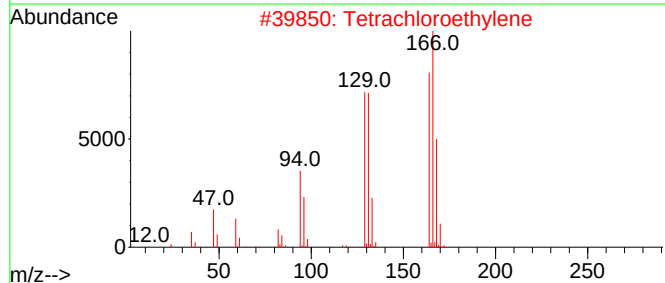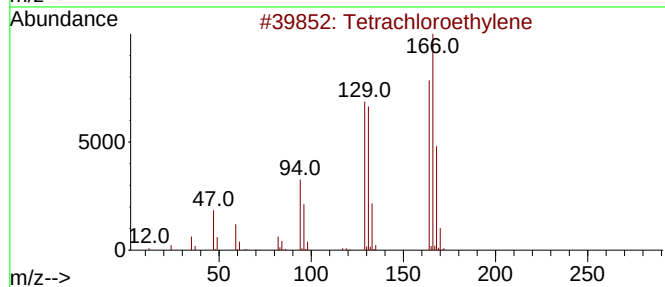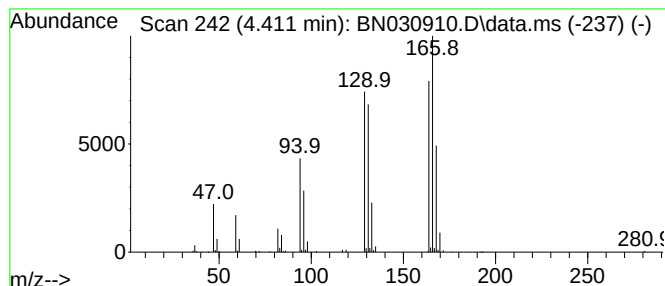

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030910.D
Acq On : 14 Apr 2024 11:43
Operator : MA/JU
Sample : P2036-08
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.411	8.3	ng/u1	338817	1	7.663	819930	20.0