

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030911.D
 Acq On : 14 Apr 2024 12:23
 Operator : MA/JU
 Sample : P2032-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EOME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	29	32	37	rBV	23509	30925	0.35%	0.053%
2	3.452	77	79	90	rVB4	9168	19706	0.22%	0.034%
3	3.587	99	102	124	rBV	189167	350784	4.00%	0.599%
4	6.834	649	654	665	rVB	163738	263154	3.00%	0.450%
5	7.005	676	683	695	rBV	637625	995278	11.34%	1.701%
6	7.199	709	716	727	rBV	590981	964577	10.99%	1.648%
7	7.664	787	795	802	rBV	549782	866872	9.87%	1.481%
8	8.364	908	914	927	rBV	481914	777438	8.86%	1.329%
9	8.816	984	991	1005	rBV	778561	1259083	14.34%	2.152%
10	8.928	1005	1010	1013	rVV6	4616	9066	0.10%	0.015%
11	9.222	1053	1060	1065	rVB6	7098	13609	0.16%	0.023%
12	9.534	1106	1113	1125	rBV	578605	932247	10.62%	1.593%
13	9.946	1178	1183	1189	rBV	10201	17326	0.20%	0.030%
14	10.063	1196	1203	1221	rBV	898520	1526036	17.38%	2.608%
15	10.446	1260	1268	1277	rVB	803097	1330395	15.15%	2.274%
16	10.587	1284	1292	1312	rBV	938416	1586371	18.07%	2.711%
17	11.199	1389	1396	1399	rBV6	5222	9518	0.11%	0.016%
18	12.040	1534	1539	1546	rVB3	16718	28803	0.33%	0.049%
19	13.151	1723	1728	1731	rVB5	5885	9090	0.10%	0.016%
20	13.204	1731	1737	1743	rBV	101390	162514	1.85%	0.278%
21	13.722	1818	1825	1833	rBV	1998238	2743329	31.25%	4.688%
22	13.999	1863	1872	1887	rBV	2318045	3398853	38.72%	5.808%
23	14.304	1918	1924	1931	rBV	1324196	1950866	22.22%	3.334%
24	14.357	1931	1933	1938	rVB4	14228	19004	0.22%	0.032%
25	14.516	1953	1960	1972	rBV	180051	344073	3.92%	0.588%
26	14.675	1981	1987	1991	rBV6	6540	10828	0.12%	0.019%
27	15.116	2055	2062	2064	rBV4	8571	14612	0.17%	0.025%
28	15.140	2064	2066	2076	rVB6	7691	13511	0.15%	0.023%
29	15.304	2087	2094	2103	rBV	3145592	4526546	51.56%	7.736%
30	15.422	2109	2114	2123	rBV	863829	1160870	13.22%	1.984%
31	15.545	2131	2135	2142	rVB2	16137	25234	0.29%	0.043%
32	15.869	2184	2190	2193	rBV8	5299	9093	0.10%	0.016%
33	15.998	2206	2212	2221	rBV10	9917	27023	0.31%	0.046%
34	16.087	2224	2227	2233	rVB6	10844	15744	0.18%	0.027%
35	17.057	2385	2392	2402	rBV	1917361	2697881	30.73%	4.611%
36	17.157	2402	2409	2426	rVV	3922207	5607170	63.87%	9.582%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030911.D
Acq On : 14 Apr 2024 12:23
Operator : MA/JU
Sample : P2032-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0ME7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.351	2437	2442	2444	rBV2	6722	10025	0.11%	0.017%
38	17.734	2502	2507	2513	rVB3	30177	41199	0.47%	0.070%
39	17.951	2540	2544	2551	rBV	71354	105241	1.20%	0.180%
40	18.028	2555	2557	2565	rVB2	9841	12909	0.15%	0.022%
41	18.439	2624	2627	2631	rBV3	8429	9689	0.11%	0.017%
42	19.022	2721	2726	2731	rBV2	57519	81157	0.92%	0.139%
43	19.086	2733	2737	2742	rBV	53555	78693	0.90%	0.134%
44	19.245	2760	2764	2768	rBV	44278	55687	0.63%	0.095%
45	19.457	2794	2800	2808	rBV	5442755	7493411	85.36%	12.806%
46	21.292	3106	3112	3123	rBV2	2669401	3918392	44.64%	6.696%
47	24.022	3566	3576	3588	rBV2	3609079	8778631	100.00%	15.002%
48	24.216	3600	3609	3622	rVB	1652138	4212760	47.99%	7.199%




Sum of corrected areas: 58515223

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030911.D
Acq On : 14 Apr 2024 12:23
Operator : MA/JU
Sample : P2032-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0ME7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

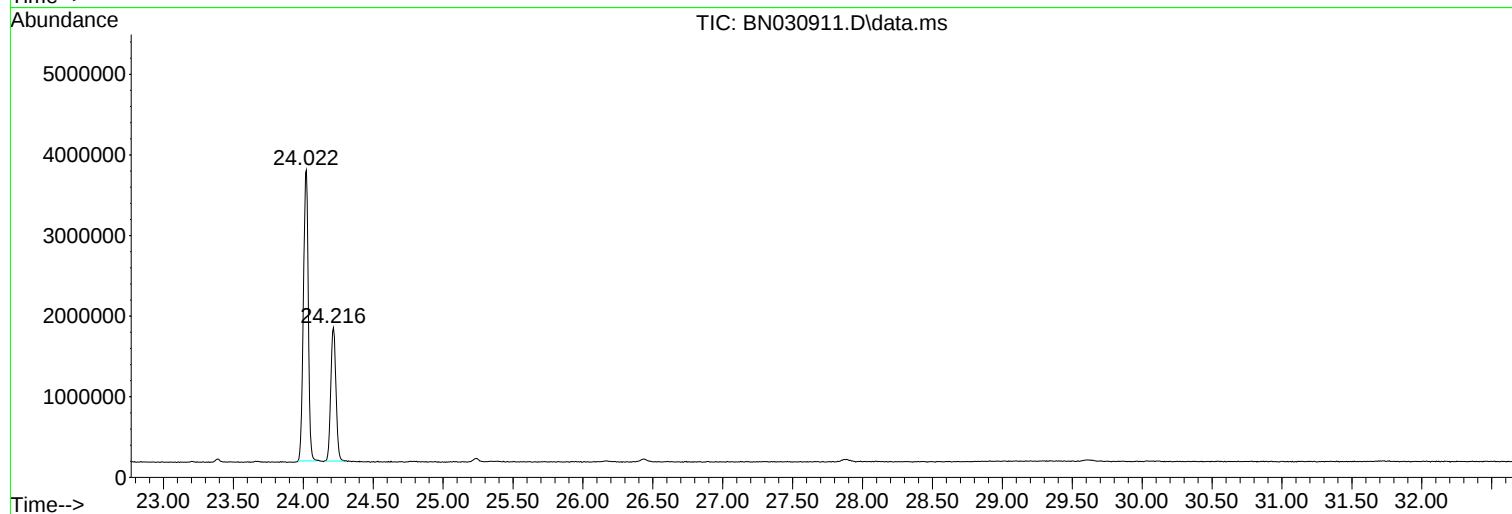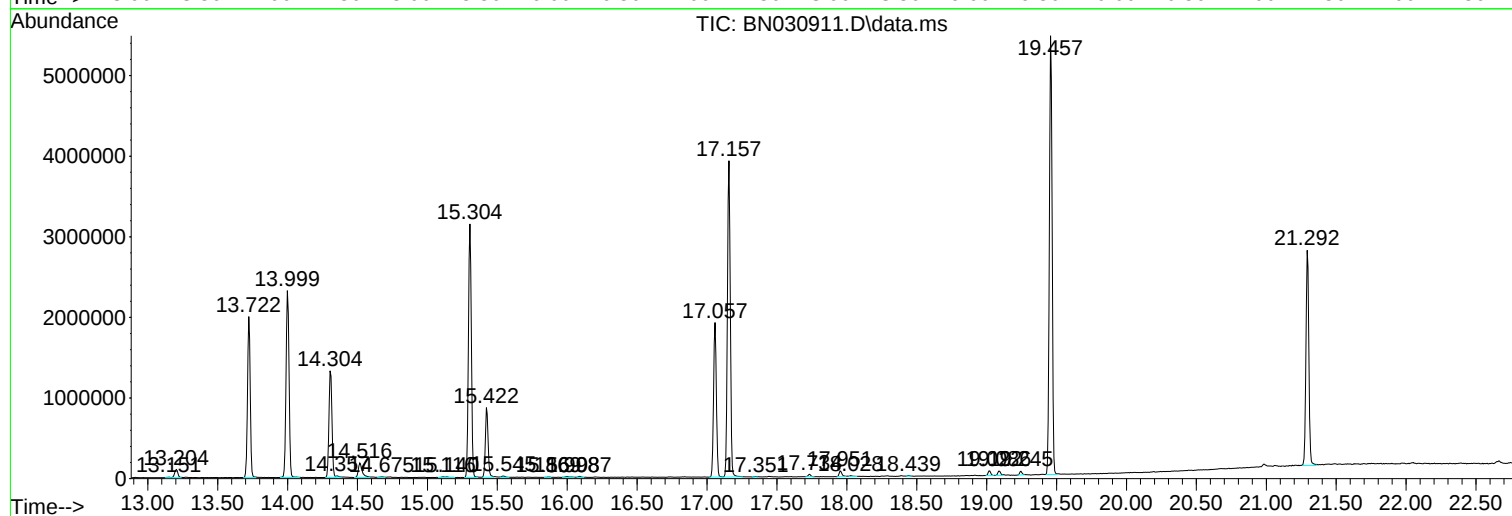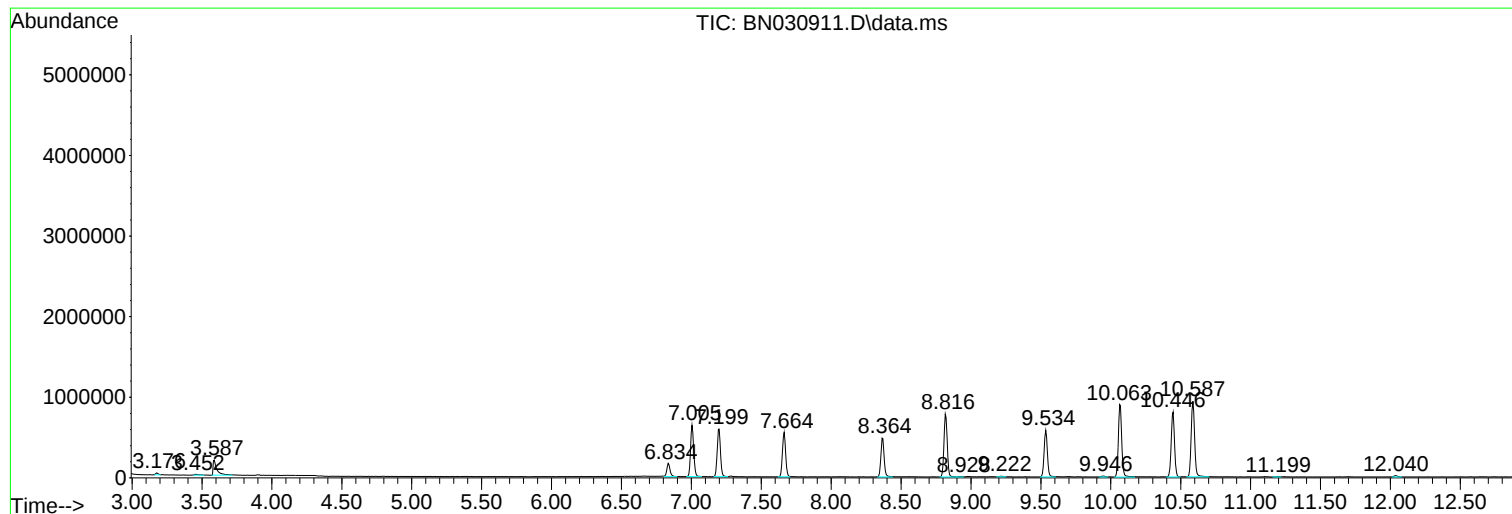

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030911.D
Acq On : 14 Apr 2024 12:23
Operator : MA/JU
Sample : P2032-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0ME7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030911.D
Acq On : 14 Apr 2024 12:23
Operator : MA/JU
Sample : P2032-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0ME7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc