

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030913.D
 Acq On : 14 Apr 2024 13:41
 Operator : MA/JU
 Sample : P2036-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030913.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	41	rVB2	19294	33042	0.46%	0.067%
2	3.593	101	103	116	rBV	68223	137433	1.92%	0.278%
3	3.893	152	154	159	rVB2	6688	8439	0.12%	0.017%
4	4.099	185	189	192	rVB6	6810	9051	0.13%	0.018%
5	5.740	465	468	473	rVB7	4641	8137	0.11%	0.016%
6	6.834	645	654	663	rVB2	113700	209676	2.93%	0.424%
7	7.005	677	683	697	rVB	524617	831421	11.62%	1.681%
8	7.199	709	716	725	rBV	457198	744004	10.40%	1.504%
9	7.663	789	795	806	rBV	557962	881531	12.32%	1.782%
10	8.363	908	914	928	rBV	342264	570476	7.97%	1.153%
11	8.816	984	991	999	rBV	628250	1023200	14.30%	2.069%
12	8.981	1014	1019	1026	rVB3	14142	24241	0.34%	0.049%
13	9.534	1104	1113	1122	rBV	458650	727518	10.17%	1.471%
14	10.063	1196	1203	1218	rBV	707425	1197838	16.74%	2.422%
15	10.446	1261	1268	1276	rVB	813991	1364090	19.06%	2.758%
16	10.587	1284	1292	1308	rBV	648432	1114133	15.57%	2.253%
17	11.228	1397	1401	1406	rBV6	5439	10182	0.14%	0.021%
18	12.040	1533	1539	1544	rBV3	14326	23377	0.33%	0.047%
19	13.204	1732	1737	1742	rBV3	13916	22962	0.32%	0.046%
20	13.722	1818	1825	1838	rBV	1577950	2168775	30.30%	4.385%
21	13.998	1862	1872	1885	rBV	1912044	2745662	38.36%	5.551%
22	14.304	1918	1924	1936	rBV	1341515	1969143	27.51%	3.981%
23	14.516	1953	1960	1970	rBV	82023	164653	2.30%	0.333%
24	15.104	2055	2060	2065	rBV8	3467	7260	0.10%	0.015%
25	15.304	2087	2094	2108	rBV	2541187	3616952	50.54%	7.313%
26	15.422	2108	2114	2124	rBV	634105	838184	11.71%	1.695%
27	15.545	2131	2135	2141	rVB2	13252	20389	0.28%	0.041%
28	16.087	2224	2227	2233	rVB4	9433	11260	0.16%	0.023%
29	17.057	2385	2392	2402	rBV	1868001	2651548	37.05%	5.361%
30	17.157	2402	2409	2419	rBV	3409560	4748921	66.36%	9.602%
31	17.445	2455	2458	2466	rVB7	4127	7798	0.11%	0.016%
32	17.951	2540	2544	2550	rBV2	53019	75965	1.06%	0.154%
33	19.016	2721	2725	2732	rBV2	45885	67825	0.95%	0.137%
34	19.092	2733	2738	2742	rBV	40887	58739	0.82%	0.119%
35	19.245	2760	2764	2768	rBV3	44430	61166	0.85%	0.124%
36	19.457	2794	2800	2808	rBV	4747690	6363536	88.92%	12.866%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030913.D
Acq On : 14 Apr 2024 13:41
Operator : MA/JU
Sample : P2036-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSW7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	21.292	3106	3112	3122	rBV	2608138	3753669	52.45%	7.590%
38	24.016	3566	3575	3593	rVB	3085669	7156836	100.00%	14.470%
39	24.216	3600	3609	3622	rVB	1678566	4029337	56.30%	8.147%




Sum of corrected areas: 49458369

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030913.D
Acq On : 14 Apr 2024 13:41
Operator : MA/JU
Sample : P2036-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

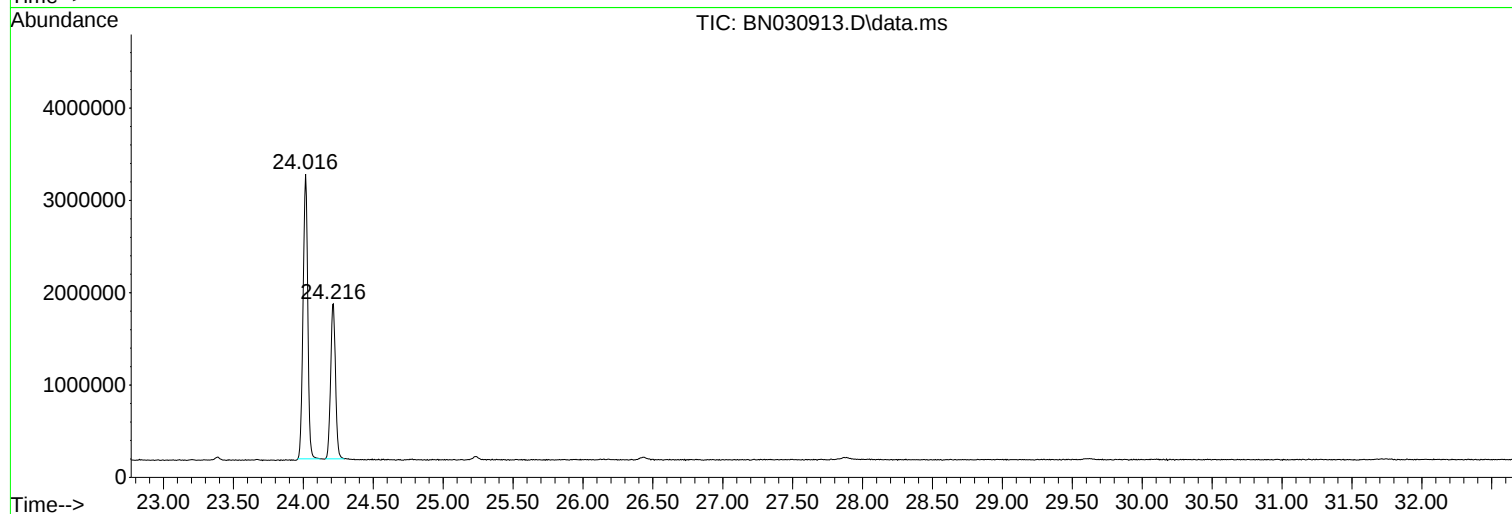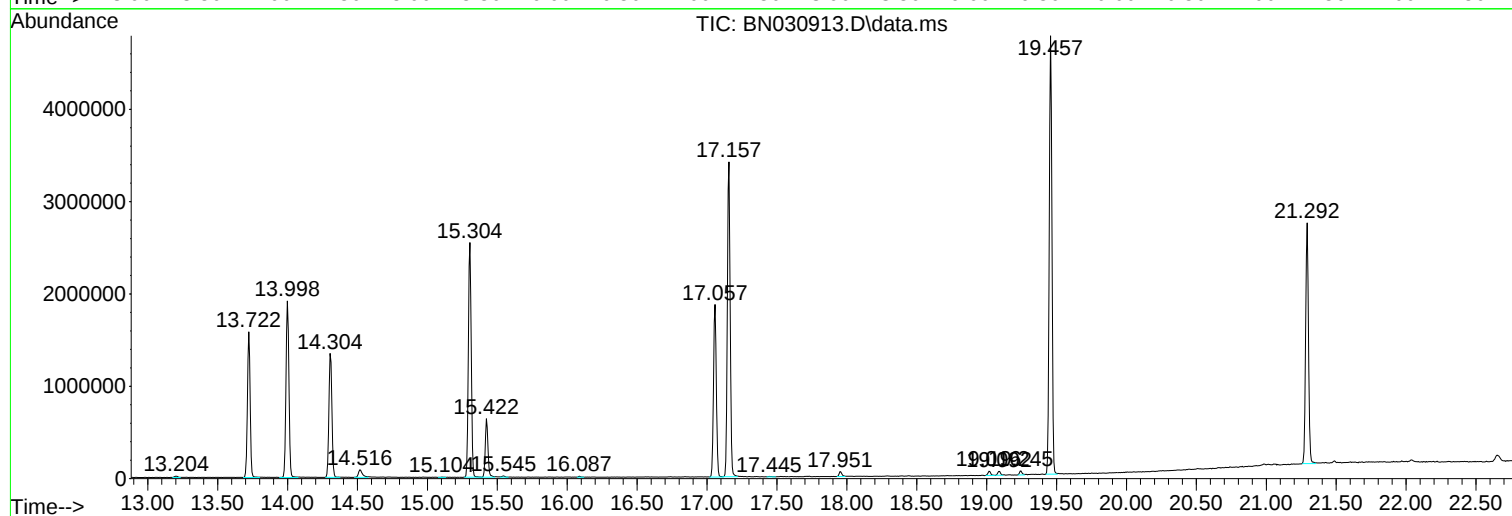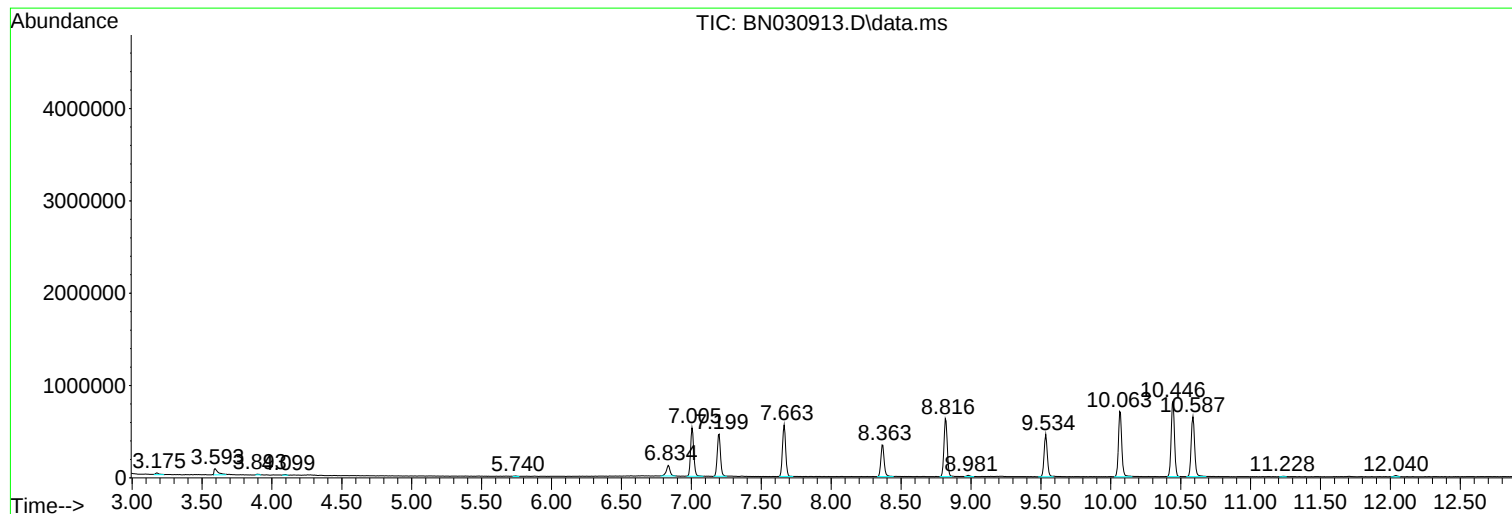

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030913.D
Acq On : 14 Apr 2024 13:41
Operator : MA/JU
Sample : P2036-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030913.D
Acq On : 14 Apr 2024 13:41
Operator : MA/JU
Sample : P2036-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------