

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030914.D
 Acq On : 14 Apr 2024 14:21
 Operator : MA/JU
 Sample : P2036-02
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	22	27	46	rVB	467585	864048	12.49%	1.763%
2	3.587	100	102	119	rBV	107468	211088	3.05%	0.431%
3	3.893	152	154	158	rVB4	6077	7484	0.11%	0.015%
4	4.417	237	243	255	rVB	145002	244019	3.53%	0.498%
5	5.734	462	467	471	rBV4	10750	15996	0.23%	0.033%
6	6.834	649	654	665	rVB	120763	197277	2.85%	0.403%
7	7.005	677	683	697	rVB	544202	844140	12.20%	1.723%
8	7.199	708	716	726	rBV	481358	778856	11.26%	1.590%
9	7.663	788	795	803	rBV	530846	826680	11.95%	1.687%
10	8.369	908	915	924	rBV	378793	617523	8.92%	1.260%
11	8.816	983	991	1001	rBV	635145	1047303	15.13%	2.137%
12	8.981	1014	1019	1023	rBV8	4253	8036	0.12%	0.016%
13	9.216	1054	1059	1063	rVB8	5369	8457	0.12%	0.017%
14	9.534	1105	1113	1127	rBV	467911	747217	10.80%	1.525%
15	10.069	1194	1204	1220	rBV	719552	1231588	17.80%	2.513%
16	10.446	1260	1268	1276	rBV	760666	1262225	18.24%	2.576%
17	10.587	1284	1292	1307	rBV	680400	1158428	16.74%	2.364%
18	12.040	1533	1539	1545	rVB2	15742	26369	0.38%	0.054%
19	13.204	1730	1737	1741	rBV2	12743	18762	0.27%	0.038%
20	13.722	1818	1825	1837	rBV	1585459	2177125	31.46%	4.443%
21	13.998	1864	1872	1885	rBV	1903698	2734595	39.52%	5.581%
22	14.304	1918	1924	1937	rBV	1219470	1813676	26.21%	3.701%
23	14.516	1955	1960	1972	rBV	94588	187259	2.71%	0.382%
24	14.728	1992	1996	1999	rBV5	6391	9714	0.14%	0.020%
25	15.304	2087	2094	2101	rBV	2623711	3656870	52.84%	7.463%
26	15.422	2108	2114	2127	rBV	650763	859070	12.41%	1.753%
27	15.545	2131	2135	2140	rVB	11974	15963	0.23%	0.033%
28	16.092	2224	2228	2231	rBV4	8859	12386	0.18%	0.025%
29	16.863	2350	2359	2364	rVV5	6854	16850	0.24%	0.034%
30	17.057	2386	2392	2402	rBV	1736716	2407638	34.79%	4.914%
31	17.157	2402	2409	2423	rBV	3083217	4560208	65.90%	9.307%
32	17.728	2501	2506	2512	rBV6	13511	19294	0.28%	0.039%
33	17.951	2540	2544	2552	rBV	71894	108720	1.57%	0.222%
34	19.016	2721	2725	2731	rBV4	43438	63576	0.92%	0.130%
35	19.092	2733	2738	2742	rBV	42667	59376	0.86%	0.121%
36	19.245	2760	2764	2769	rBV2	44771	55359	0.80%	0.113%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030914.D
Acq On : 14 Apr 2024 14:21
Operator : MA/JU
Sample : P2036-02
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSW9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.457	2794	2800	2813	rBV2	4397389	6077398	87.82%	12.403%
38	20.980	3056	3059	3068	rBV6	42519	74858	1.08%	0.153%
39	21.292	3106	3112	3121	rBV2	2386145	3362046	48.58%	6.861%
40	24.016	3566	3575	3591	rVB2	2899271	6920009	100.00%	14.123%
41	24.216	3600	3609	3621	rVB	1511821	3691480	53.35%	7.534%




Sum of corrected areas: 48998966

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030914.D
Acq On : 14 Apr 2024 14:21
Operator : MA/JU
Sample : P2036-02
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

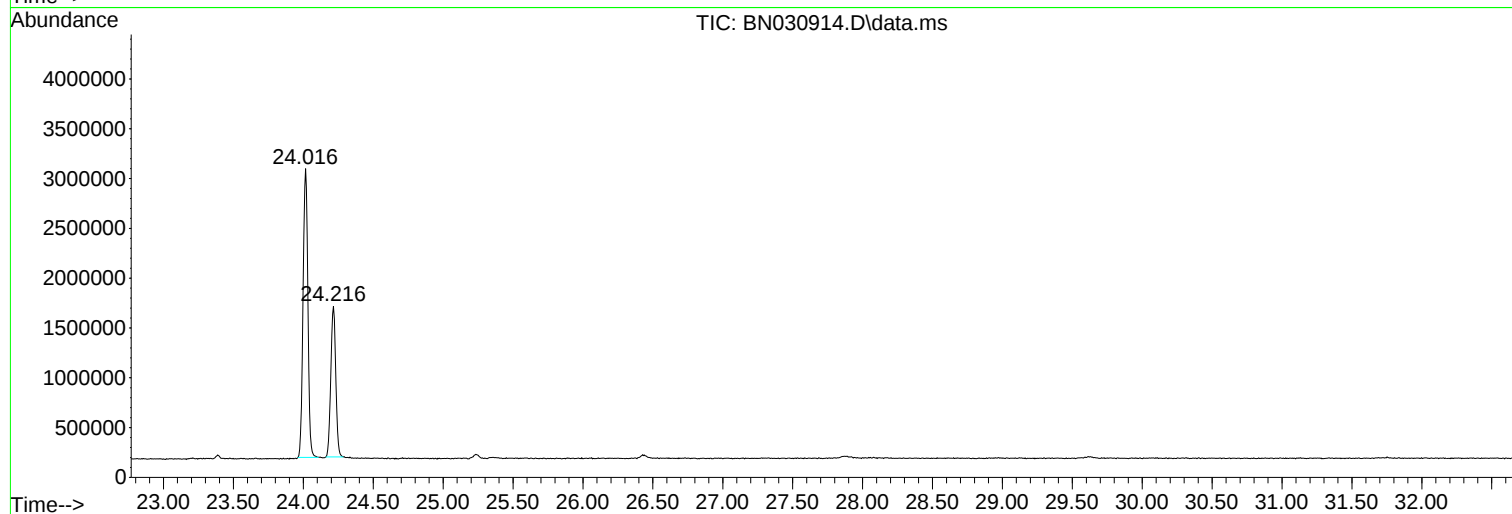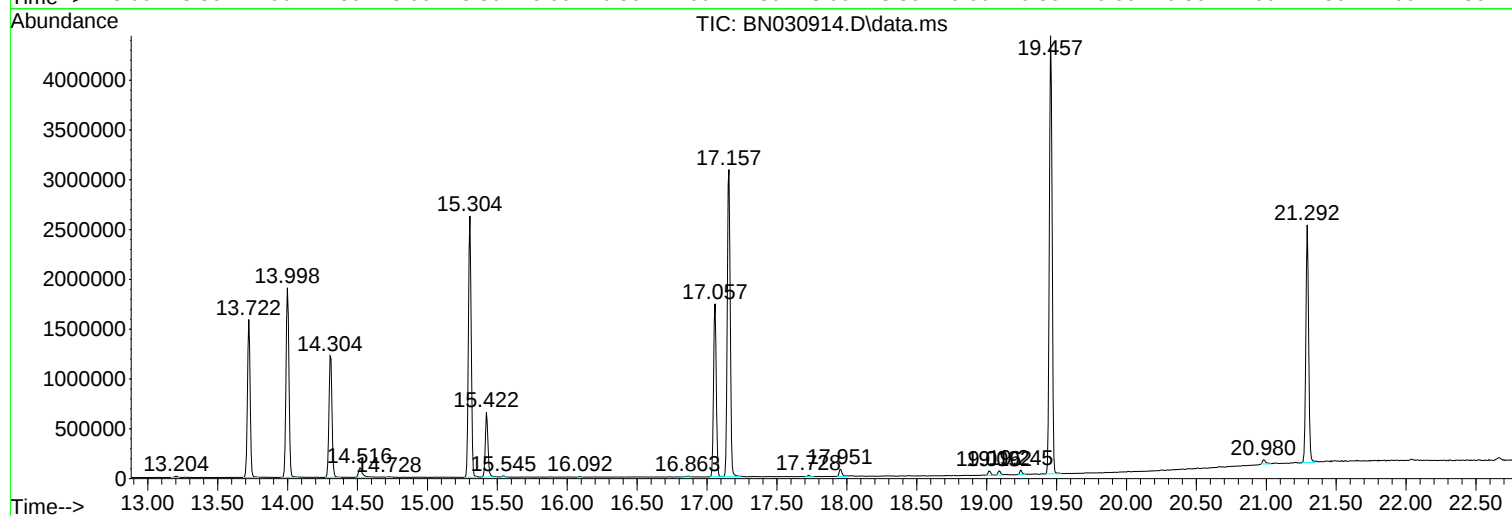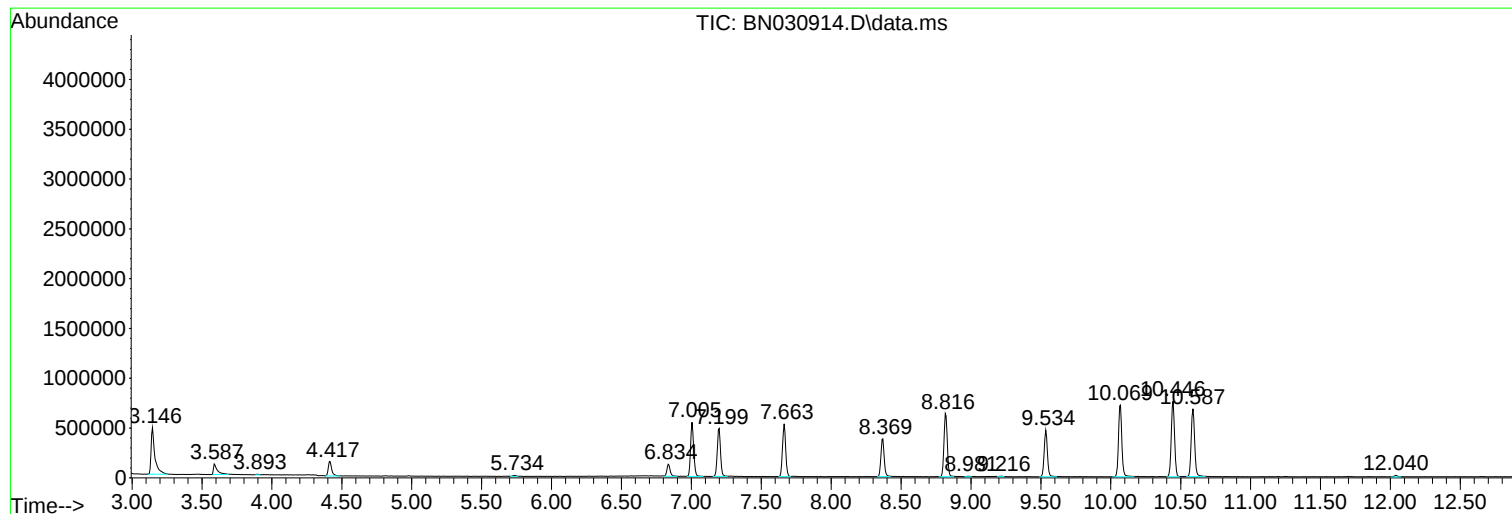

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030914.D
Acq On : 14 Apr 2024 14:21
Operator : MA/JU
Sample : P2036-02
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSW9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.417	5.90 ng/ul	244019	1,4-Dichlorobenzene-d4	7.663

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	32

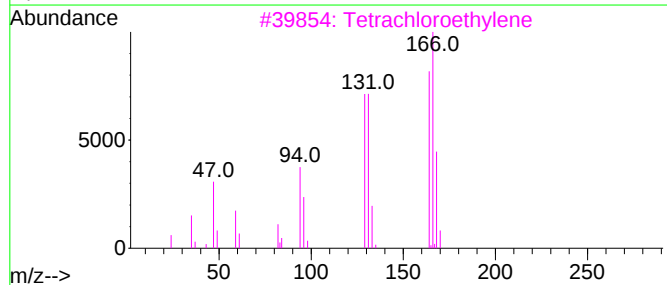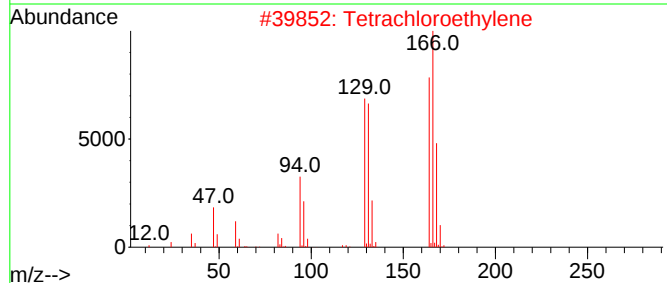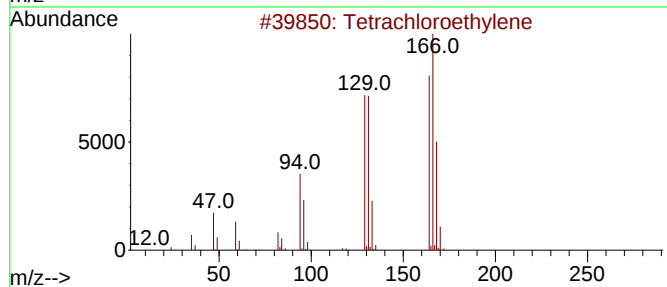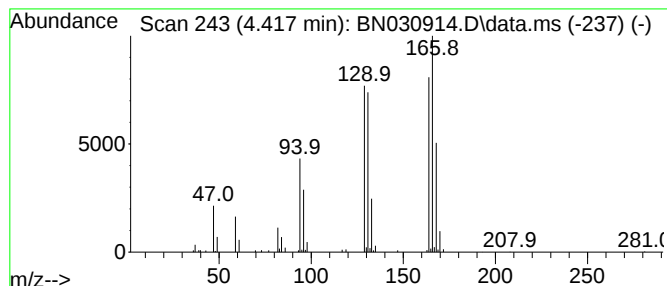

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030914.D
Acq On : 14 Apr 2024 14:21
Operator : MA/JU
Sample : P2036-02
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.417	5.9	ng/u1	244019	1	7.663	826680	20.0