

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030915.D
 Acq On : 14 Apr 2024 15:00
 Operator : MA/JU
 Sample : P2036-03
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSX0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	22	27	46	rBV	451950	823325	12.35%	1.726%
2	3.593	100	103	119	rBV	57527	124329	1.87%	0.261%
3	3.899	151	155	158	rBV5	8811	12670	0.19%	0.027%
4	4.417	237	243	254	rVB	142094	236974	3.55%	0.497%
5	5.740	463	468	472	rBV4	7495	10825	0.16%	0.023%
6	6.834	649	654	662	rVB	129974	206833	3.10%	0.434%
7	7.005	676	683	694	rBV	535841	840322	12.61%	1.762%
8	7.193	709	715	727	rBV	493573	803017	12.05%	1.683%
9	7.664	788	795	803	rBV	524834	809926	12.15%	1.698%
10	8.363	908	914	926	rBV	394231	647348	9.71%	1.357%
11	8.816	982	991	1006	rBV	636943	1051607	15.78%	2.204%
12	8.975	1013	1018	1025	rVB8	5494	9463	0.14%	0.020%
13	9.222	1053	1060	1064	rVB5	6291	12688	0.19%	0.027%
14	9.534	1106	1113	1131	rBV	467732	764980	11.48%	1.604%
15	10.063	1195	1203	1213	rBV	745802	1249659	18.75%	2.620%
16	10.446	1261	1268	1277	rBV	754630	1233899	18.51%	2.587%
17	10.587	1285	1292	1307	rBV	440270	753048	11.30%	1.579%
18	11.252	1402	1405	1413	rVB7	3498	7159	0.11%	0.015%
19	12.034	1533	1538	1545	rVB	13394	23881	0.36%	0.050%
20	13.204	1732	1737	1745	rVB2	12386	19543	0.29%	0.041%
21	13.722	1819	1825	1837	rBV	1554743	2110950	31.67%	4.425%
22	13.998	1865	1872	1884	rBV	1873343	2703895	40.56%	5.668%
23	14.304	1917	1924	1938	rBV	1243828	1796984	26.96%	3.767%
24	14.516	1955	1960	1977	rBV	96600	199692	3.00%	0.419%
25	14.728	1992	1996	2000	rVB4	4886	7752	0.12%	0.016%
26	15.304	2087	2094	2101	rBV	2543742	3532596	52.99%	7.405%
27	15.422	2108	2114	2128	rBV	598883	809877	12.15%	1.698%
28	15.545	2130	2135	2139	rVB5	11370	18750	0.28%	0.039%
29	16.087	2222	2227	2232	rBV5	7998	12152	0.18%	0.025%
30	16.869	2357	2360	2365	rVB5	6565	8760	0.13%	0.018%
31	17.057	2385	2392	2402	rBV	1731477	2448498	36.73%	5.133%
32	17.157	2402	2409	2422	rVV	3009606	4367085	65.51%	9.154%
33	17.728	2503	2506	2509	rVB3	13370	14252	0.21%	0.030%
34	17.951	2540	2544	2549	rBV2	61658	88052	1.32%	0.185%
35	19.016	2721	2725	2732	rVB2	43207	58402	0.88%	0.122%
36	19.086	2734	2737	2741	rVV	33990	42122	0.63%	0.088%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030915.D
Acq On : 14 Apr 2024 15:00
Operator : MA/JU
Sample : P2036-03
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.245	2760	2764	2772	rBV3	32975	50500	0.76%	0.106%
38	19.457	2794	2800	2810	rBV2	4221279	5857768	87.87%	12.279%
39	20.986	3056	3060	3068	rBV8	38870	83446	1.25%	0.175%
40	21.292	3106	3112	3121	rBV	2437272	3447147	51.71%	7.226%
41	24.016	3566	3575	3591	rVB2	2890749	6666120	100.00%	13.974%
42	24.216	3600	3609	3625	rVB	1491823	3738365	56.08%	7.836%




Sum of corrected areas: 47704661

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030915.D
Acq On : 14 Apr 2024 15:00
Operator : MA/JU
Sample : P2036-03
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

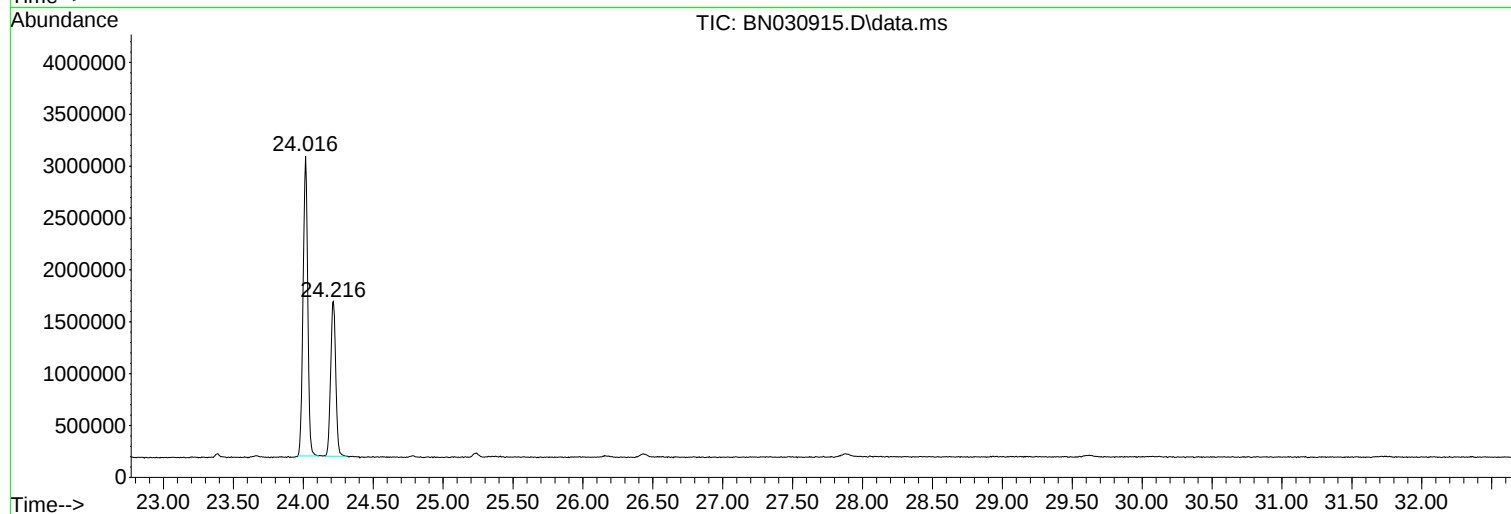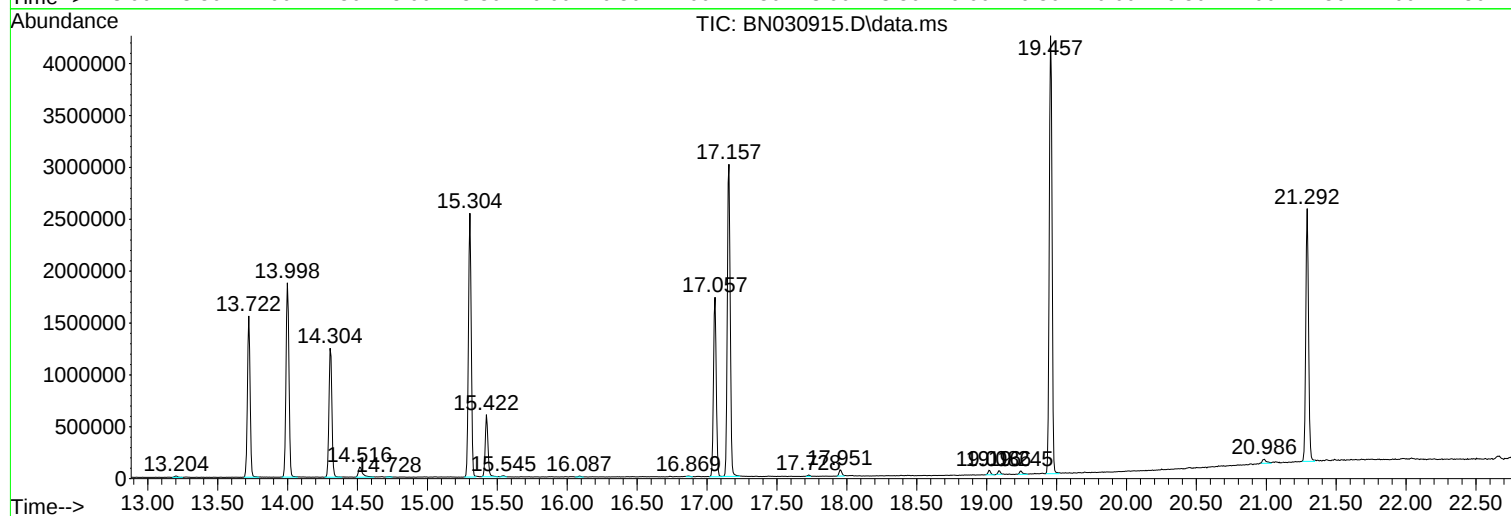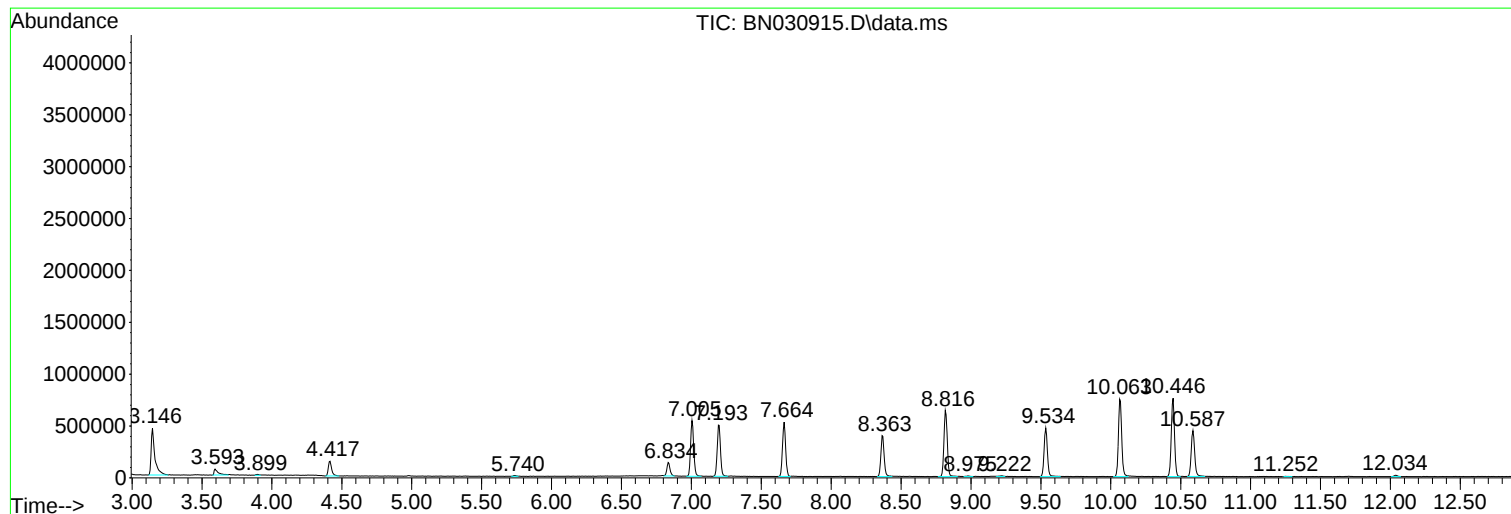

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030915.D
Acq On : 14 Apr 2024 15:00
Operator : MA/JU
Sample : P2036-03
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.417	5.85 ng/ul	236974	1,4-Dichlorobenzene-d4	7.664

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	25

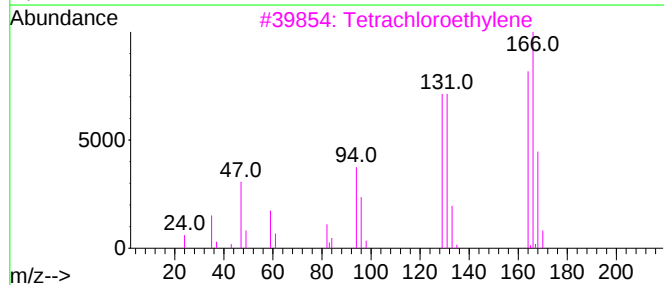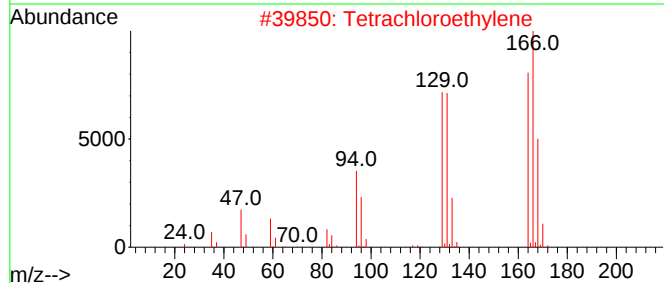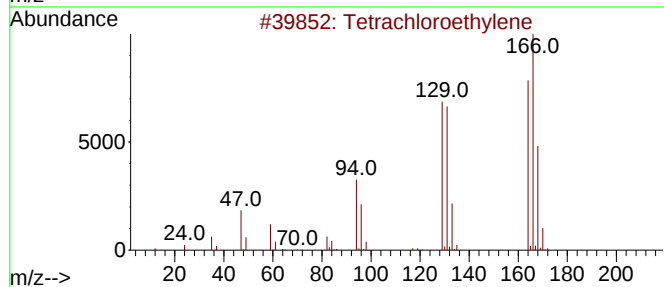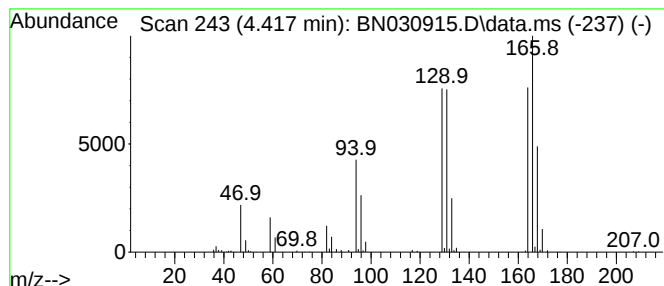

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030915.D
Acq On : 14 Apr 2024 15:00
Operator : MA/JU
Sample : P2036-03
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.417	5.8	ng/u1	236974	1	7.664	809926	20.0