

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030924.D
 Acq On : 14 Apr 2024 21:34
 Operator : MA/JU
 Sample : PB160113BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK113

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	38	rBV	38031	57633	0.87%	0.101%
2	3.581	97	101	120	rBV	539127	1015350	15.27%	1.780%
3	3.899	151	155	158	rBV	9500	12490	0.19%	0.022%
4	6.834	648	654	668	rVB	792764	1248171	18.77%	2.189%
5	7.005	677	683	694	rVB	641667	984680	14.81%	1.727%
6	7.193	709	715	726	rBV	770285	1235329	18.58%	2.166%
7	7.663	786	795	806	rBV	605631	965209	14.51%	1.692%
8	8.363	907	914	926	rBV	1007620	1584160	23.82%	2.778%
9	8.816	984	991	1003	rBV	758967	1220820	18.36%	2.141%
10	9.534	1105	1113	1128	rBV	607535	982757	14.78%	1.723%
11	10.063	1195	1203	1219	rBV	982160	1646142	24.75%	2.887%
12	10.440	1260	1267	1278	rBV	881694	1479666	22.25%	2.595%
13	10.587	1285	1292	1313	rBV	1073769	1842228	27.70%	3.230%
14	12.040	1532	1539	1546	rVB3	16796	29461	0.44%	0.052%
15	13.204	1728	1737	1741	rBV3	17026	29408	0.44%	0.052%
16	13.722	1818	1825	1834	rBV	1879928	2531625	38.07%	4.439%
17	13.998	1865	1872	1886	rBV	2183502	3202331	48.15%	5.615%
18	14.304	1917	1924	1934	rBV	1500055	2130491	32.04%	3.736%
19	14.510	1952	1959	1980	rBV	878763	1430438	21.51%	2.508%
20	15.304	2087	2094	2103	rBV	2829768	4110910	61.82%	7.208%
21	15.422	2107	2114	2127	rBV	759460	1039902	15.64%	1.823%
22	15.539	2130	2134	2138	rVB3	13676	19493	0.29%	0.034%
23	16.086	2222	2227	2231	rBV5	8728	12491	0.19%	0.022%
24	16.728	2334	2336	2343	rVB5	4923	9158	0.14%	0.016%
25	16.839	2350	2355	2360	rBV6	4409	7860	0.12%	0.014%
26	17.057	2385	2392	2402	rBV	1985596	2808545	42.23%	4.925%
27	17.157	2402	2409	2424	rVV	3291993	4791429	72.05%	8.402%
28	17.728	2500	2506	2510	rVB7	9162	14566	0.22%	0.026%
29	17.951	2542	2544	2551	rVB5	6392	9263	0.14%	0.016%
30	18.286	2598	2601	2604	rBV5	6109	8544	0.13%	0.015%
31	19.016	2721	2725	2730	rBV	43082	59939	0.90%	0.105%
32	19.086	2733	2737	2744	rVV	38648	53530	0.80%	0.094%
33	19.457	2794	2800	2807	rBV	4634804	6196996	93.18%	10.866%
34	21.292	3106	3112	3120	rBV	2565970	3621829	54.46%	6.351%
35	24.015	3565	3575	3592	rVB2	2820366	6650210	100.00%	11.661%
36	24.210	3599	3608	3624	rVB	1610825	3985736	59.93%	6.989%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030924.D
Acq On : 14 Apr 2024 21:34
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK113

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 57028790

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030924.D
Acq On : 14 Apr 2024 21:34
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK113

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

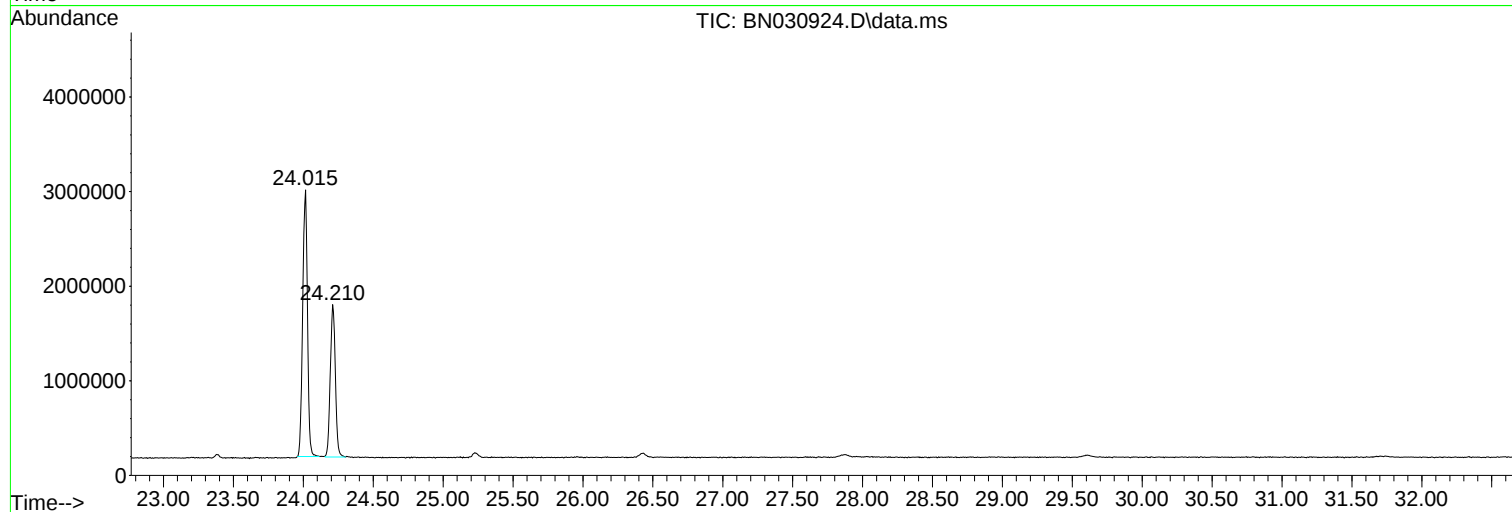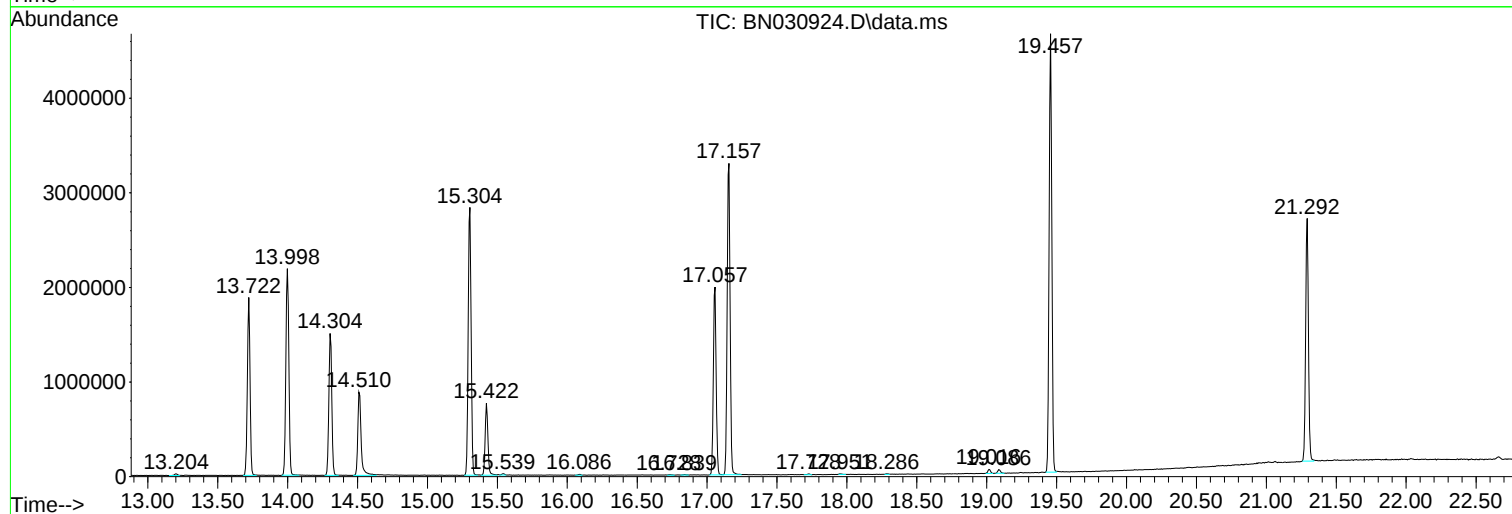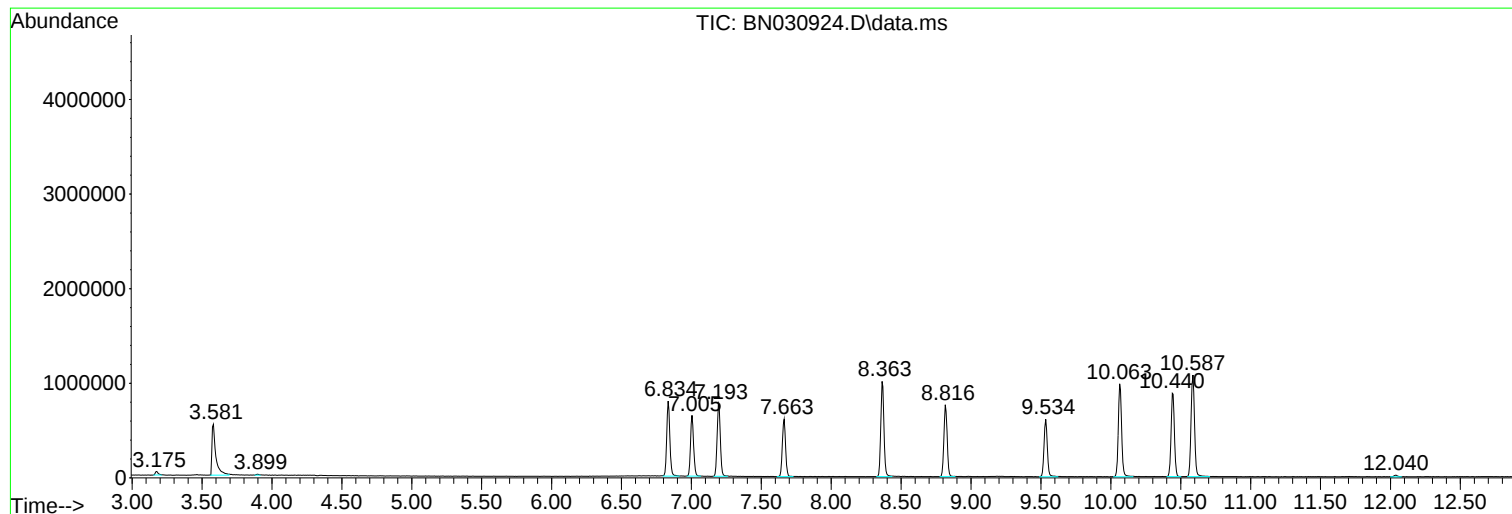

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030924.D
Acq On : 14 Apr 2024 21:34
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK113

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030924.D
Acq On : 14 Apr 2024 21:34
Operator : MA/JU
Sample : PB160113BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK113

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc