

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030927.D
 Acq On : 14 Apr 2024 23:32
 Operator : MA/JU
 Sample : P2006-03
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	46	rVB	53129	84332	0.52%	0.068%
2	3.452	76	79	88	rBV4	10984	26159	0.16%	0.021%
3	3.581	98	101	125	rVB	298544	554238	3.44%	0.445%
4	3.899	151	155	162	rVB2	18050	28655	0.18%	0.023%
5	5.005	338	343	354	rVB	83178	135500	0.84%	0.109%
6	6.610	612	616	620	rBV2	10251	21340	0.13%	0.017%
7	6.834	648	654	668	rVB	353719	567091	3.52%	0.455%
8	7.005	676	683	696	rBV	1379501	2146661	13.31%	1.724%
9	7.193	708	715	727	rBV	1272555	2073431	12.85%	1.665%
10	7.663	786	795	806	rBV	1452779	2356135	14.61%	1.892%
11	8.010	849	854	859	rVB2	17118	27292	0.17%	0.022%
12	8.363	908	914	922	rBV	1036534	1707058	10.58%	1.371%
13	8.434	922	926	931	rVB6	13341	26784	0.17%	0.022%
14	8.822	983	992	1001	rBV	1661045	2776174	17.21%	2.230%
15	9.216	1053	1059	1068	rVB	17452	32281	0.20%	0.026%
16	9.534	1105	1113	1125	rBV	1398629	2222055	13.78%	1.785%
17	10.063	1196	1203	1221	rBV	1998618	3334692	20.67%	2.678%
18	10.446	1260	1268	1281	rBV	2082147	3467865	21.50%	2.785%
19	10.587	1281	1292	1312	rBV	1974270	3340026	20.71%	2.683%
20	11.704	1476	1482	1487	rVB	15247	23512	0.15%	0.019%
21	12.040	1533	1539	1546	rVB2	39188	65749	0.41%	0.053%
22	13.198	1730	1736	1742	rBV2	19925	34395	0.21%	0.028%
23	13.722	1818	1825	1839	rBV	4108222	5990004	37.14%	4.811%
24	13.998	1863	1872	1886	rBV2	4820074	7399134	45.87%	5.943%
25	14.304	1917	1924	1933	rBV	3213870	4892805	30.33%	3.930%
26	14.516	1954	1960	1976	rBV	438677	747811	4.64%	0.601%
27	14.728	1991	1996	2002	rVB7	14225	28795	0.18%	0.023%
28	15.304	2087	2094	2102	rBV	6449357	9386027	58.19%	7.538%
29	15.428	2108	2115	2128	rBV	2211545	3185394	19.75%	2.558%
30	15.545	2130	2135	2144	rVB2	35784	68643	0.43%	0.055%
31	16.086	2223	2227	2233	rVB2	28286	37474	0.23%	0.030%
32	16.733	2332	2337	2342	rBV5	15315	27260	0.17%	0.022%
33	16.839	2348	2355	2360	rBV3	12978	25982	0.16%	0.021%
34	17.057	2385	2392	2402	rBV	4496105	6364730	39.46%	5.112%
35	17.157	2402	2409	2424	rVV2	7709167	11369014	70.48%	9.131%
36	17.345	2436	2441	2447	rBV3	10293	16681	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030927.D
 Acq On : 14 Apr 2024 23:32
 Operator : MA/JU
 Sample : P2006-03
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	17.728	2501	2506	2510	rBV7	33255	44847	0.28%	0.036%
38	17.957	2539	2545	2552	rBV	201680	304555	1.89%	0.245%
39	18.286	2597	2601	2608	rBV4	19868	35392	0.22%	0.028%
40	18.439	2624	2627	2632	rVB5	16284	22319	0.14%	0.018%
41	19.016	2720	2725	2732	rBV2	136972	184153	1.14%	0.148%
42	19.086	2732	2737	2741	rBV	127463	182694	1.13%	0.147%
43	19.245	2759	2764	2771	rBV	128023	192808	1.20%	0.155%
44	19.392	2786	2789	2793	rBV4	16641	20408	0.13%	0.016%
45	19.457	2794	2800	2808	rBV2	9363260	14310063	88.72%	11.493%
46	20.010	2892	2894	2898	rVB2	24929	23496	0.15%	0.019%
47	20.504	2976	2978	2982	rVB3	34465	37512	0.23%	0.030%
48	20.980	3055	3059	3068	rBV	130662	221245	1.37%	0.178%
49	21.292	3105	3112	3127	rBV2	5324137	8024045	49.75%	6.444%
50	21.480	3142	3144	3150	rVB2	58611	70480	0.44%	0.057%
51	22.039	3235	3239	3244	rBV2	72523	104684	0.65%	0.084%
52	22.657	3339	3344	3356	rVB4	186191	382771	2.37%	0.307%
53	23.380	3462	3467	3473	rVB	170713	305116	1.89%	0.245%
54	24.021	3564	3576	3591	rBV	6239514	16130191	100.00%	12.955%
55	24.215	3599	3609	3623	rVB2	3436027	8830971	54.75%	7.093%
56	25.227	3775	3781	3791	rVB2	194127	491371	3.05%	0.395%




Sum of corrected areas: 124510300

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030927.D
Acq On : 14 Apr 2024 23:32
Operator : MA/JU
Sample : P2006-03
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

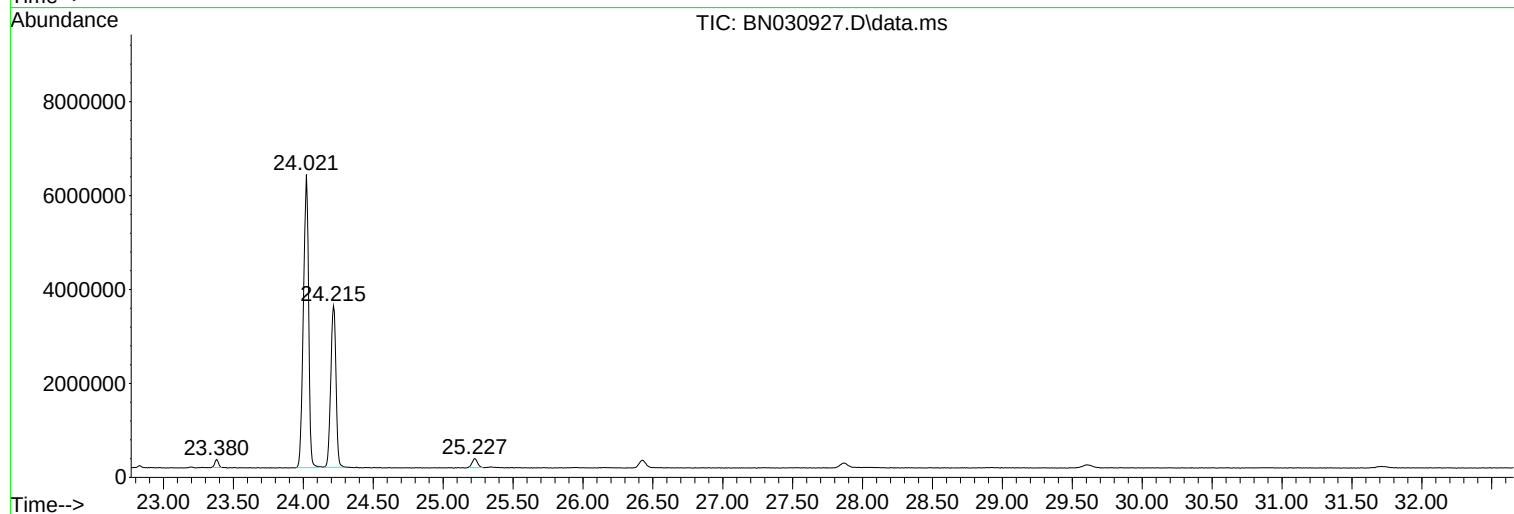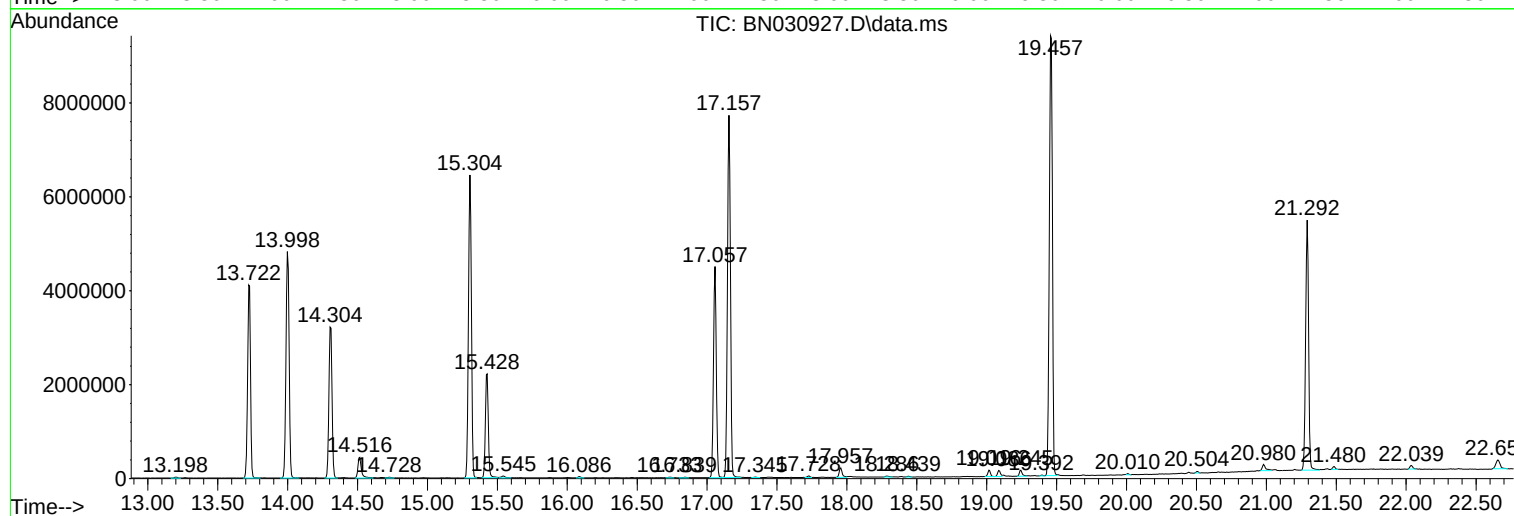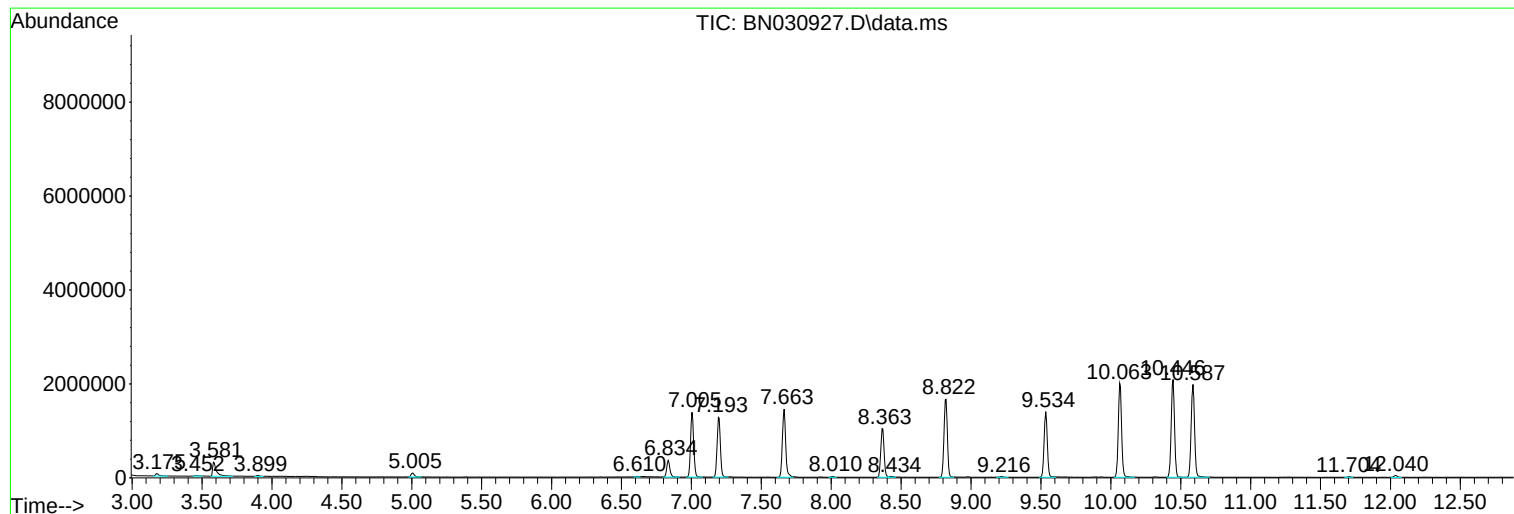

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030927.D
Acq On : 14 Apr 2024 23:32
Operator : MA/JU
Sample : P2006-03
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030927.D
Acq On : 14 Apr 2024 23:32
Operator : MA/JU
Sample : P2006-03
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------