

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030928.D
 Acq On : 15 Apr 2024 00:11
 Operator : MA/JU
 Sample : P2006-04
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	44	rVB	40928	67177	0.46%	0.064%
2	3.452	75	79	82	rBV2	13122	20500	0.14%	0.019%
3	3.581	99	101	115	rBV	199654	382076	2.60%	0.363%
4	3.899	151	155	158	rBV2	12721	19257	0.13%	0.018%
5	6.834	648	654	666	rVB	230501	367090	2.50%	0.348%
6	7.005	674	683	693	rBV	1130538	1770102	12.03%	1.680%
7	7.193	707	715	727	rBV	979411	1589399	10.80%	1.509%
8	7.663	788	795	802	rBV	1165522	1835760	12.48%	1.742%
9	7.722	802	805	815	rVB2	21624	36866	0.25%	0.035%
10	8.363	907	914	924	rBV	751553	1192742	8.11%	1.132%
11	8.816	983	991	1003	rBV	1392776	2263467	15.38%	2.148%
12	8.981	1013	1019	1023	rBV6	10804	19682	0.13%	0.019%
13	9.216	1054	1059	1063	rVB	16503	24586	0.17%	0.023%
14	9.534	1104	1113	1127	rBV	1092716	1777733	12.08%	1.687%
15	10.063	1195	1203	1222	rBV	1578467	2628458	17.87%	2.495%
16	10.234	1226	1232	1240	rVB7	8056	17129	0.12%	0.016%
17	10.446	1260	1268	1276	rBV	1679876	2823217	19.19%	2.680%
18	10.587	1284	1292	1311	rVB	1592690	2631872	17.89%	2.498%
19	11.157	1384	1389	1399	rBV2	52241	89496	0.61%	0.085%
20	12.034	1531	1538	1545	rBV	30535	52213	0.35%	0.050%
21	12.822	1666	1672	1677	rVB4	11614	20424	0.14%	0.019%
22	13.198	1732	1736	1744	rBV	24840	39527	0.27%	0.038%
23	13.722	1818	1825	1838	rBV	3419571	4812579	32.71%	4.568%
24	13.998	1865	1872	1881	rBV2	4002851	5812025	39.50%	5.517%
25	14.304	1917	1924	1932	rBV	2691739	4040369	27.46%	3.835%
26	14.516	1954	1960	1974	rBV	267753	472409	3.21%	0.448%
27	14.722	1991	1995	2002	rVB9	9847	18173	0.12%	0.017%
28	15.304	2087	2094	2104	rBV	5304366	7733040	52.56%	7.340%
29	15.422	2108	2114	2128	rVV	1793622	2531731	17.21%	2.403%
30	15.540	2130	2134	2144	rVB3	31179	57287	0.39%	0.054%
31	16.087	2222	2227	2232	rBV4	21072	32129	0.22%	0.030%
32	16.845	2350	2356	2359	rBV	9818	16865	0.11%	0.016%
33	17.057	2385	2392	2402	rBV	3831464	5362886	36.45%	5.090%
34	17.157	2402	2409	2421	rVV2	6454981	9667499	65.71%	9.176%
35	17.728	2500	2506	2510	rBV5	24389	33404	0.23%	0.032%
36	17.951	2539	2544	2553	rBV	88636	138544	0.94%	0.132%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030928.D
 Acq On : 15 Apr 2024 00:11
 Operator : MA/JU
 Sample : P2006-04
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	18.286	2597	2601	2612	rBV5	21002	53043	0.36%	0.050%
38	18.439	2623	2627	2633	rVB6	13589	20807	0.14%	0.020%
39	18.857	2695	2698	2704	rVB8	12227	21358	0.15%	0.020%
40	19.016	2721	2725	2732	rBV2	111121	148744	1.01%	0.141%
41	19.086	2733	2737	2741	rBV	99492	132807	0.90%	0.126%
42	19.239	2759	2763	2768	rBV2	61473	84579	0.57%	0.080%
43	19.398	2786	2790	2793	rBV5	14326	22272	0.15%	0.021%
44	19.457	2793	2800	2813	rVV2	8142258	12398642	84.27%	11.768%
45	21.204	3093	3097	3103	rBV2	89584	121729	0.83%	0.116%
46	21.292	3106	3112	3127	rVV2	4717987	7015943	47.69%	6.659%
47	22.663	3341	3345	3352	rVB	135912	221785	1.51%	0.211%
48	23.380	3462	3467	3474	rVB	189893	351229	2.39%	0.333%
49	24.021	3565	3576	3595	rBV2	5703156	14712205	100.00%	13.964%
50	24.216	3599	3609	3625	rVB2	3303037	8376766	56.94%	7.951%
51	25.227	3774	3781	3789	rVB	236643	604132	4.11%	0.573%
52	26.421	3978	3984	3999	rVB3	210665	671114	4.56%	0.637%




Sum of corrected areas: 105354868

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030928.D
Acq On : 15 Apr 2024 00:11
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

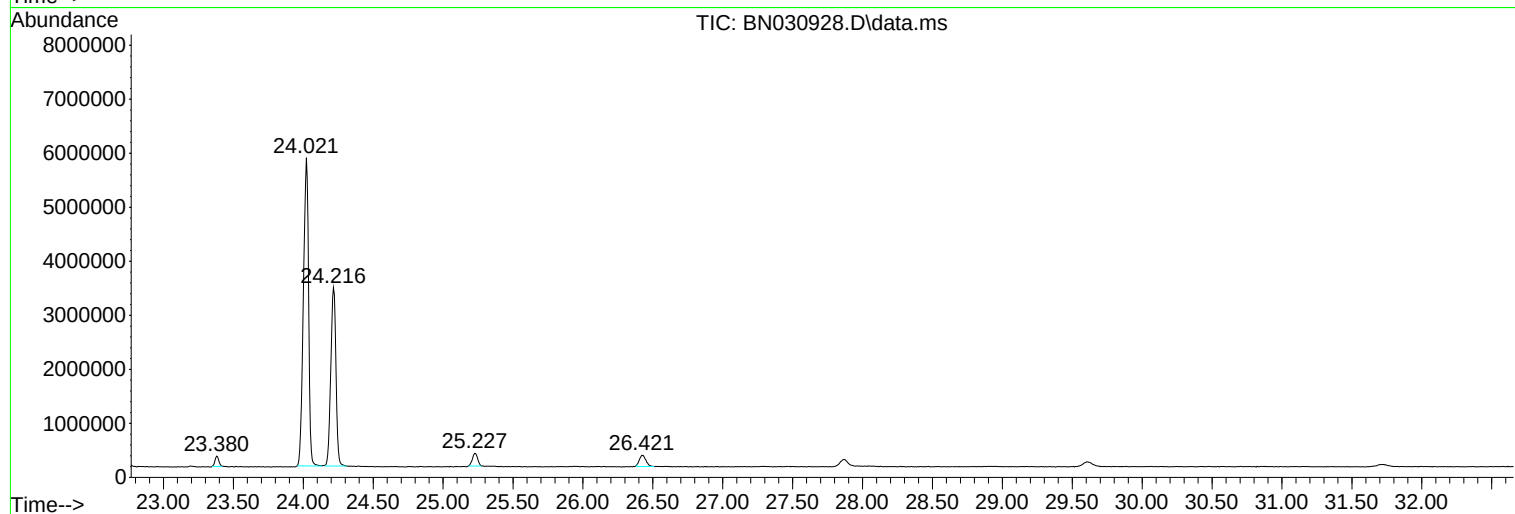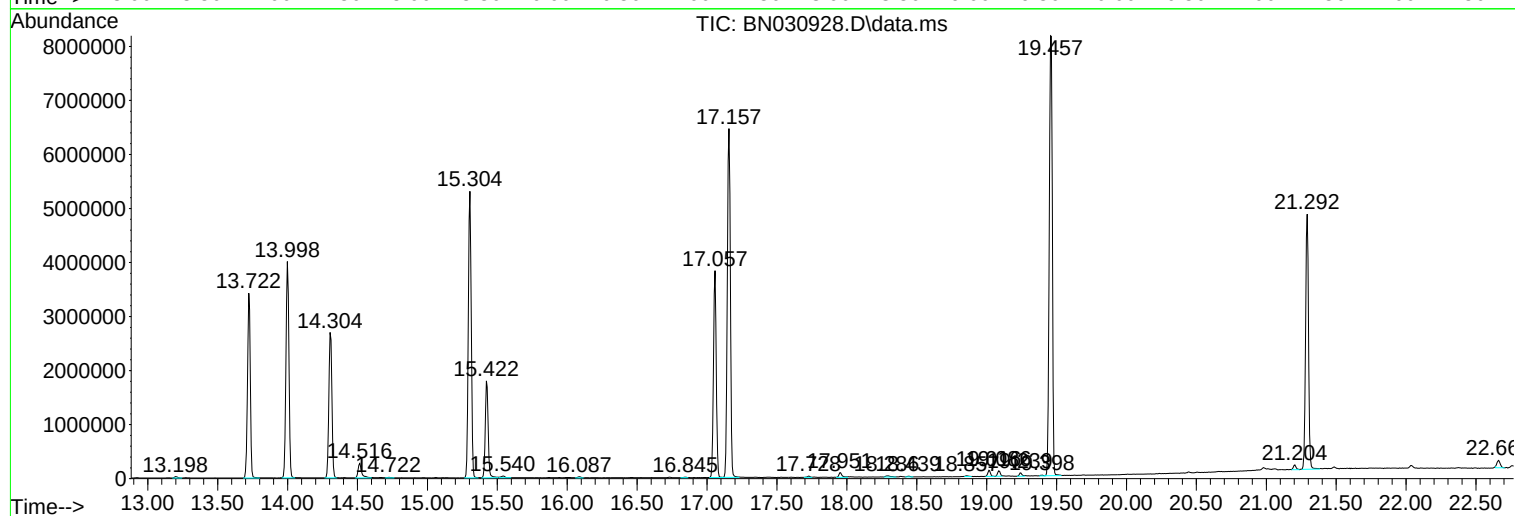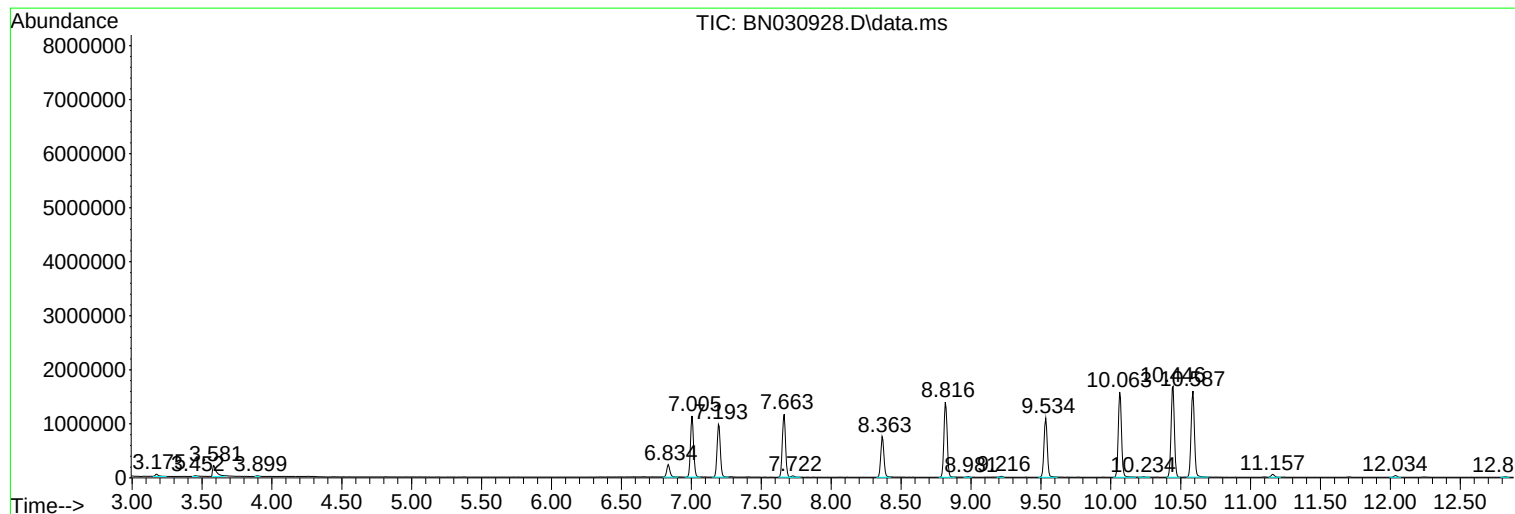

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030928.D
Acq On : 15 Apr 2024 00:11
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030928.D
Acq On : 15 Apr 2024 00:11
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc