

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030930.D
 Acq On : 15 Apr 2024 01:30
 Operator : MA/JU
 Sample : P2006-06
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030930.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	28	32	40	rBV	39349	58606	0.44%	0.059%
2	3.452	76	79	86	rBV5	9711	19673	0.15%	0.020%
3	3.587	100	102	114	rBV	168310	302340	2.26%	0.306%
4	3.899	151	155	161	rVB2	10055	17217	0.13%	0.017%
5	6.834	648	654	670	rVB	277736	451665	3.37%	0.458%
6	7.005	676	683	695	rBV	1181535	1853612	13.85%	1.879%
7	7.193	708	715	724	rBV	1084513	1750730	13.08%	1.774%
8	7.663	788	795	804	rBV	1029950	1642861	12.27%	1.665%
9	8.363	904	914	930	rBV	843143	1379772	10.31%	1.398%
10	8.816	984	991	1000	rBV	1412479	2365491	17.67%	2.397%
11	8.975	1015	1018	1024	rVB4	13502	21782	0.16%	0.022%
12	9.216	1054	1059	1066	rVB	12279	21284	0.16%	0.022%
13	9.534	1104	1113	1126	rBV	1156875	1859778	13.89%	1.885%
14	10.063	1195	1203	1221	rBV	1664288	2828027	21.13%	2.866%
15	10.446	1259	1268	1276	rBV	1517217	2523265	18.85%	2.557%
16	10.587	1282	1292	1306	rBV	1527296	2624000	19.60%	2.659%
17	12.034	1530	1538	1546	rBV2	32775	60806	0.45%	0.062%
18	12.922	1684	1689	1693	rBV3	9485	14059	0.11%	0.014%
19	13.204	1732	1737	1742	rBV3	14630	22982	0.17%	0.023%
20	13.722	1818	1825	1833	rBV	3512699	4947539	36.96%	5.014%
21	13.998	1861	1872	1880	rBV	4099092	6088206	45.48%	6.170%
22	14.304	1917	1924	1933	rBV	2380953	3576026	26.71%	3.624%
23	14.392	1936	1939	1946	rVB9	6999	14514	0.11%	0.015%
24	14.516	1953	1960	1973	rBV	307010	540147	4.04%	0.547%
25	14.722	1991	1995	2002	rVB9	11617	18630	0.14%	0.019%
26	15.304	2087	2094	2106	rBV	5556388	7928660	59.23%	8.036%
27	15.422	2108	2114	2126	rVV	1727607	2362018	17.65%	2.394%
28	15.539	2129	2134	2142	rVB	28677	52655	0.39%	0.053%
29	15.992	2205	2211	2221	rBV	6861	18251	0.14%	0.018%
30	16.087	2223	2227	2233	rVB3	22346	32813	0.25%	0.033%
31	16.463	2288	2291	2296	rBV6	9954	13630	0.10%	0.014%
32	16.734	2333	2337	2341	rVB5	11338	14873	0.11%	0.015%
33	17.057	2385	2392	2402	rBV	3268750	4617149	34.49%	4.679%
34	17.157	2402	2409	2420	rBV	6520099	9410868	70.30%	9.538%
35	17.728	2502	2506	2510	rVB5	24873	30759	0.23%	0.031%
36	17.951	2539	2544	2553	rBV	184560	290205	2.17%	0.294%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030930.D
 Acq On : 15 Apr 2024 01:30
 Operator : MA/JU
 Sample : P2006-06
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	18.286	2597	2601	2610	rBV4	25916	57401	0.43%	0.058%
38	18.386	2615	2618	2621	rBV4	14110	16302	0.12%	0.017%
39	18.439	2623	2627	2632	rVB4	21615	32436	0.24%	0.033%
40	19.016	2720	2725	2731	rBV2	113582	155972	1.17%	0.158%
41	19.086	2732	2737	2741	rBV	103999	148300	1.11%	0.150%
42	19.239	2760	2763	2768	rBV	82251	105067	0.78%	0.106%
43	19.392	2786	2789	2793	rBV4	20725	23636	0.18%	0.024%
44	19.457	2794	2800	2807	rBV	7940455	11893740	88.85%	12.054%
45	19.692	2837	2840	2843	rBV	14479	19178	0.14%	0.019%
46	19.728	2844	2846	2850	rVB5	16718	15928	0.12%	0.016%
47	20.445	2965	2968	2972	rBV2	32507	36354	0.27%	0.037%
48	20.980	3055	3059	3070	rBV2	136687	283542	2.12%	0.287%
49	21.292	3106	3112	3121	rBV2	4075962	5945186	44.41%	6.025%
50	23.380	3463	3467	3474	rVB2	104610	189217	1.41%	0.192%
51	24.021	3565	3576	3590	rBV2	5268438	13385961	100.00%	13.567%
52	24.216	3599	3609	3624	rVB	2614010	6585363	49.20%	6.674%




Sum of corrected areas: 98668476

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030930.D
Acq On : 15 Apr 2024 01:30
Operator : MA/JU
Sample : P2006-06
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

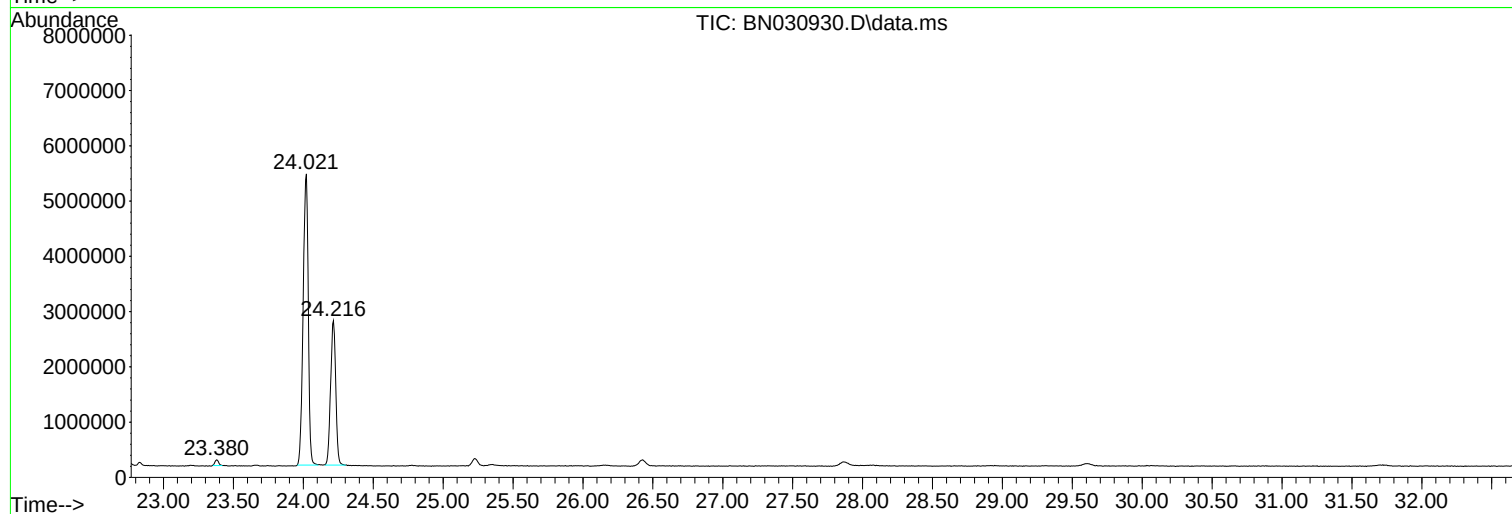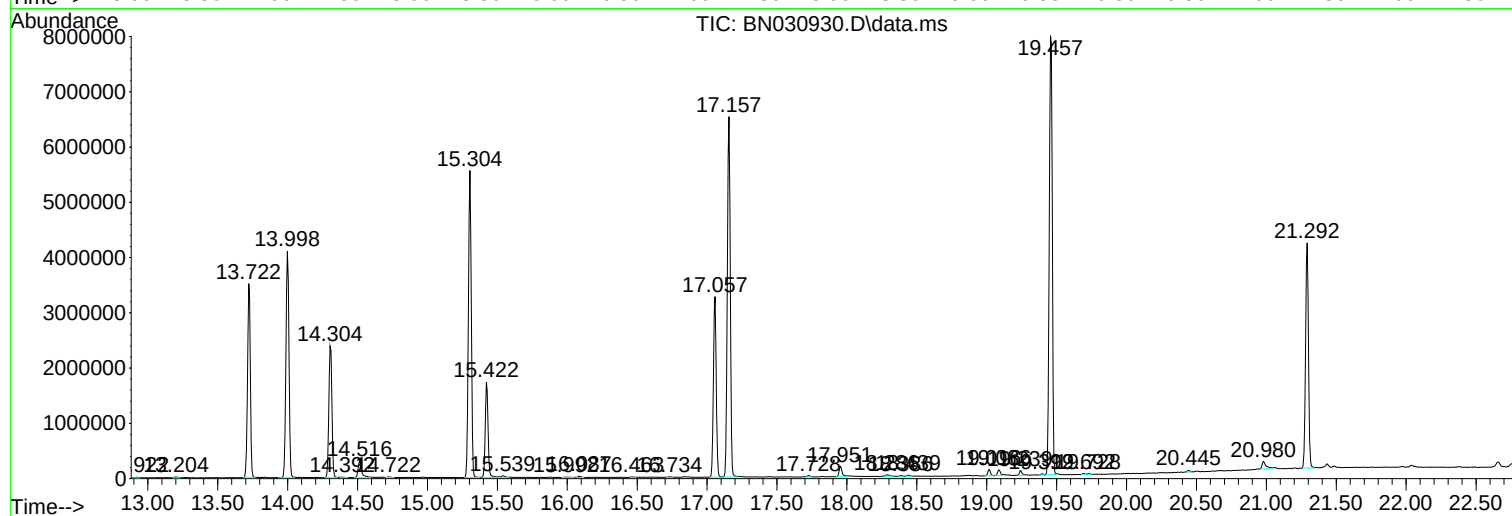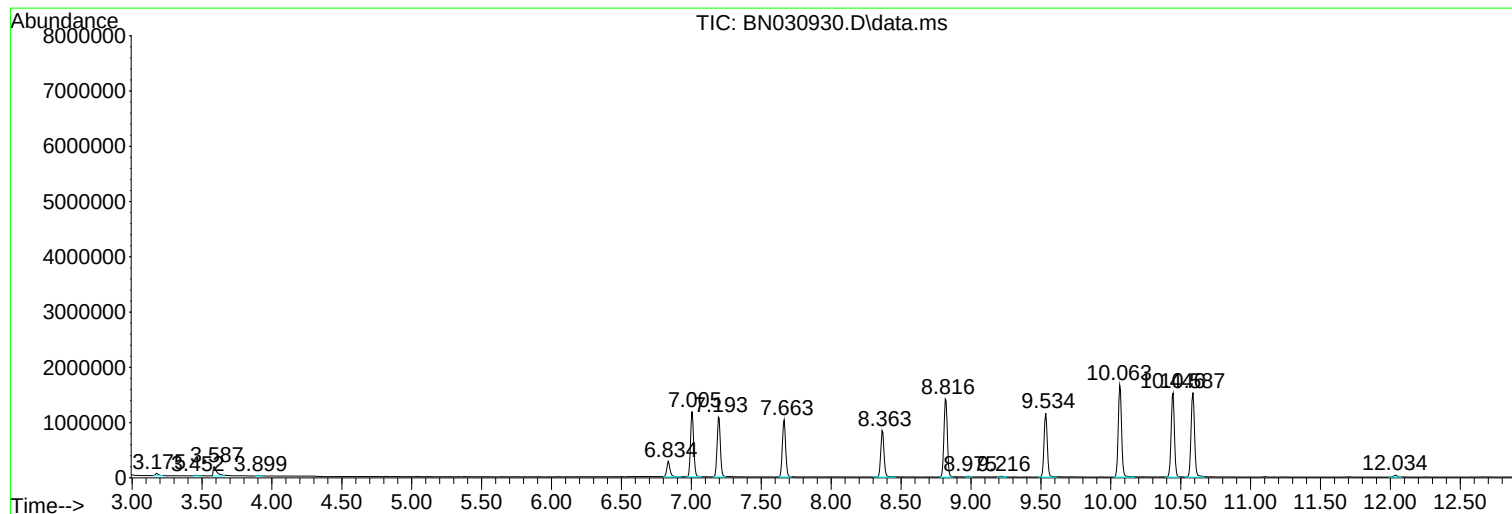

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030930.D
Acq On : 15 Apr 2024 01:30
Operator : MA/JU
Sample : P2006-06
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030930.D
Acq On : 15 Apr 2024 01:30
Operator : MA/JU
Sample : P2006-06
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R65

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------