




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
Data File : BN019450.D
Acq On : 14 Apr 2022 10:51
Operator : CG/JU
Sample : PB143958BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK958

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:02:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 14:35:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/15/2022

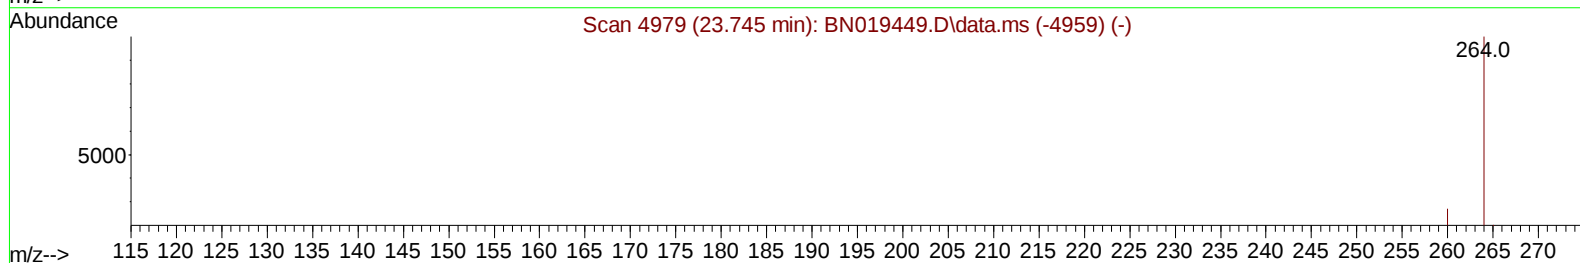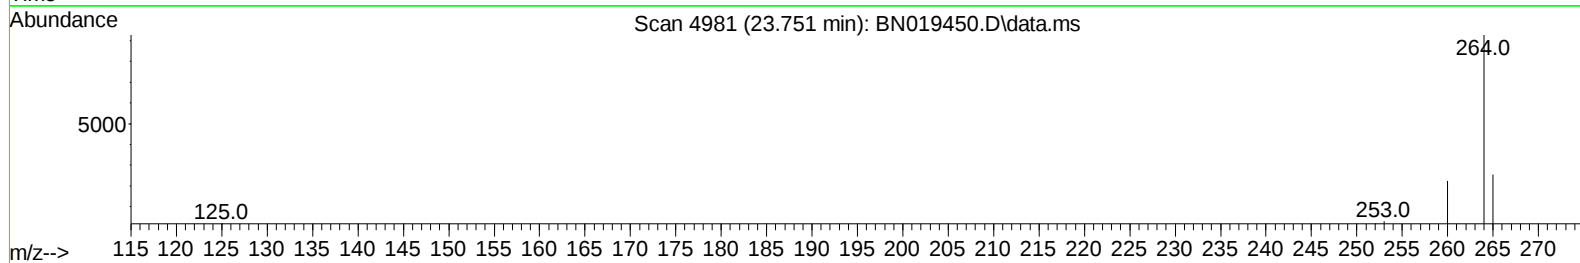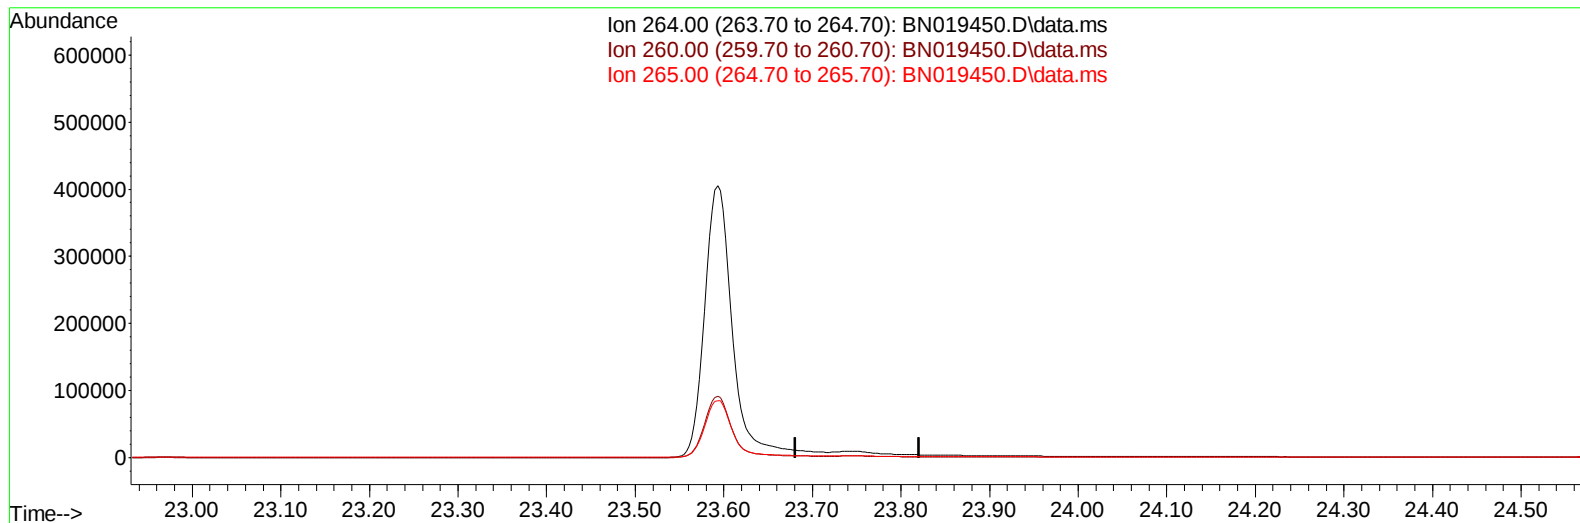

TIC: BN019450.D\data.ms

(23) Perylene-d12 (I)

23.751min (-23.751) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
 Data File : BN019450.D
 Acq On : 14 Apr 2022 10:51
 Operator : CG/JU
 Sample : PB143958BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK958

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:02:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/15/2022

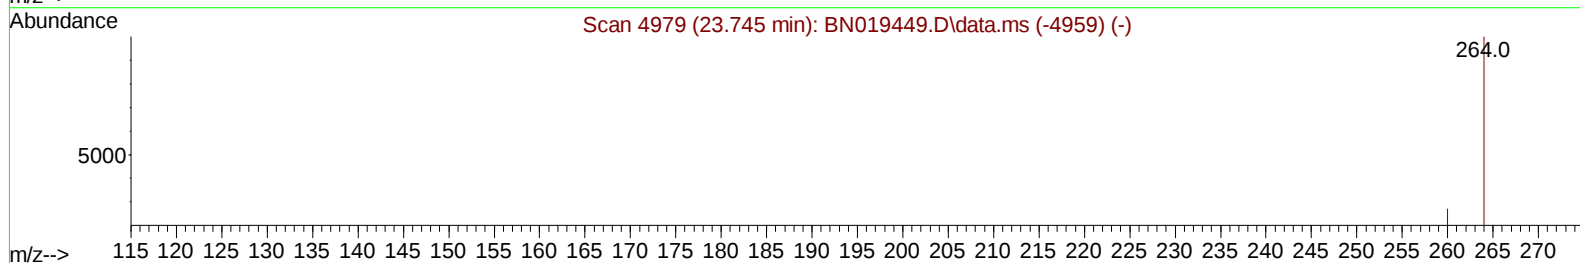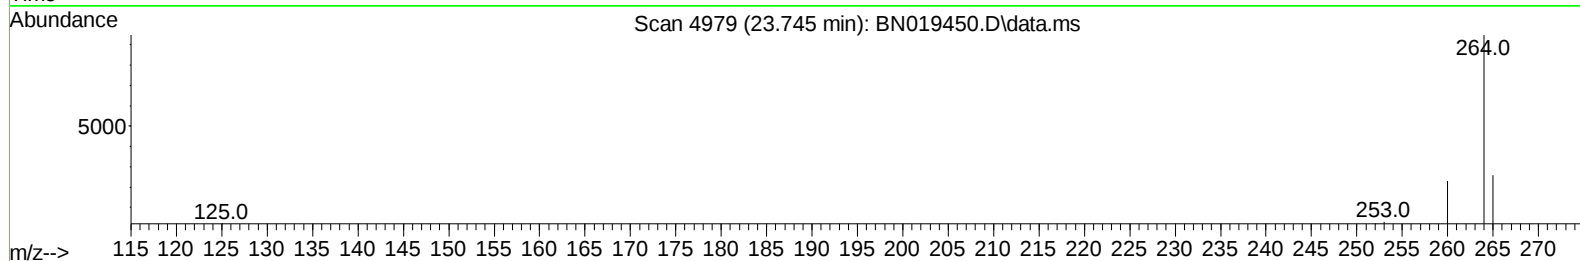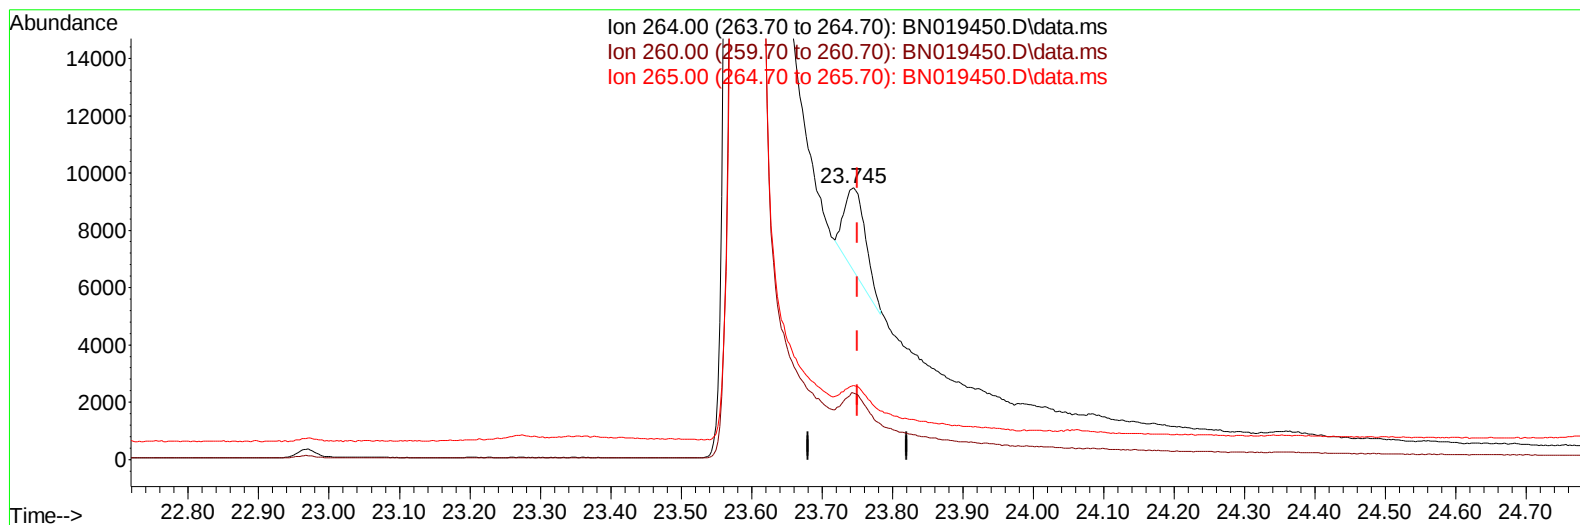

TIC: BN019450.D\data.ms

(23) Perylene-d12 (I)

23.745min (-0.006) 0.40 ng/ul m

response 6010

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.39
265.00	45.70	27.29#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
 Data File : BN019450.D
 Acq On : 14 Apr 2022 10:51
 Operator : CG/JU
 Sample : PB143958BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK958

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/15/2022

Quant Time: Apr 15 04:02:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.814	152		4855	0.400	ng/ul	0.00
4) Naphthalene-d8	10.613	136		14845	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.461	164		9065	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.201	188		18528	0.400	ng/ul	0.00
17) Chrysene-d12	21.404	240		10291	0.400	ng/ul	0.00
23) Perylene-d12	23.745	264		6010m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.173	96		33804	5.411	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.219	152		6767	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.231	212		15102	0.396	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
Data File : BN019450.D
Acq On : 14 Apr 2022 10:51
Operator : CG/JU
Sample : PB143958BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK958

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:02:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 14:35:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/15/2022

