




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
 Data File : BN019451.D
 Acq On : 14 Apr 2022 11:41
 Operator : CG/JU
 Sample : N2320-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:49:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/15/2022

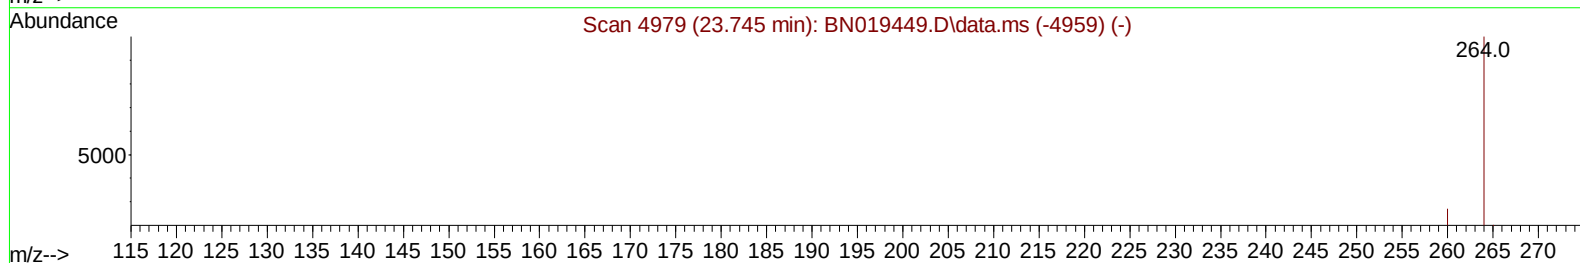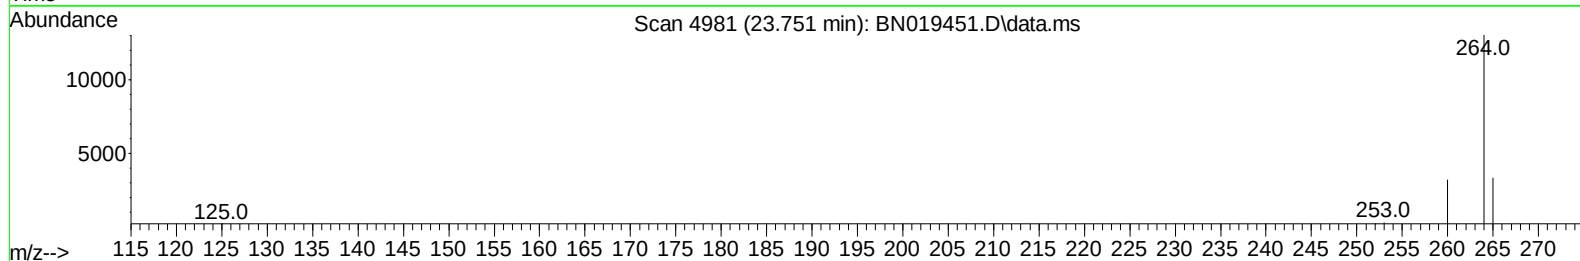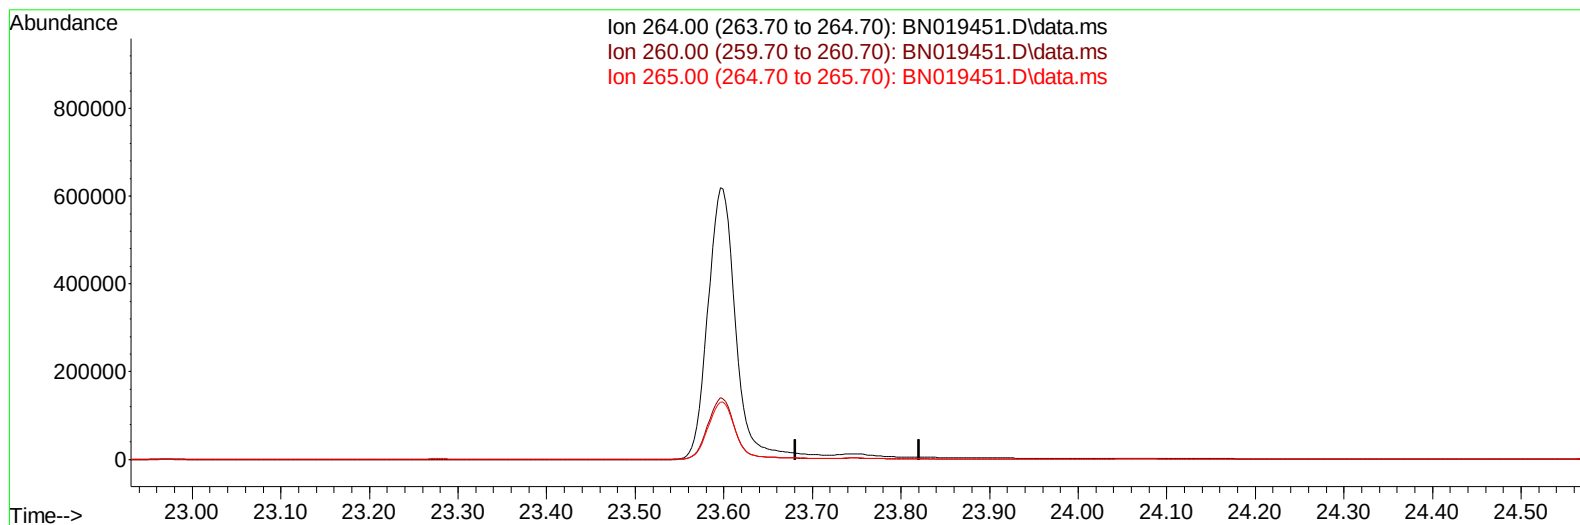

TIC: BN019451.D\data.ms

(23) Perylene-d12 (I)

23.751min (-23.751) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
Data File : BN019451.D
Acq On : 14 Apr 2022 11:41
Operator : CG/JU
Sample : N2320-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:49:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 14:35:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/15/2022

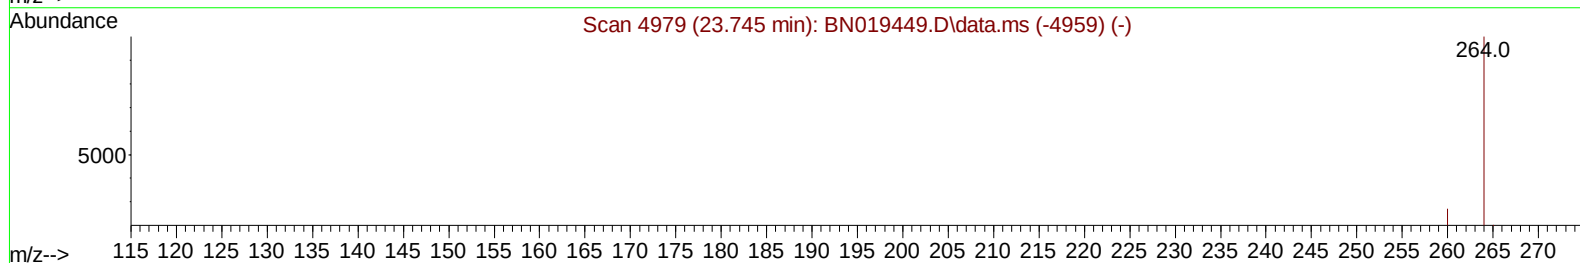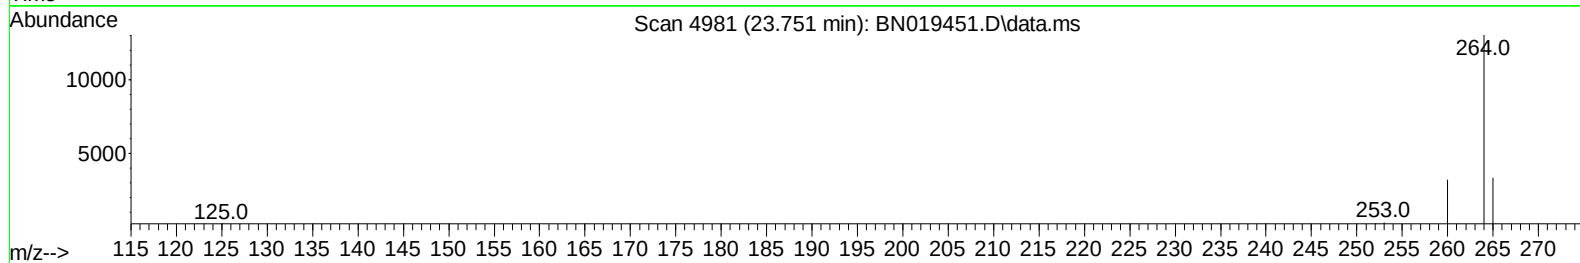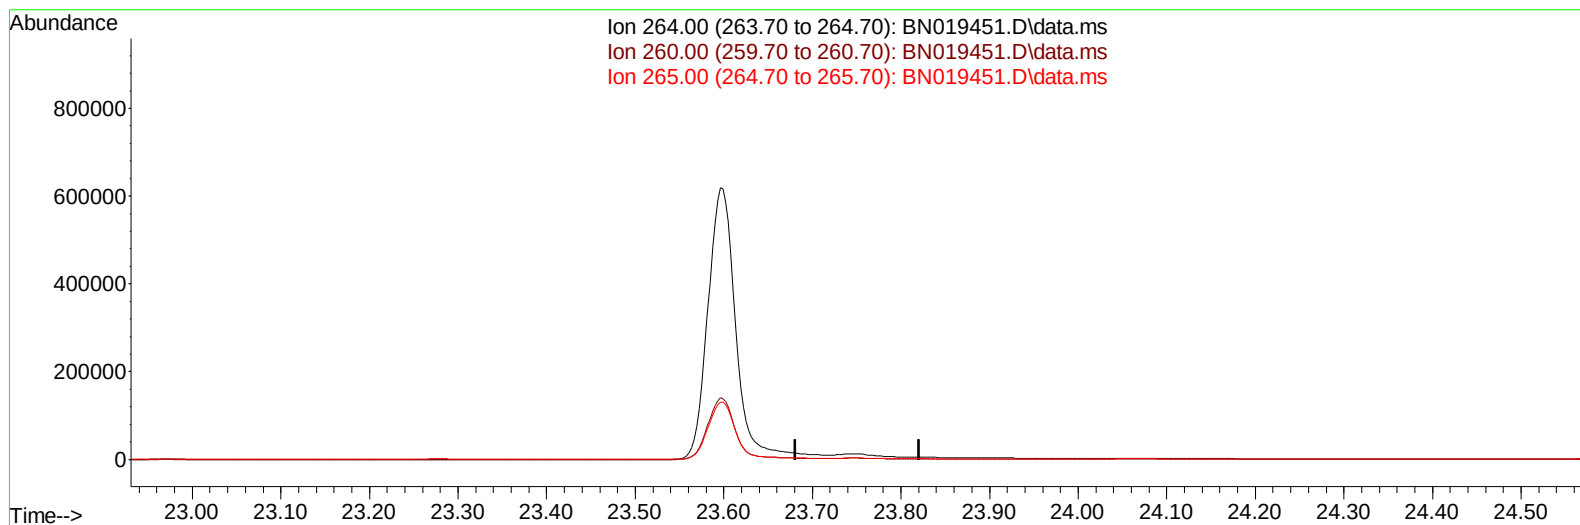

TIC: BN019451.D\data.ms

(23) Perylene-d12 (I)

23.751min (-23.751) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
 Data File : BN019451.D
 Acq On : 14 Apr 2022 11:41
 Operator : CG/JU
 Sample : N2320-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:49:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/15/2022

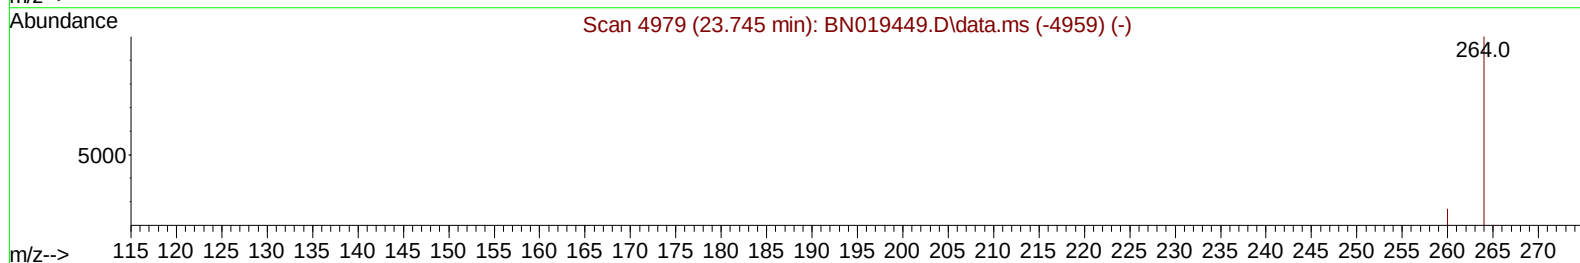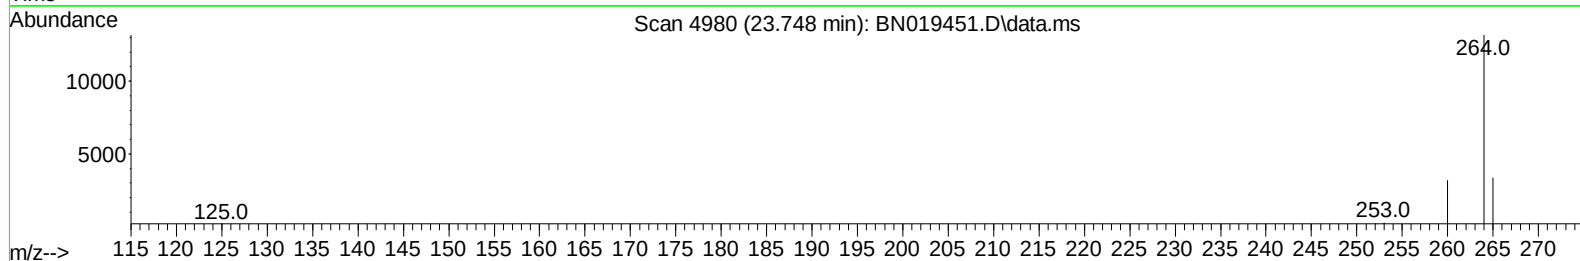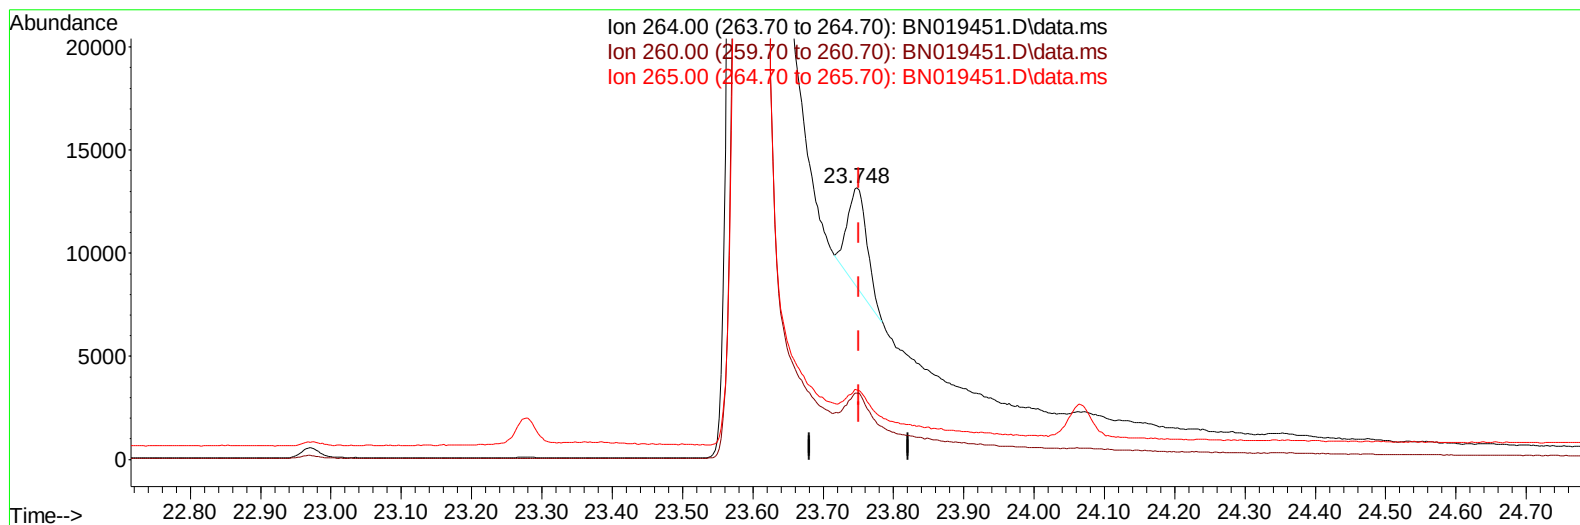

TIC: BN019451.D\data.ms

(23) Perylene-d12 (I)

23.748min (-0.003) 0.40 ng/ul m

response 9087

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.32
265.00	45.70	25.51#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
 Data File : BN019451.D
 Acq On : 14 Apr 2022 11:41
 Operator : CG/JU
 Sample : N2320-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2P4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/15/2022

Quant Time: Apr 15 04:49:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.810	152		5835	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.613	136		17902	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.457	164		11646	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.201	188		23517	0.400	ng/ul	0.00
17) Chrysene-d12	21.401	240		14220	0.400	ng/ul	0.00
23) Perylene-d12	23.748	264		9087m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.173	96		28441	3.788	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.213	152		9336	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.231	212		24152	0.459	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
Data File : BN019451.D
Acq On : 14 Apr 2022 11:41
Operator : CG/JU
Sample : N2320-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB2P4

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:49:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 14:35:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/15/2022

