




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
 Data File : BN019453.D
 Acq On : 14 Apr 2022 16:57
 Operator : CG/JU
 Sample : SP5861
 Misc : SFAM SIM SURROGATE
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP5861

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:02:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/15/2022

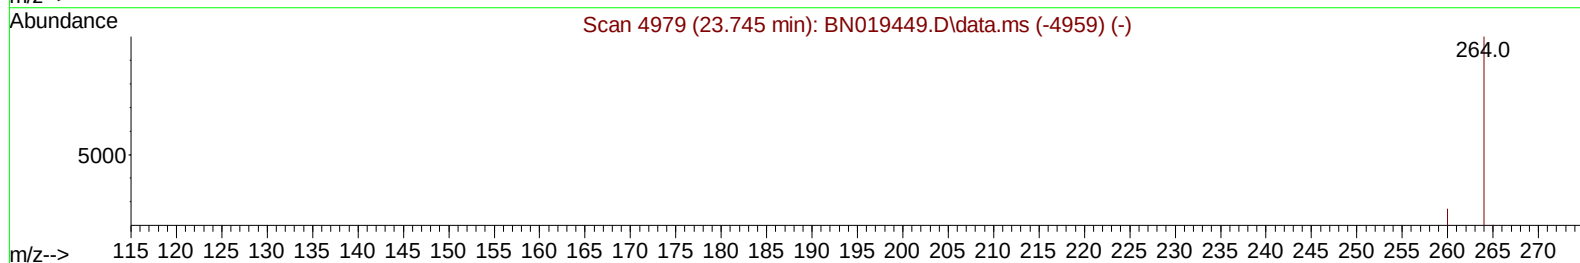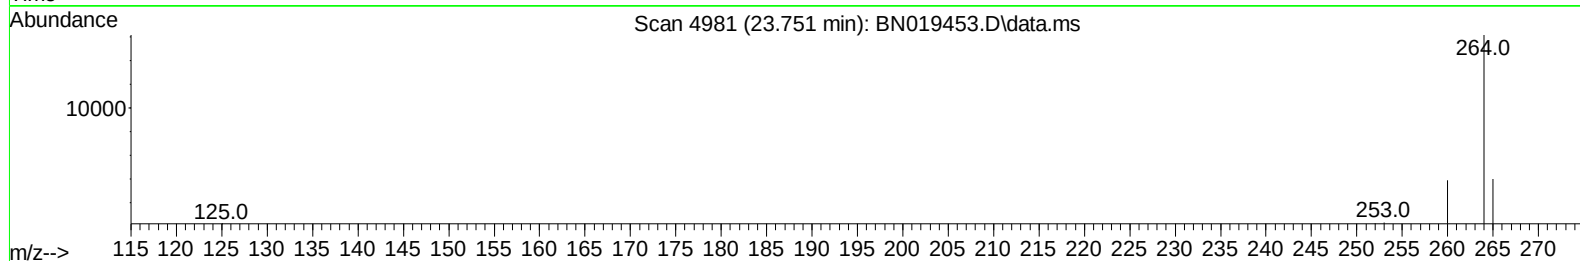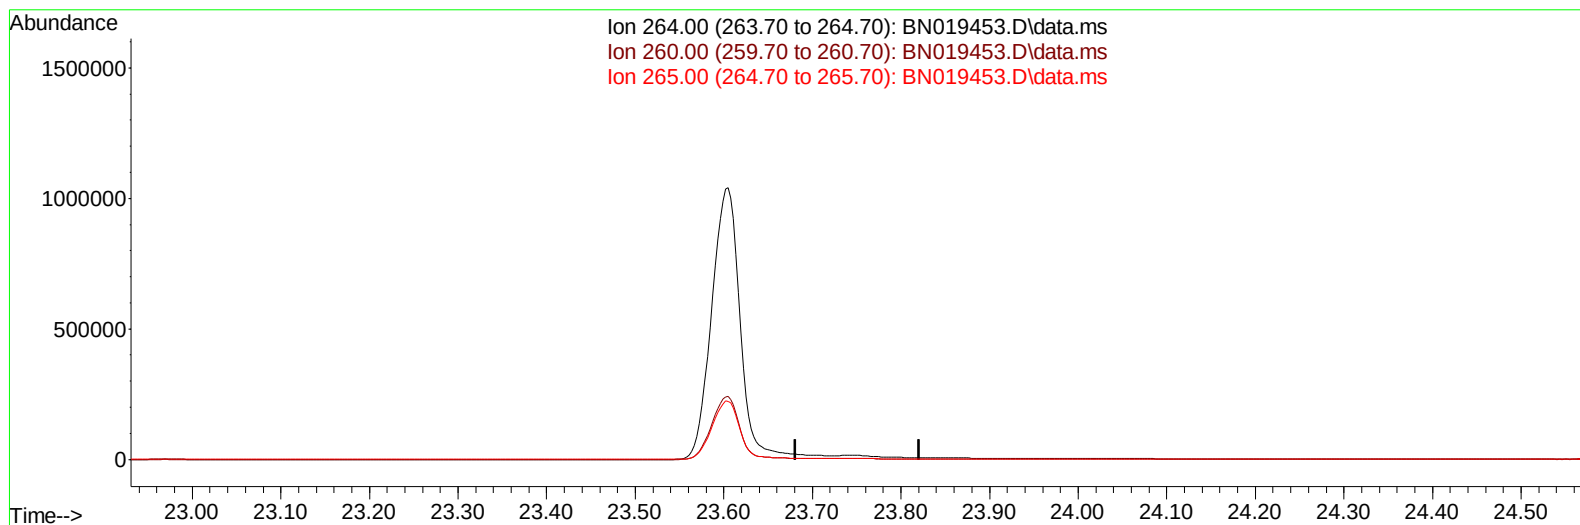

TIC: BN019453.D\data.ms

(23) Perylene-d12 (I)

23.751min (-23.751) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
 Data File : BN019453.D
 Acq On : 14 Apr 2022 16:57
 Operator : CG/JU
 Sample : SP5861
 Misc : SFAM SIM SURROGATE
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP5861

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:02:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/15/2022

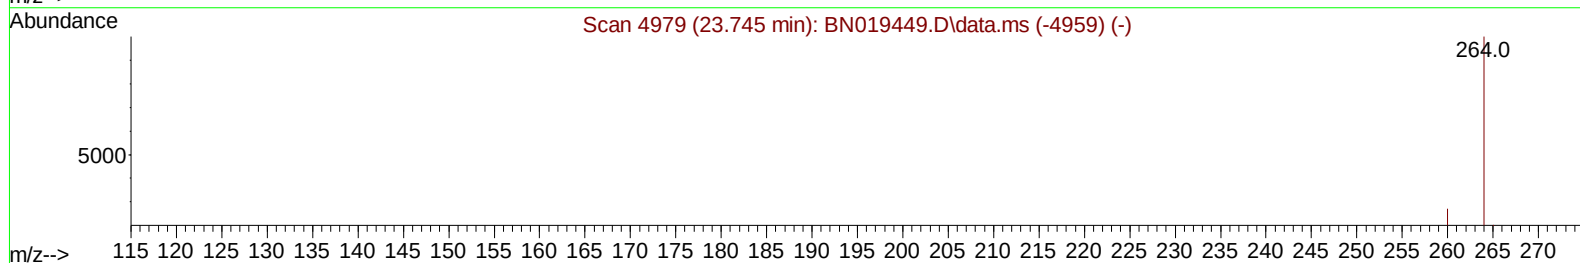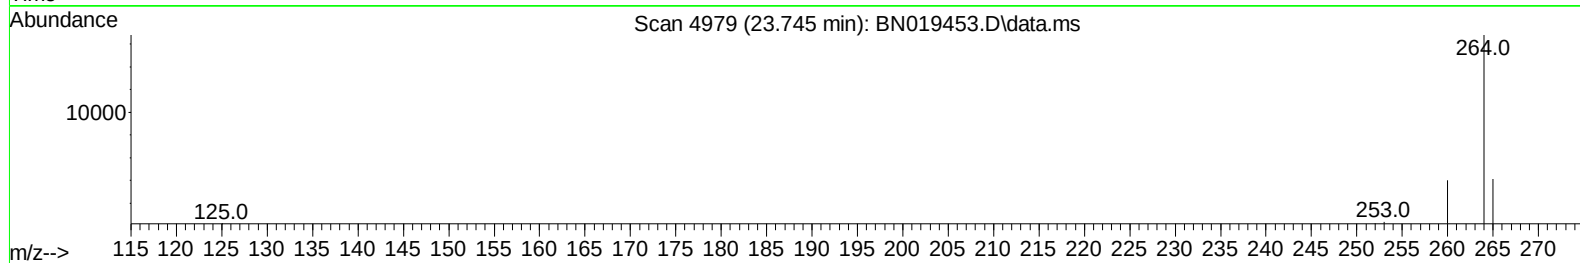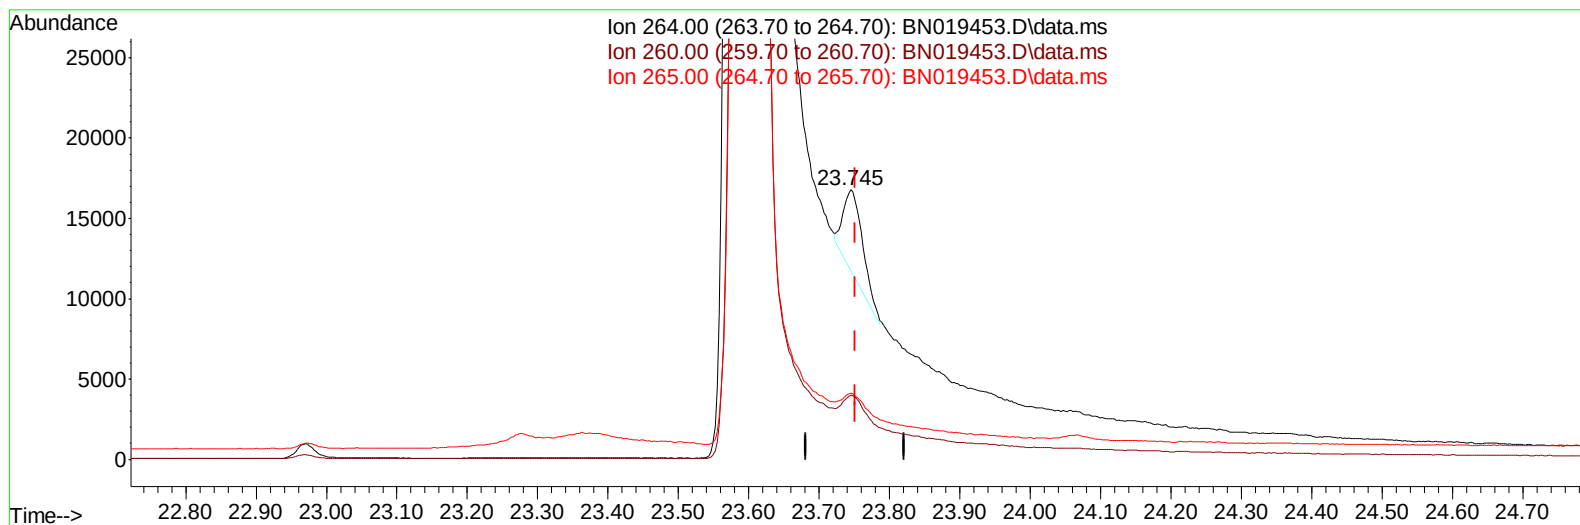

TIC: BN019453.D\data.ms

(23) Perylene-d12 (I)

23.745min (-0.006) 0.40 ng/ul m

response 9381

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	23.86
265.00	45.70	24.57#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
 Data File : BN019453.D
 Acq On : 14 Apr 2022 16:57
 Operator : CG/JU
 Sample : SP5861
 Misc : SFAM SIM SURROGATE
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP5861

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/15/2022

Quant Time: Apr 15 04:02:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.806	152		5720	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.607	136		17961	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.457	164		11866	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.197	188		24279	0.400	ng/ul	0.00
17) Chrysene-d12	21.401	240		14248	0.400	ng/ul	0.00
23) Perylene-d12	23.745	264		9381m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.165	96		102692	13.951	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.208	152		22360	0.880	ng/ul	-0.01
18) Fluoranthene-d10	19.231	212		47856	0.907	ng/ul	0.00

Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041422\
Data File : BN019453.D
Acq On : 14 Apr 2022 16:57
Operator : CG/JU
Sample : SP5861
Misc : SFAM SIM SURROGATE
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP5861

Manual IntegrationsAPPROVED

Quant Time: Apr 15 04:02:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 14:35:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/15/2022

