

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
 Data File : BN014298.D
 Acq On : 15 Apr 2021 23:59
 Operator : CG/JU
 Sample : M2031-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG531

Quant Time: Apr 16 01:32:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 15 15:18:04 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	136735	20.00	ng/ul	0.00
20) Naphthalene-d8	10.48	136	549098	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.33	164	331022	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.07	188	688302	20.00	ng/ul	0.00
79) Chrysene-d12	21.27	240	692766	20.00	ng/ul	0.00
88) Perylene-d12	23.50	264	770607	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	19547	5.44	ng/uL	0.00
4) Pyridine-d5	3.61	84	218	0.02	ng/ul	-0.01
7) Phenol-d5	6.86	99	94764	8.29	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.03	67	196692	28.74	ng/ul	0.00
11) 2-Chlorophenol-d4	7.23	132	238624	26.54	ng/ul	0.00
15) 4-Methylphenol-d8	8.39	113	152382	17.59	ng/ul	0.00
21) Nitrobenzene-d5	8.85	128	116709	29.41	ng/ul	0.00
24) 2-Nitrophenol-d4	9.56	143	114591	29.49	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.09	165	235980	28.19	ng/ul	0.00
31) 4-Chloroaniline-d4	10.61	131	9827	0.79	ng/ul	0.00
46) Dimethylphthalate-d6	13.75	166	780624	32.55	ng/ul	0.00
49) Acenaphthylene-d8	14.02	160	968327	33.56	ng/ul	0.00
54) 4-Nitrophenol-d4	14.52	143	29608	6.37	ng/ul	0.00
60) Fluorene-d10	15.33	176	709694	33.48	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.44	200	91725	24.90	ng/ul	0.00
73) Anthracene-d10	17.17	188	1248587	38.87	ng/ul	0.00
81) Pyrene-d10	19.47	212	1461182	43.45	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.36	264	1682088	41.15	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.79	163	84648	3.400	ng/ul	Ovalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
Data File : BN014298.D
Acq On : 15 Apr 2021 23:59
Operator : CG/JU
Sample : M2031-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG531

Quant Time: Apr 16 01:32:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 15 15:18:04 2021
Response via : Initial Calibration

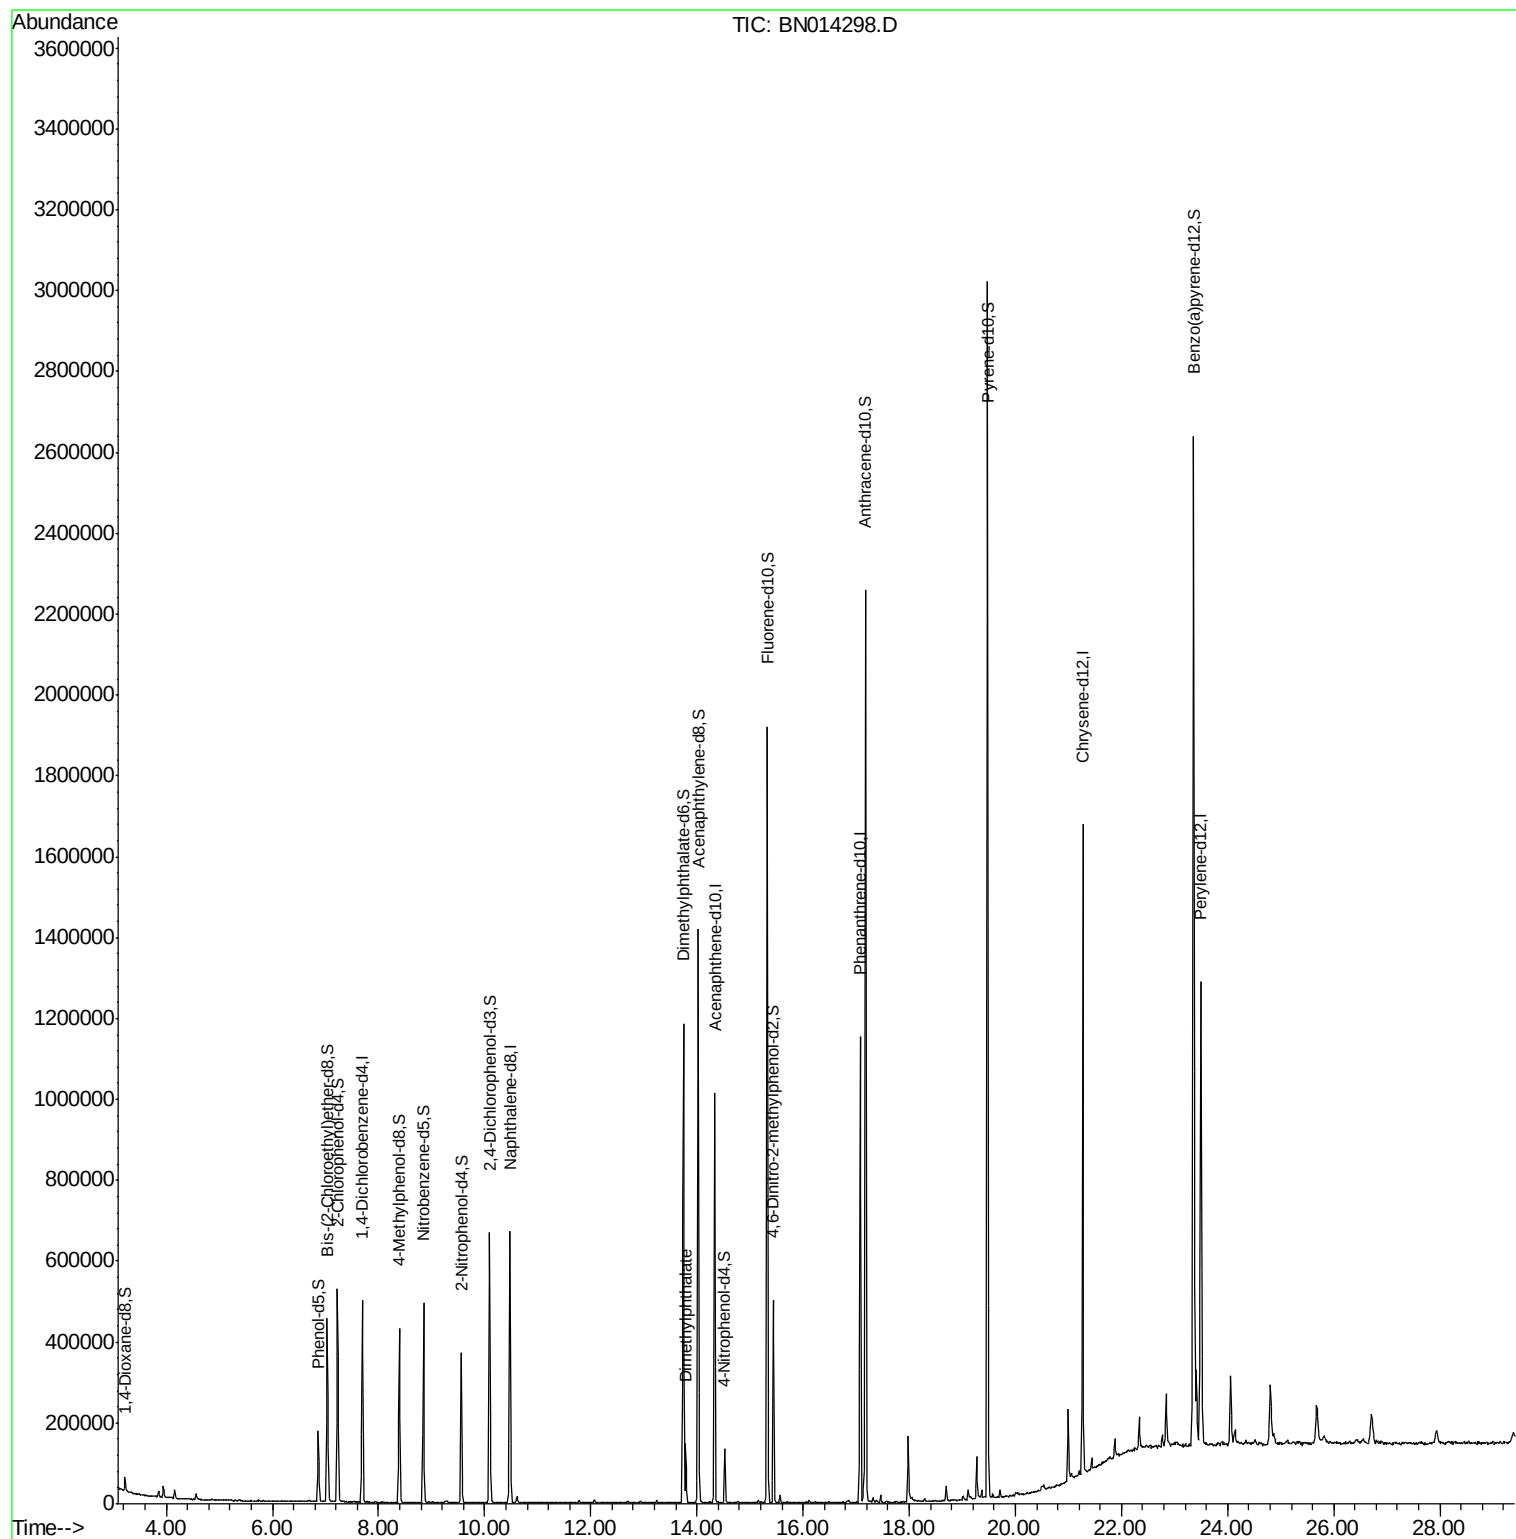

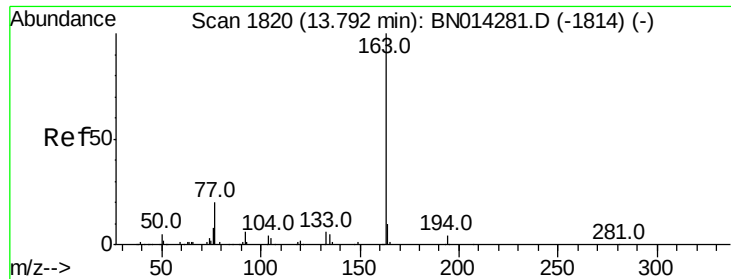

#47

Dimethylphthalate

Concen: 3.400 ng/ul

RT: 13.79 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BN014298.D

Acq: 15 Apr 2021 23:59

Instrument :

BNA_N

ClientSampleId :

BG531


Tot Ion:163 Resp: 84648

Ion Ratio Lower Upper

163 100

194 3.5 3.3 4.9

164 10.0 7.8 11.8

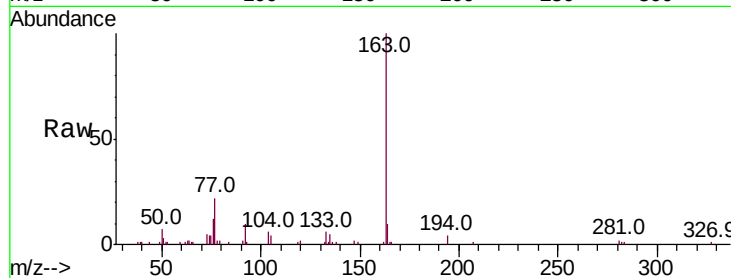

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

