

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041521\
 Data File : BN014288.D
 Acq On : 15 Apr 2021 17:25
 Operator : CG/JU
 Sample : M2031-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG539

Quant Time: Apr 16 01:39:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 15 15:18:04 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	146522	20.00	ng/ul	0.00
20) Naphthalene-d8	10.48	136	577358	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.33	164	349002	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.07	188	713992	20.00	ng/ul	0.00
79) Chrysene-d12	21.27	240	725801	20.00	ng/ul	0.00
88) Perylene-d12	23.50	264	769808	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	23226	6.03	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.86	99	98248	8.02	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.03	67	223467	30.47	ng/ul	0.00
11) 2-Chlorophenol-d4	7.23	132	266927	27.70	ng/ul	0.00
15) 4-Methylphenol-d8	8.39	113	166617	17.94	ng/ul	0.00
21) Nitrobenzene-d5	8.85	128	138034	33.08	ng/ul	0.00
24) 2-Nitrophenol-d4	9.56	143	139006	34.02	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.09	165	273604	31.09	ng/ul	0.00
31) 4-Chloroaniline-d4	10.61	131	16566	1.27	ng/ul	0.00
46) Dimethylphthalate-d6	13.75	166	910346	36.01	ng/ul	0.00
49) Acenaphthylene-d8	14.02	160	1149078	37.78	ng/ul	0.00
54) 4-Nitrophenol-d4	14.52	143	29717	6.06	ng/ul	0.00
60) Fluorene-d10	15.33	176	846787	37.89	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.44	200	105786	27.69	ng/ul	0.00
73) Anthracene-d10	17.17	188	1376095	41.29	ng/ul	0.00
81) Pyrene-d10	19.47	212	1610278	45.70	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.36	264	1708088	41.83	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.79	163	92010	3.505	ng/ul	Ovalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
Data File : BN014288.D
Acq On : 15 Apr 2021 17:25
Operator : CG/JU
Sample : M2031-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG539

Quant Time: Apr 16 01:39:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 15 15:18:04 2021
Response via : Initial Calibration

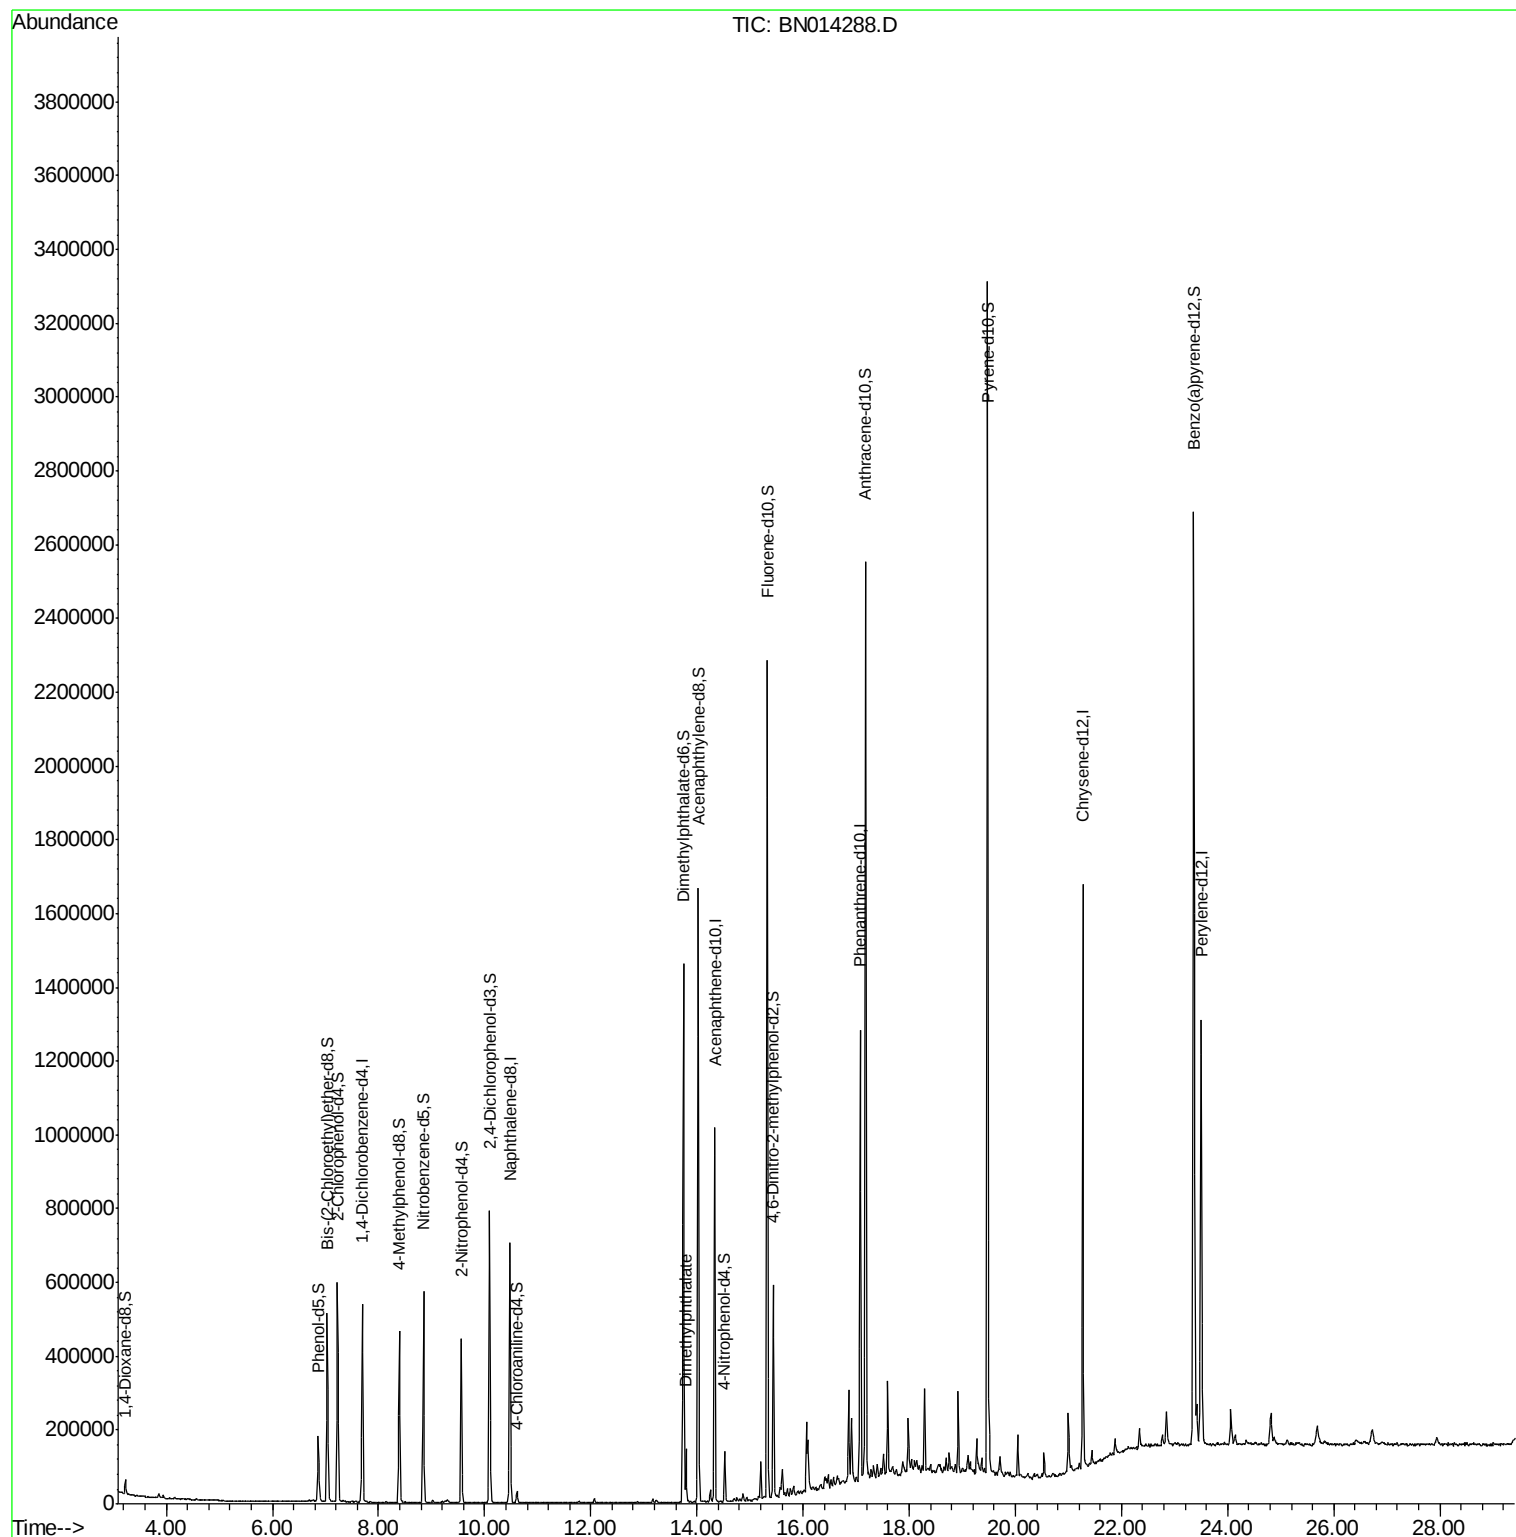


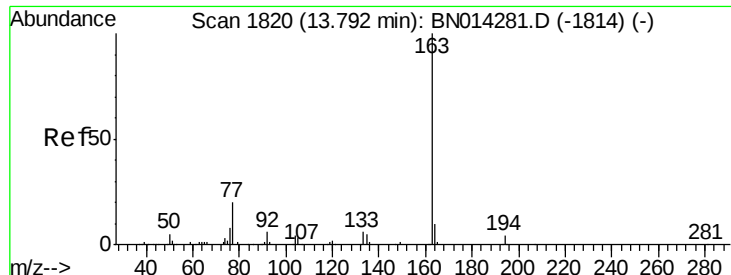

#47
 Dimethylphthalate
 Concen: 3.505 ng/ul
 RT: 13.79 min Scan# 1820
 Delta R.T. 0.00 min
 Lab File: BN014288.D
 Acq: 15 Apr 2021 17:25

Instrument :
 BNA_N
 ClientSampleId :
 BG539

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.3	4.9
164	9.0	7.8	11.8

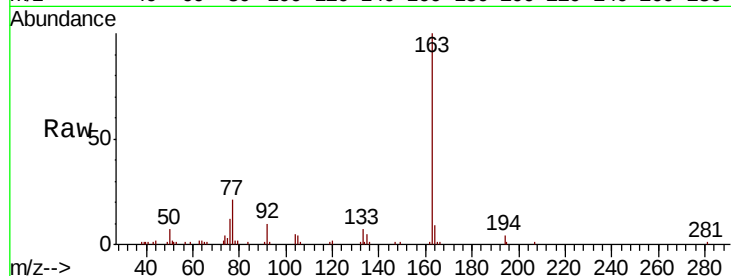

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

