

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
 Data File : BN014293.D
 Acq On : 15 Apr 2021 20:25
 Operator : CG/JU
 Sample : M2031-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG536

Quant Time: Apr 16 01:57:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 15 15:18:04 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	141034	20.00	ng/ul	0.00
20) Naphthalene-d8	10.48	136	559910	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.33	164	329674	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.07	188	658879	20.00	ng/ul	0.00
79) Chrysene-d12	21.27	240	673733	20.00	ng/ul	0.00
88) Perylene-d12	23.50	264	713034	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	18484	4.99	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.86	99	79743	6.76	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.03	67	185745	26.31	ng/ul	0.00
11) 2-Chlorophenol-d4	7.23	132	222203	23.96	ng/ul	0.00
15) 4-Methylphenol-d8	8.39	113	134913	15.10	ng/ul	0.00
21) Nitrobenzene-d5	8.85	128	110518	27.31	ng/ul	0.00
24) 2-Nitrophenol-d4	9.56	143	109568	27.65	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.09	165	216541	25.37	ng/ul	0.00
31) 4-Chloroaniline-d4	10.61	131	9233	0.73	ng/ul	0.00
46) Dimethylphthalate-d6	13.75	166	718880	30.10	ng/ul	0.00
49) Acenaphthylene-d8	14.02	160	879570	30.61	ng/ul	0.00
54) 4-Nitrophenol-d4	14.52	143	20850	4.50	ng/ul	0.00
60) Fluorene-d10	15.33	176	634103	30.03	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.44	200	72702	20.62	ng/ul	0.00
73) Anthracene-d10	17.17	188	1033788	33.62	ng/ul	0.00
81) Pyrene-d10	19.47	212	1192095	36.45	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.36	264	1304801	34.49	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.79	163	64642	2.607	ng/ul	Ovalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
Data File : BN014293.D
Acq On : 15 Apr 2021 20:25
Operator : CG/JU
Sample : M2031-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG536

Quant Time: Apr 16 01:57:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 15 15:18:04 2021
Response via : Initial Calibration

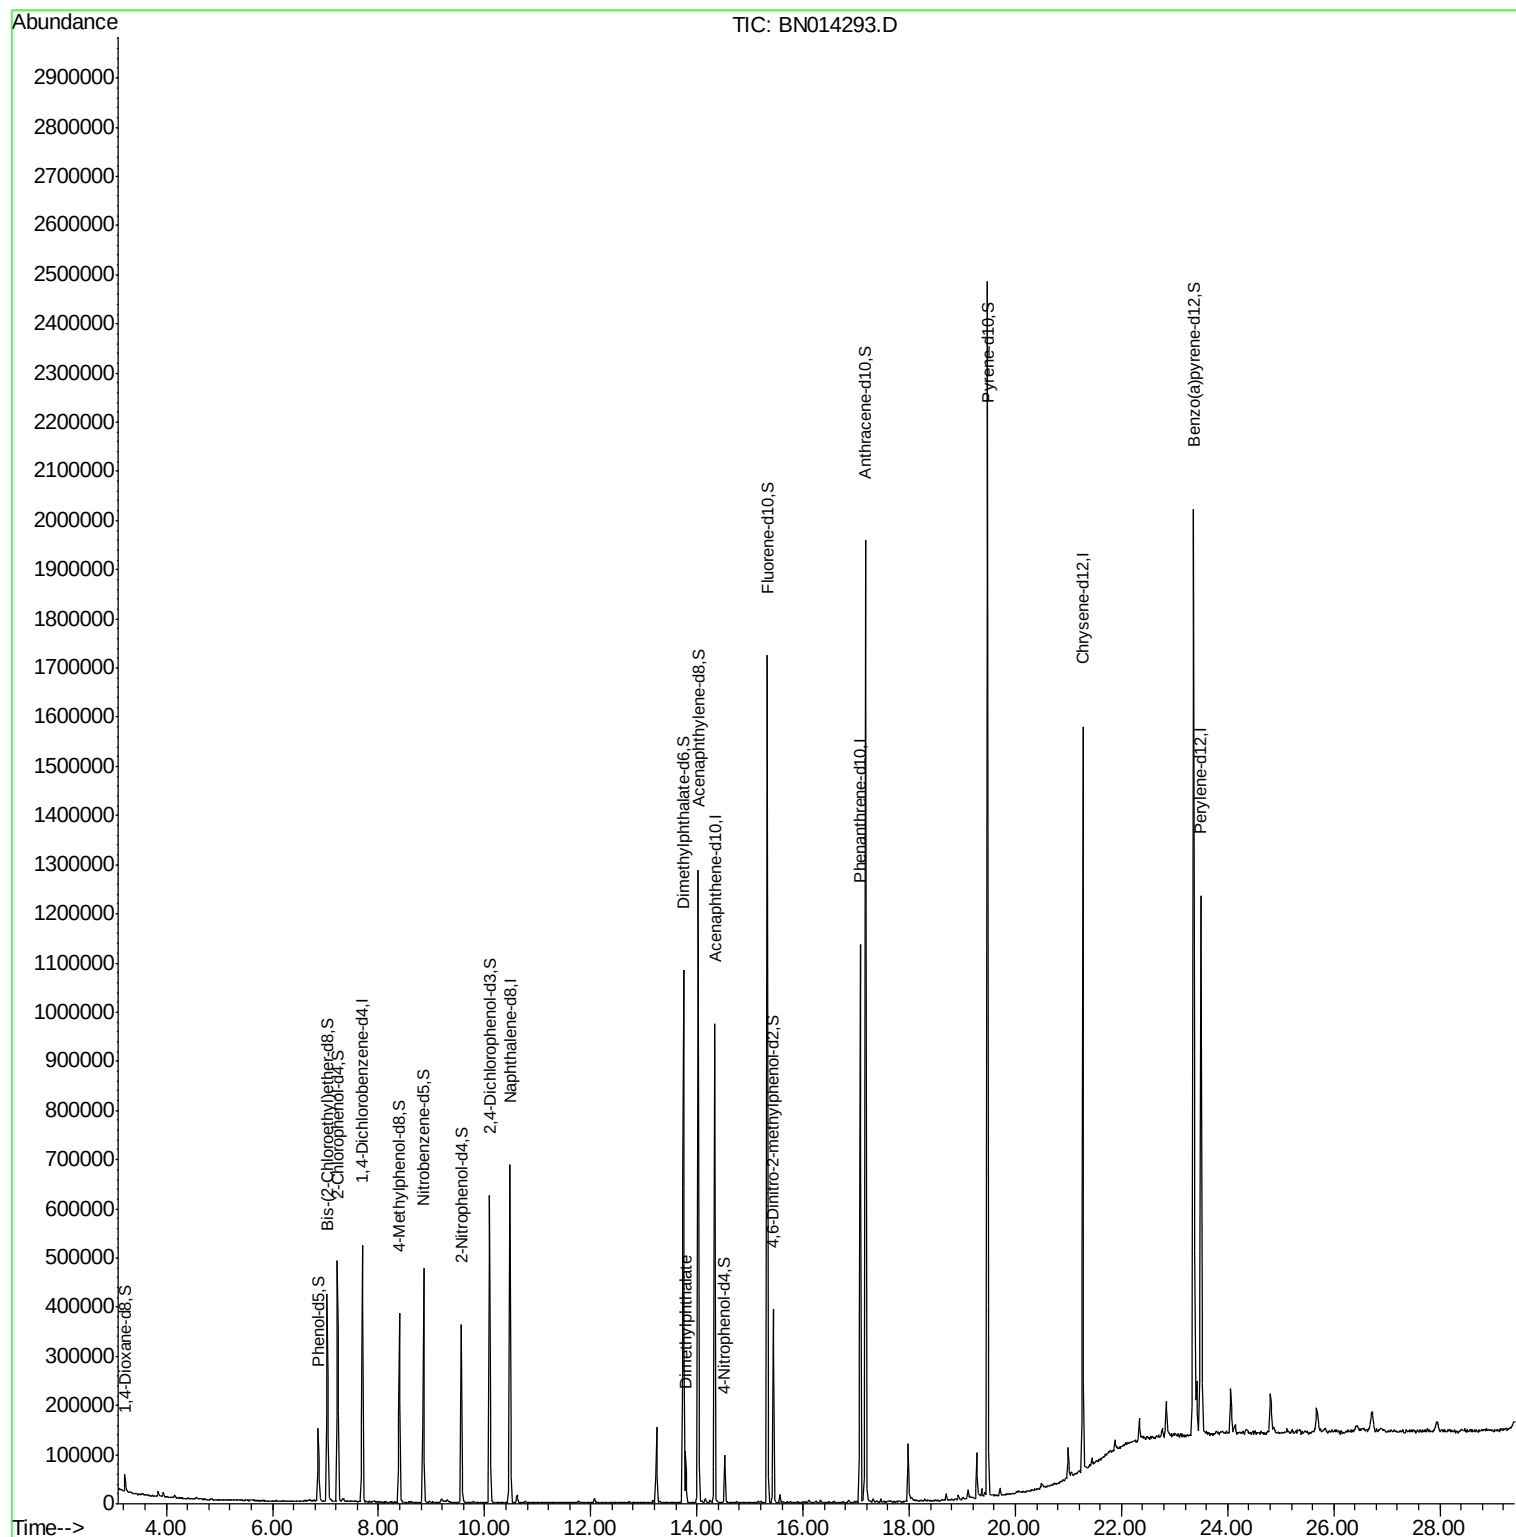

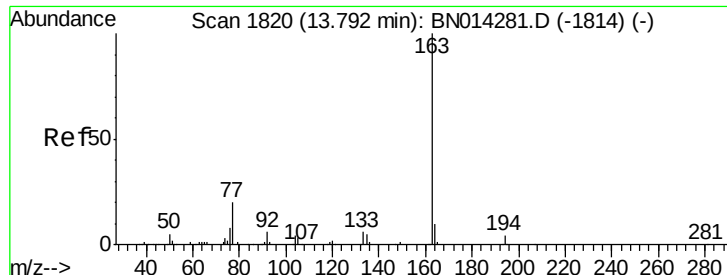

#47

Dimethylphthalate

Concen: 2.607 ng/ul

RT: 13.79 min Scan# 1820

Delta R.T. 0.00 min

Lab File: BN014293.D

Acq: 15 Apr 2021 20:25

Instrument :

BNA_N

ClientSampleId :

BG536


Tot Ion:163 Resp: 64642

Ion Ratio Lower Upper

163 100

194 3.7 3.3 4.9

164 9.6 7.8 11.8

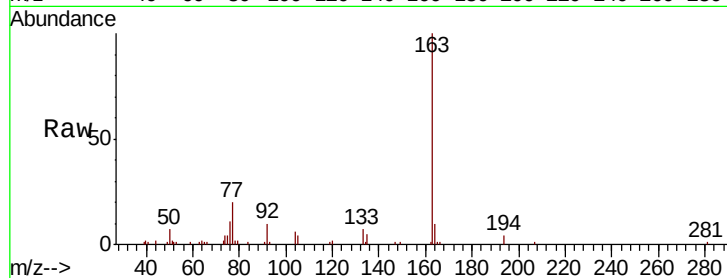

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

