

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
 Data File : BN014297.D
 Acq On : 15 Apr 2021 23:24
 Operator : CG/JU
 Sample : M2031-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG530

Quant Time: Apr 16 02:35:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 15 15:18:04 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	131985	20.00	ng/ul	0.00
20) Naphthalene-d8	10.48	136	524110	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.33	164	312360	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.07	188	628290	20.00	ng/ul	0.00
79) Chrysene-d12	21.27	240	645454	20.00	ng/ul	0.00
88) Perylene-d12	23.50	264	693763	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	17641	5.09	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.86	99	84430	7.65	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.03	67	180667	27.34	ng/ul	0.00
11) 2-Chlorophenol-d4	7.23	132	218271	25.15	ng/ul	0.00
15) 4-Methylphenol-d8	8.39	113	135718	16.23	ng/ul	0.00
21) Nitrobenzene-d5	8.85	128	105377	27.82	ng/ul	0.00
24) 2-Nitrophenol-d4	9.56	143	104549	28.19	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.09	165	208752	26.13	ng/ul	0.00
31) 4-Chloroaniline-d4	10.61	131	10889	0.92	ng/ul	0.00
46) Dimethylphthalate-d6	13.75	166	690417	30.51	ng/ul	0.00
49) Acenaphthylene-d8	14.02	160	845817	31.07	ng/ul	0.00
54) 4-Nitrophenol-d4	14.52	143	24215	5.52	ng/ul	0.00
60) Fluorene-d10	15.33	176	635809	31.78	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.44	200	78497	23.35	ng/ul	0.00
73) Anthracene-d10	17.17	188	1091729	37.23	ng/ul	0.00
81) Pyrene-d10	19.47	212	1257596	40.14	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.36	264	1423044	38.67	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.79	163	57285	2.439	ng/ul	Ovalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041521\
Data File : BN014297.D
Acq On : 15 Apr 2021 23:24
Operator : CG/JU
Sample : M2031-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG530

Quant Time: Apr 16 02:35:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 15 15:18:04 2021
Response via : Initial Calibration

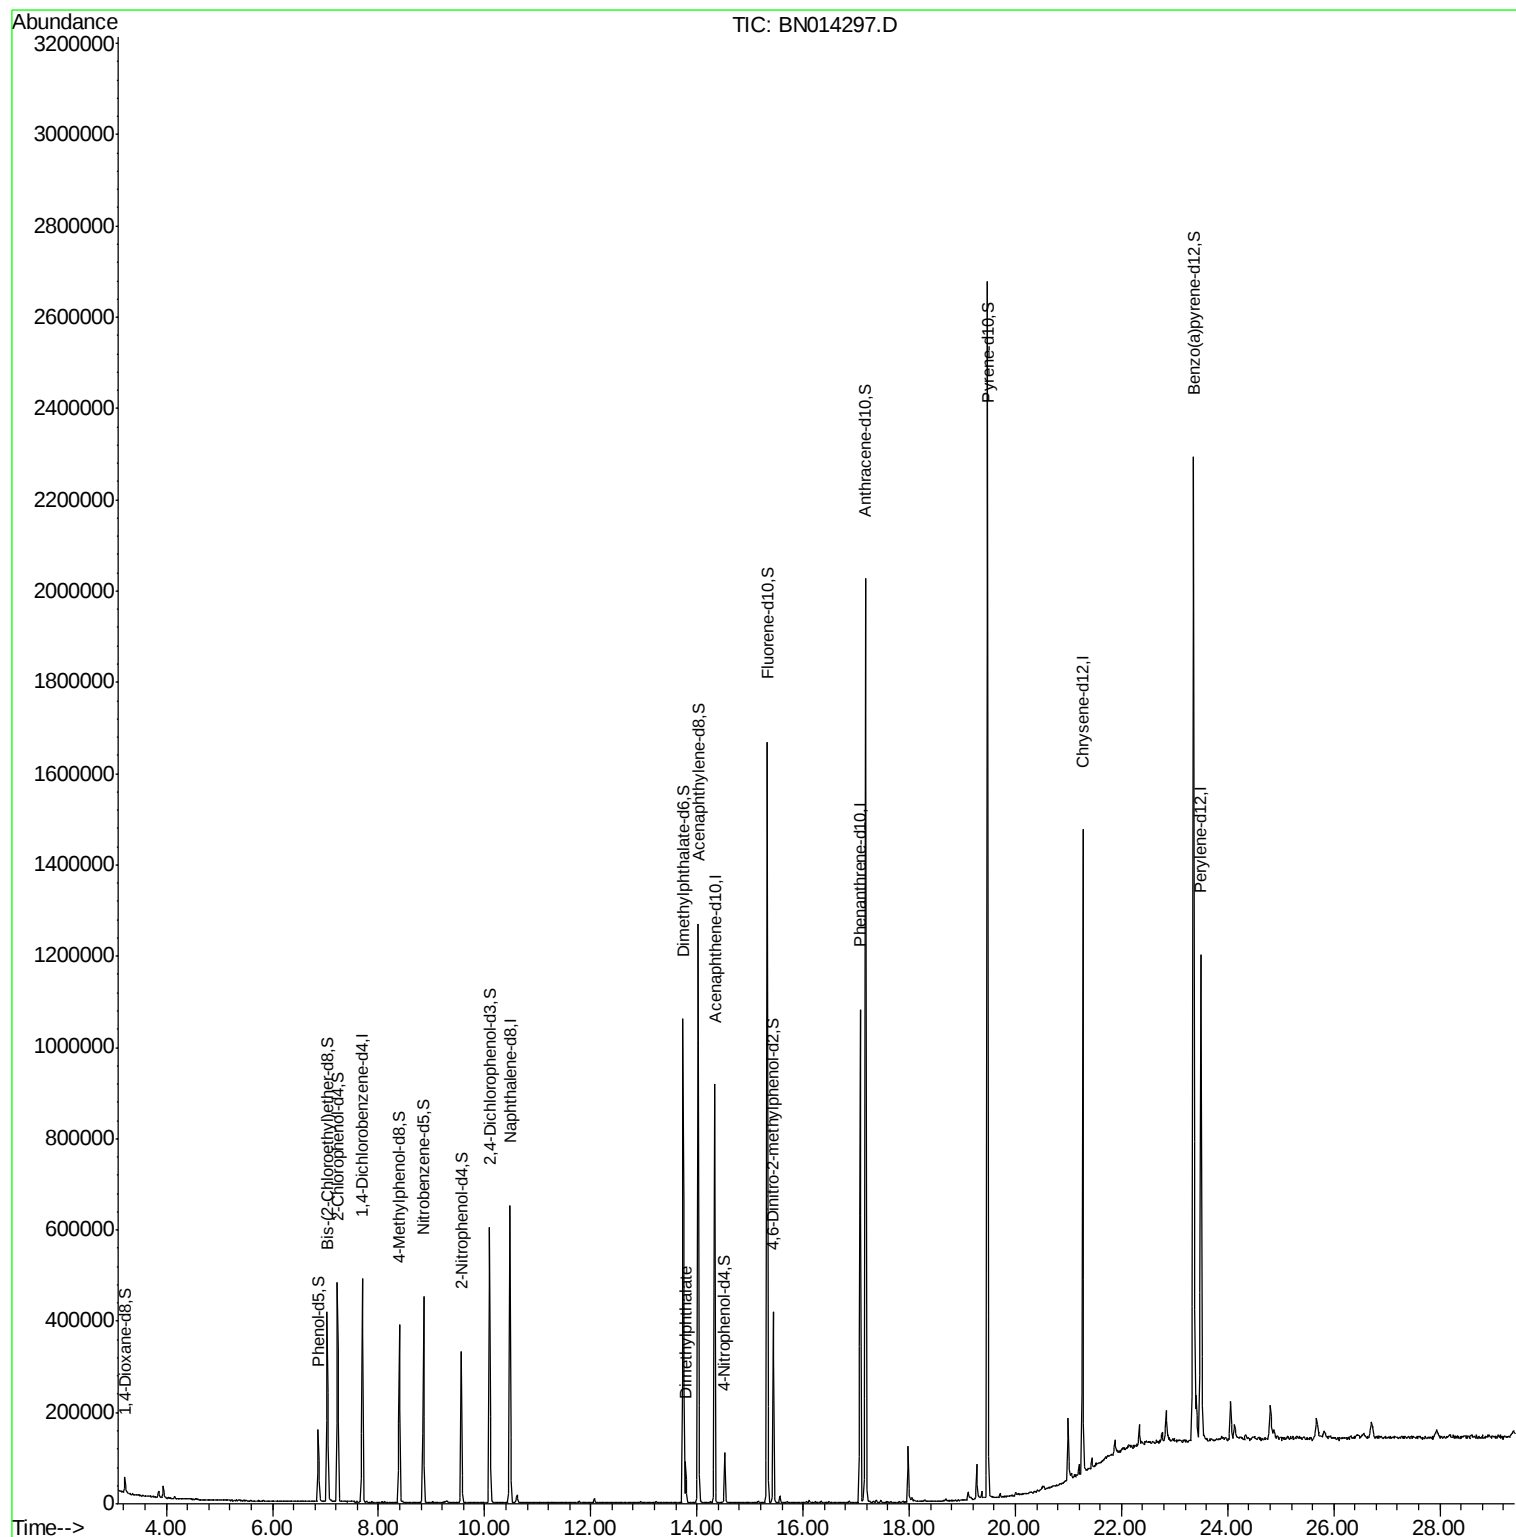

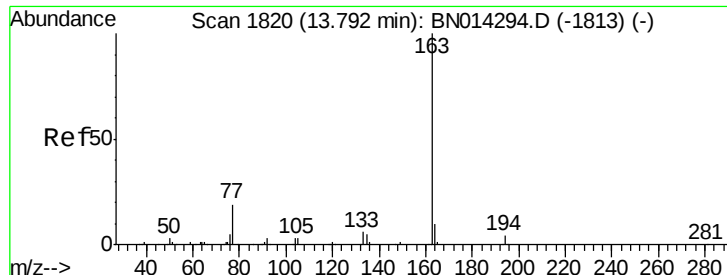

#47

Dimethylphthalate

Concen: 2.439 ng/ul

RT: 13.79 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BN014297.D

Acq: 15 Apr 2021 23:24

Instrument :

BNA_N

ClientSampleId :

BG530


Tot Ion:163 Resp: 57285

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.8 7.8 11.8

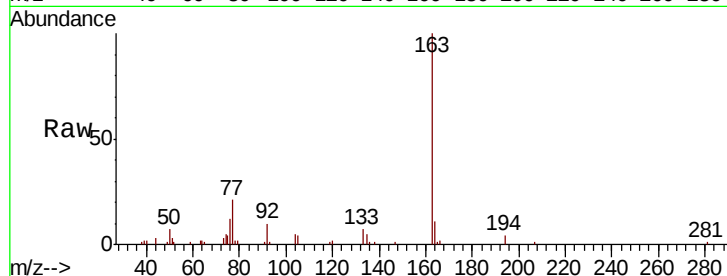

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

