

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041521\
 Data File : BN014291.D
 Acq On : 15 Apr 2021 19:13
 Operator : CG/JU
 Sample : M2031-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG538

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	20	23	34	rVB	32634	47690	1.18%	0.144%
2	3.858	126	131	138	rVB	12346	20997	0.52%	0.064%
3	3.946	143	146	151	rVB	9135	11926	0.30%	0.036%
4	4.158	180	182	188	rVB5	5280	6997	0.17%	0.021%
5	6.863	636	642	653	rVB	139686	233539	5.79%	0.707%
6	7.034	665	671	686	rBV	433734	686504	17.03%	2.077%
7	7.234	698	705	712	rVB	510602	791465	19.63%	2.395%
8	7.340	719	723	727	rVB4	2833	4122	0.10%	0.012%
9	7.699	777	784	792	rVB	535011	816716	20.25%	2.471%
10	8.393	896	902	910	rBV	374166	582906	14.46%	1.764%
11	8.846	971	979	988	rBV	501109	784826	19.46%	2.375%
12	9.251	1040	1048	1050	rBV4	2000	5126	0.13%	0.016%
13	9.287	1050	1054	1062	rVB4	5088	10754	0.27%	0.033%
14	9.563	1094	1101	1110	rBV	375318	595994	14.78%	1.803%
15	10.093	1185	1191	1199	rBV	655800	1051009	26.07%	3.180%
16	10.475	1249	1256	1264	rBV	705527	1134445	28.13%	3.433%
17	10.610	1273	1279	1284	rBV	24186	38389	0.95%	0.116%
18	11.116	1360	1365	1370	rBV5	2008	4050	0.10%	0.012%
19	12.063	1522	1526	1531	rVB2	8562	12532	0.31%	0.038%
20	12.687	1627	1632	1635	rBV3	2803	4490	0.11%	0.014%
21	12.939	1672	1675	1678	rBV3	3565	4395	0.11%	0.013%
22	13.169	1711	1714	1718	rBV3	4961	6320	0.16%	0.019%
23	13.239	1720	1726	1733	rBV	11904	18106	0.45%	0.055%
24	13.745	1806	1812	1816	rBV	1268687	1685710	41.81%	5.101%
25	13.792	1816	1820	1826	rVB	122367	169060	4.19%	0.512%
26	14.022	1850	1859	1867	rBV	1408460	2004298	49.71%	6.065%
27	14.251	1894	1898	1902	rVB4	5223	6485	0.16%	0.020%
28	14.334	1905	1912	1919	rBV	988706	1434746	35.58%	4.341%
29	14.522	1938	1944	1951	rBV	106352	151459	3.76%	0.458%
30	15.163	2047	2053	2058	rVB2	5884	9835	0.24%	0.030%
31	15.328	2074	2081	2089	rBV	1945824	2635400	65.36%	7.974%
32	15.439	2095	2100	2111	rBV	495116	640451	15.88%	1.938%
33	15.569	2115	2122	2127	rBV	17690	24559	0.61%	0.074%
34	15.892	2171	2177	2182	rBV5	2742	5662	0.14%	0.017%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041521\
 Data File : BN014291.D
 Acq On : 15 Apr 2021 19:13
 Operator : CG/JU
 Sample : M2031-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG538

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	16.063	2203	2206	2209	rBV2	3466	4041	0.10%	0.012%
36	16.110	2212	2214	2221	rVB3	7277	9051	0.22%	0.027%
37	16.333	2247	2252	2257	rVB4	5439	9250	0.23%	0.028%
38	16.492	2274	2279	2283	rBV3	2925	4209	0.10%	0.013%
39	16.863	2339	2342	2348	rBV2	5058	7940	0.20%	0.024%
40	17.080	2372	2379	2386	rBV	1178037	1642051	40.72%	4.969%
41	17.175	2386	2395	2408	rVV	2203318	3094135	76.74%	9.362%
42	17.316	2415	2419	2426	rVB5	5305	7560	0.19%	0.023%
43	17.386	2426	2431	2435	rBV6	4779	7802	0.19%	0.024%
44	17.463	2437	2444	2447	rBV4	8873	11087	0.27%	0.034%
45	17.875	2511	2514	2520	rVB4	2219	4207	0.10%	0.013%
46	17.980	2528	2532	2542	rBV	91122	138674	3.44%	0.420%
47	18.051	2542	2544	2549	rVB2	5605	8405	0.21%	0.025%
48	18.286	2581	2584	2589	rBV5	4595	6102	0.15%	0.018%
49	18.698	2650	2654	2658	rBV3	12702	14591	0.36%	0.044%
50	18.927	2689	2693	2698	rBV3	7499	12363	0.31%	0.037%
51	19.022	2705	2709	2711	rBV4	3722	6241	0.15%	0.019%
52	19.063	2713	2716	2720	rVB3	8733	10568	0.26%	0.032%
53	19.110	2720	2724	2728	rBV	24416	32166	0.80%	0.097%
54	19.145	2728	2730	2735	rVV5	3144	4995	0.12%	0.015%
55	19.269	2748	2751	2760	rBV	50996	74113	1.84%	0.224%
56	19.363	2763	2767	2771	rVB	18156	22476	0.56%	0.068%
57	19.474	2780	2786	2795	rBV	2828740	3850358	95.49%	11.651%
58	19.716	2824	2827	2830	rVB	9956	9092	0.23%	0.028%
59	20.010	2875	2877	2880	rVB4	5748	4249	0.11%	0.013%
60	20.998	3041	3045	3052	rBV3	94428	140398	3.48%	0.425%
61	21.198	3077	3079	3085	rVB	27060	27061	0.67%	0.082%
62	21.268	3086	3091	3097	rBV	1534212	1927426	47.80%	5.832%
63	22.339	3270	3273	3278	rBV3	35092	40930	1.02%	0.124%
64	22.845	3356	3359	3368	rVB4	57216	100292	2.49%	0.303%
65	23.362	3440	3447	3453	rBV	2298431	4032201	100.00%	12.201%
66	23.504	3464	3471	3480	rVB2	1117908	2019334	50.08%	6.110%
67	24.062	3562	3566	3571	rVB2	73306	124463	3.09%	0.377%


Sum of corrected areas: 33048794

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041521\
Data File : BN014291.D
Acq On : 15 Apr 2021 19:13
Operator : CG/JU
Sample : M2031-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG538

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

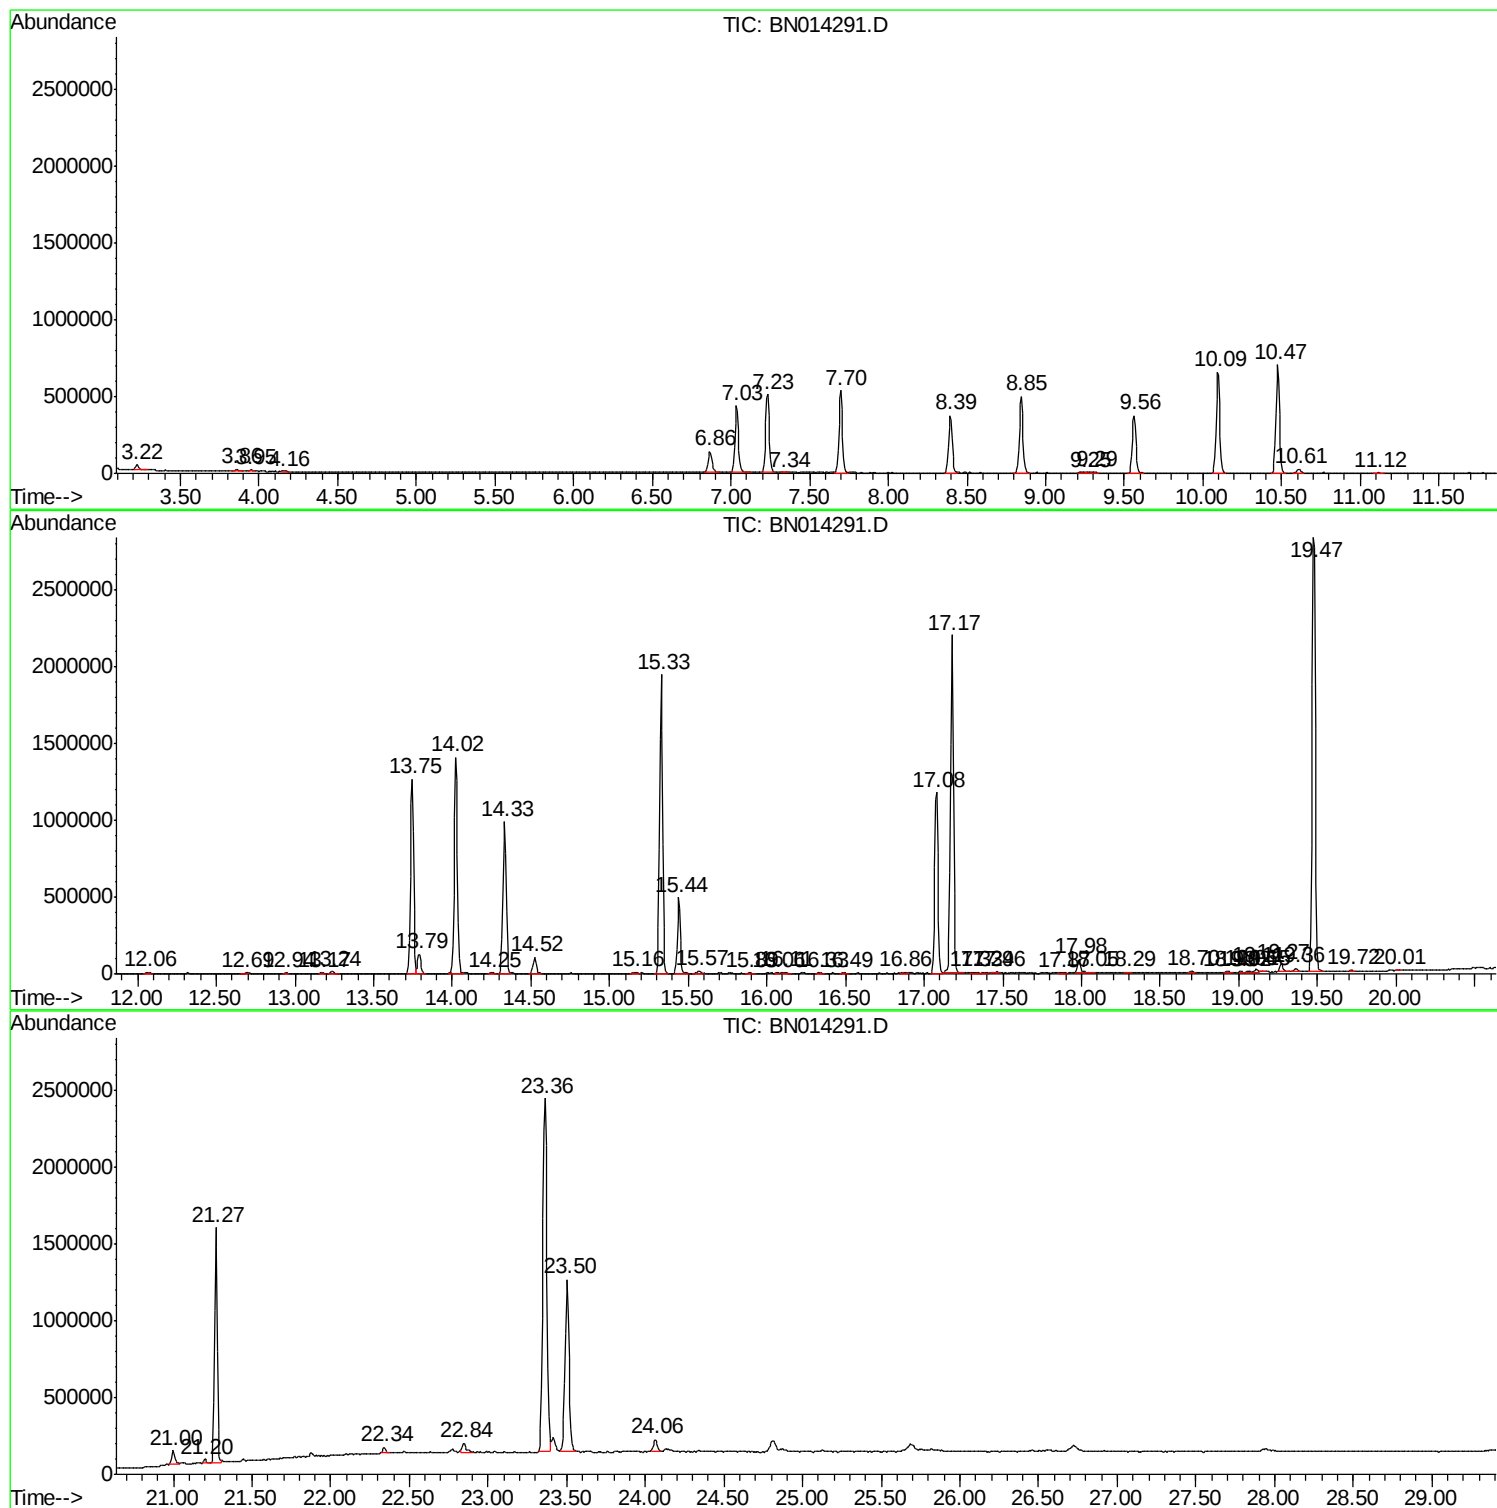

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
Data File : BN014291.D
Acq On : 15 Apr 2021 19:13
Operator : CG/JU
Sample : M2031-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG538

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
Data File : BN014291.D
Acq On : 15 Apr 2021 19:13
Operator : CG/JU
Sample : M2031-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG538

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc