

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041521\
 Data File : BN014295.D
 Acq On : 15 Apr 2021 22:12
 Operator : CG/JU
 Sample : PB135757BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK757

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	19	23	29	rVB	41358	53912	1.48%	0.161%
2	3.622	88	91	116	rBV	453380	743964	20.48%	2.225%
3	3.946	142	146	151	rVB	17582	23987	0.66%	0.072%
4	6.863	636	642	654	rBV	633870	952079	26.21%	2.848%
5	7.034	663	671	684	rBV	498383	776724	21.39%	2.323%
6	7.228	698	704	713	rBV	647552	1036151	28.53%	3.100%
7	7.699	777	784	792	rVB	463160	717833	19.76%	2.147%
8	8.393	895	902	913	rBV	753278	1144244	31.51%	3.423%
9	8.846	969	979	992	rBV	530610	852434	23.47%	2.550%
10	9.563	1094	1101	1112	rVB	409809	644677	17.75%	1.928%
11	10.093	1183	1191	1206	rBV	738369	1173032	32.30%	3.509%
12	10.475	1249	1256	1263	rBV	607346	995830	27.42%	2.979%
13	10.604	1271	1278	1288	rBV	709203	1185331	32.64%	3.546%
14	12.063	1521	1526	1535	rVB2	10209	16679	0.46%	0.050%
15	13.745	1805	1812	1823	rBV	1191506	1626970	44.80%	4.867%
16	14.022	1853	1859	1868	rBV	1431376	2016903	55.53%	6.033%
17	14.334	1905	1912	1918	rBV	868137	1260839	34.72%	3.772%
18	14.522	1938	1944	1957	rBV	533563	707171	19.47%	2.115%
19	15.163	2046	2053	2056	rBV3	2155	3701	0.10%	0.011%
20	15.328	2074	2081	2089	rBV	1778546	2472579	68.08%	7.396%
21	15.439	2094	2100	2110	rBV	410681	532460	14.66%	1.593%
22	15.569	2118	2122	2126	rVB	15500	19538	0.54%	0.058%
23	16.110	2212	2214	2217	rVB2	4431	4898	0.13%	0.015%
24	16.869	2335	2343	2346	rBV	2547	3636	0.10%	0.011%
25	17.075	2372	2378	2385	rBV	998680	1425935	39.26%	4.266%
26	17.175	2389	2395	2410	rVB	1906454	2667613	73.45%	7.980%
27	19.110	2720	2724	2728	rBV2	15842	20389	0.56%	0.061%
28	19.363	2764	2767	2772	rVB	13095	16797	0.46%	0.050%
29	19.474	2780	2786	2799	rBV	2508878	3274509	90.16%	9.795%
30	21.269	3086	3091	3096	rBV	1356028	1617287	44.53%	4.838%
31	23.357	3439	3446	3453	rBV	2086237	3631864	100.00%	10.864%
32	23.498	3463	3470	3486	rVB	984115	1809423	49.82%	5.413%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041521\
Data File : BN014295.D
Acq On : 15 Apr 2021 22:12
Operator : CG/JU
Sample : PB135757BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK757

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Title : SVOA CALIBRATION


Sum of corrected areas: 33429389

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN041521\
Data File : BN014295.D
Acq On : 15 Apr 2021 22:12
Operator : CG/JU
Sample : PB135757BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK757

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

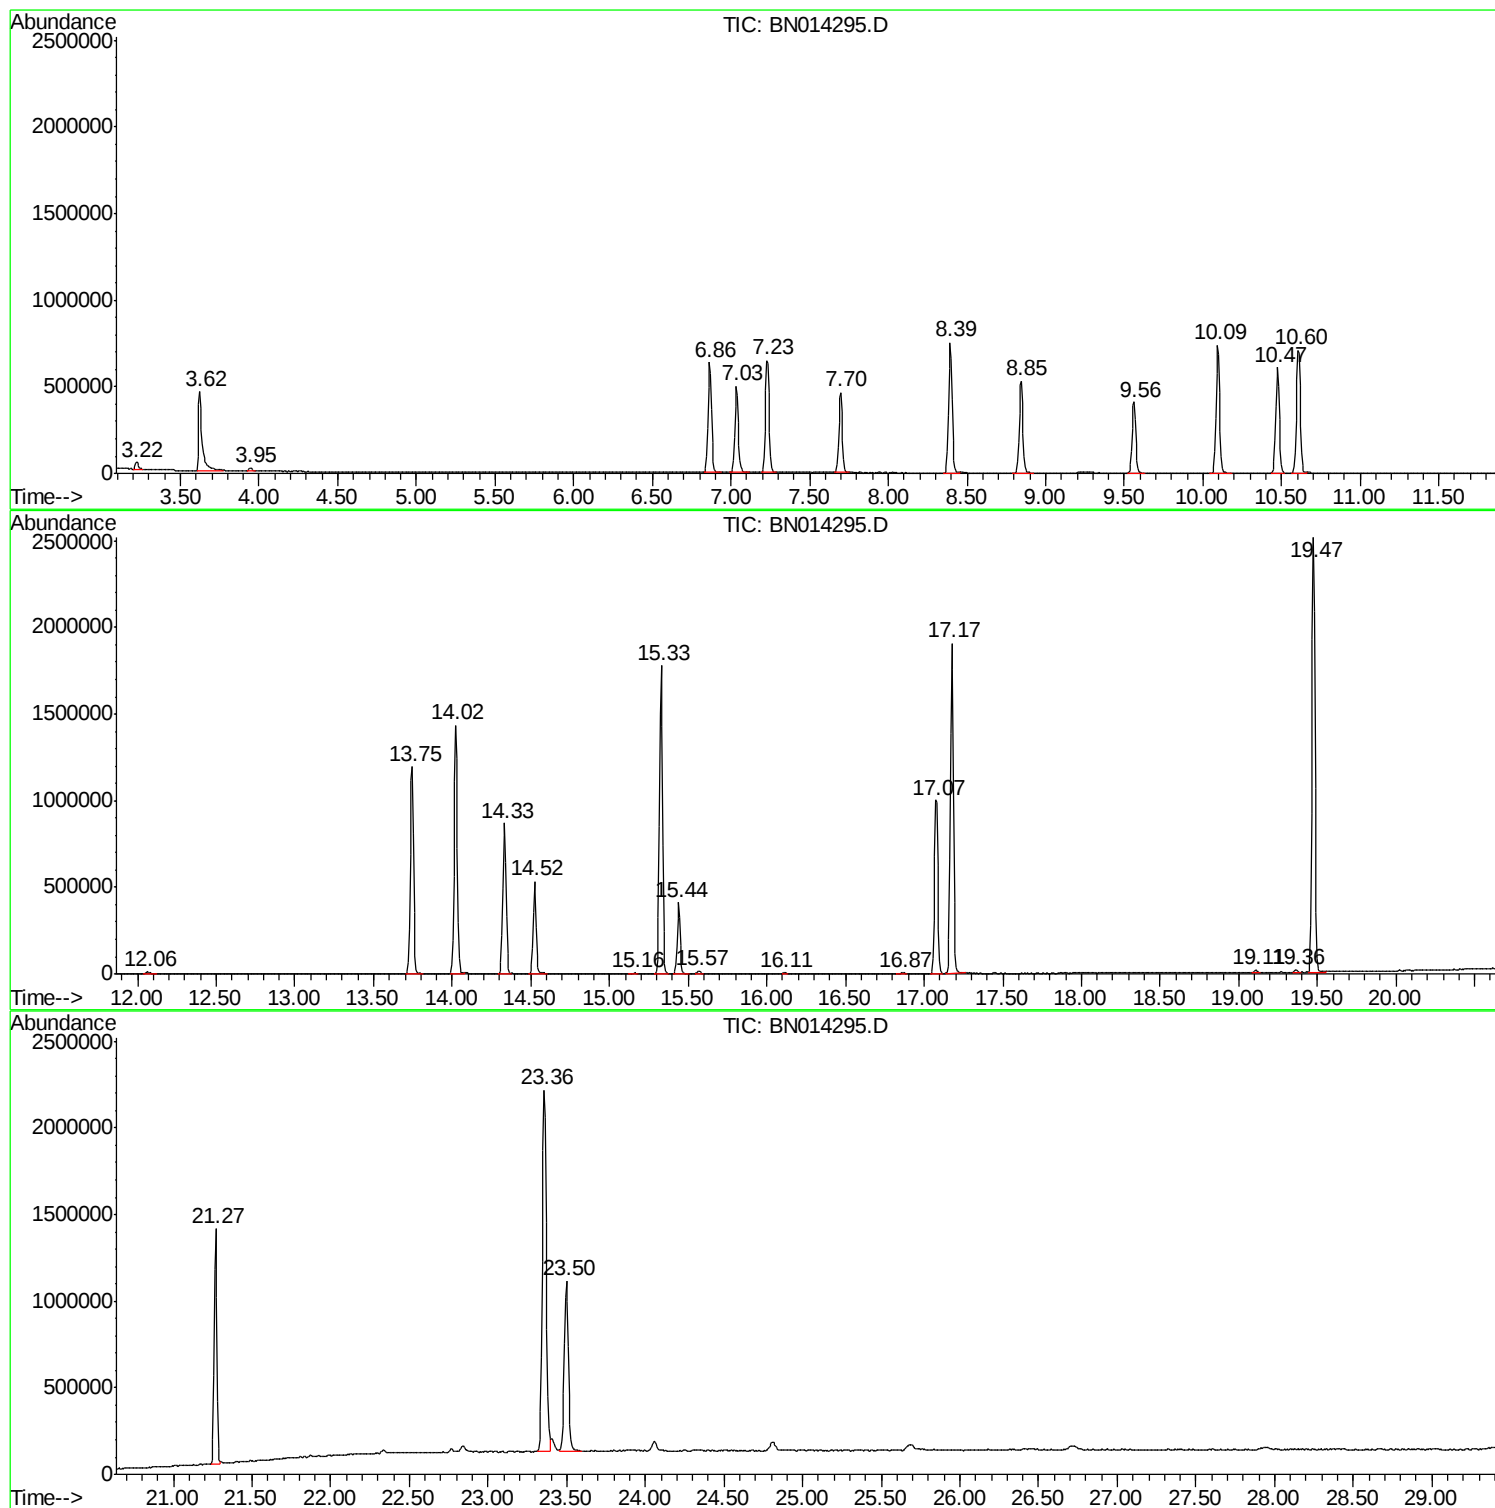

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
Data File : BN014295.D
Acq On : 15 Apr 2021 22:12
Operator : CG/JU
Sample : PB135757BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK757

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN041521\
Data File : BN014295.D
Acq On : 15 Apr 2021 22:12
Operator : CG/JU
Sample : PB135757BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK757

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc