




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
 Data File : BN019456.D
 Acq On : 15 Apr 2022 11:13
 Operator : CG/JU
 Sample : PB144123BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK123

Manual IntegrationsAPPROVED

Quant Time: Apr 18 05:01:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

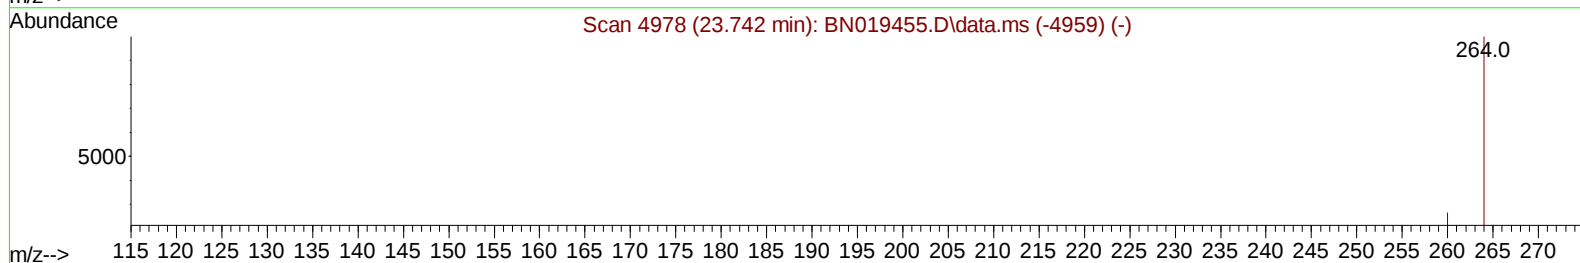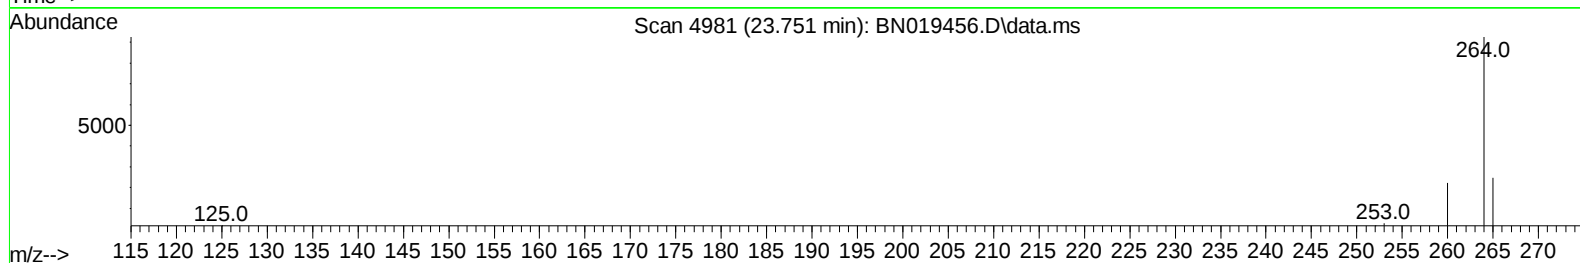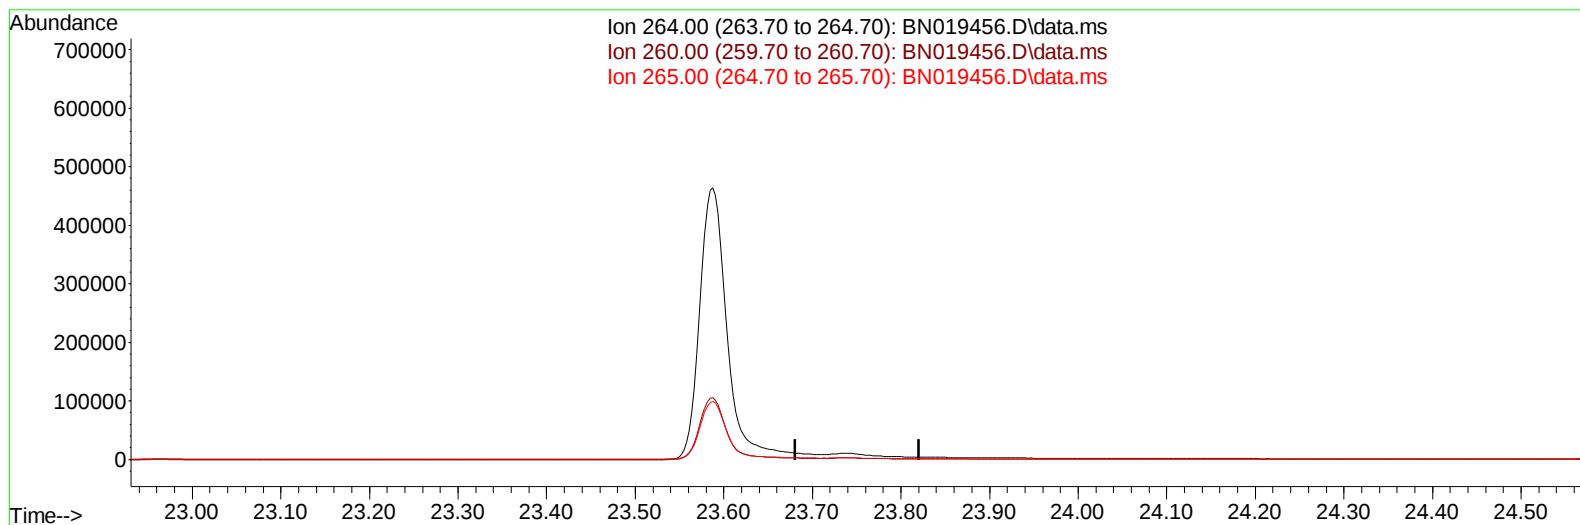

TIC: BN019456.D\data.ms

(23) Perylene-d12 (I)

23.751min (-23.751) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
 Data File : BN019456.D
 Acq On : 15 Apr 2022 11:13
 Operator : CG/JU
 Sample : PB144123BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK123

Manual IntegrationsAPPROVED

Quant Time: Apr 18 05:01:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

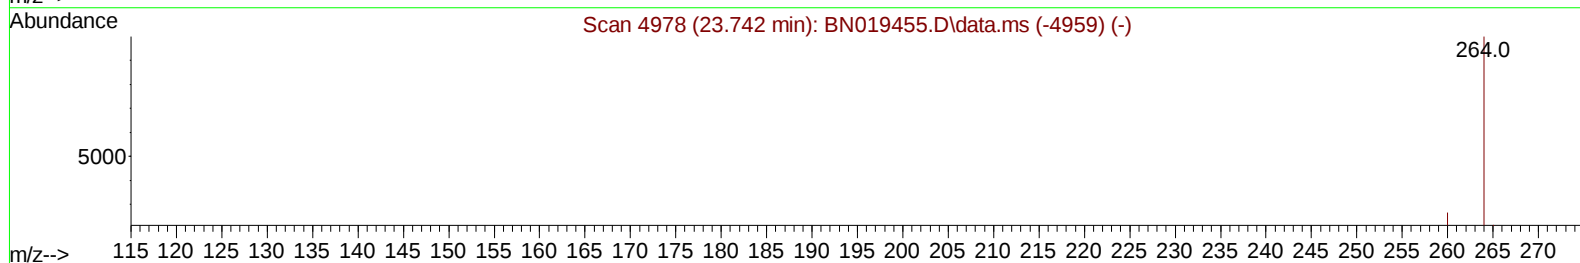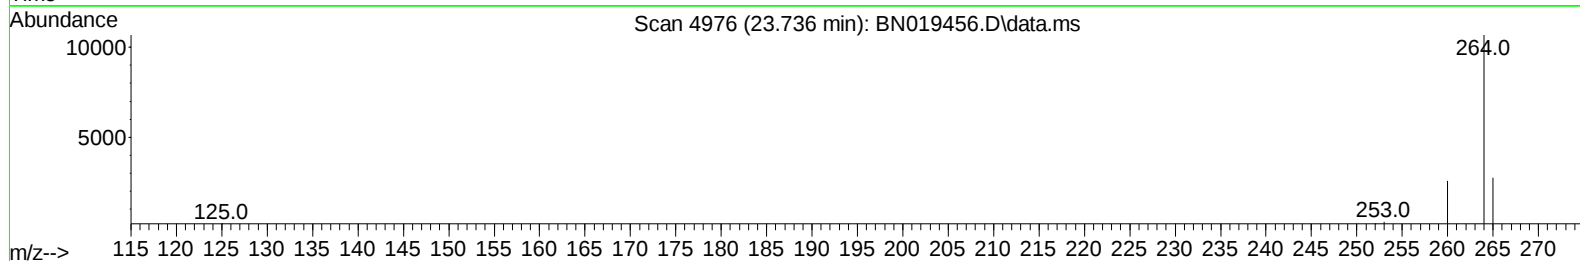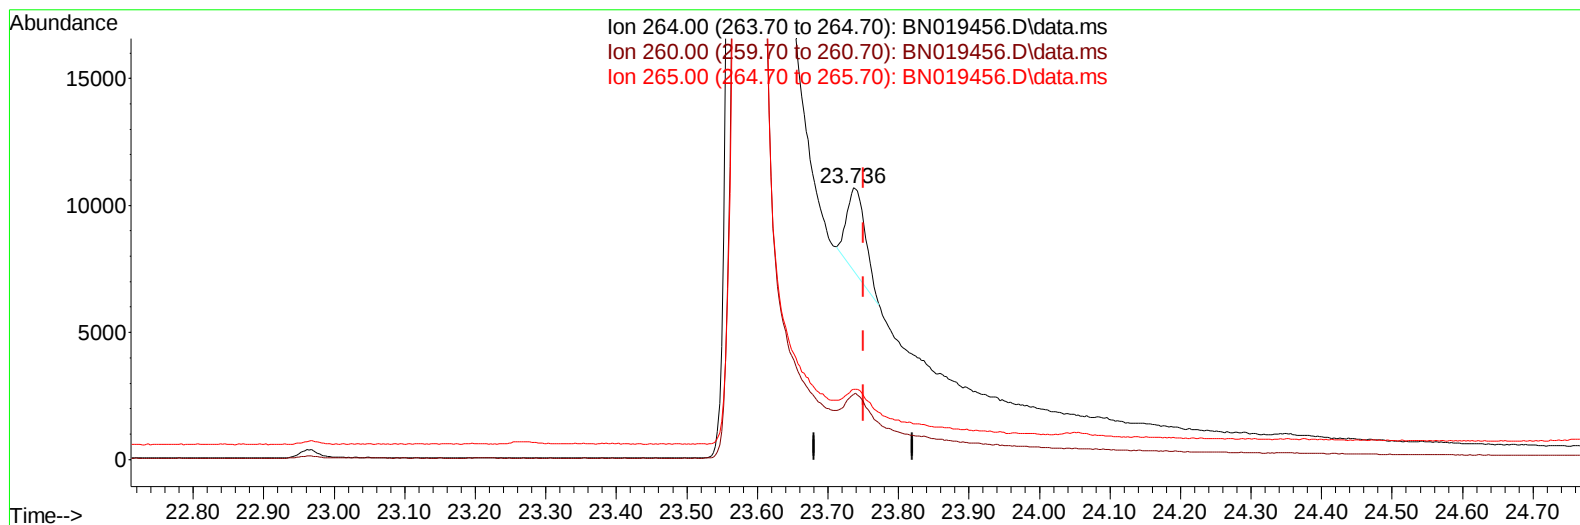

TIC: BN019456.D\data.ms

(23) Perylene-d12 (I)

23.736min (-0.014) 0.40 ng/ul m

response 5978

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.01
265.00	45.70	25.77#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
 Data File : BN019456.D
 Acq On : 15 Apr 2022 11:13
 Operator : CG/JU
 Sample : PB144123BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK123

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

Quant Time: Apr 18 05:01:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.814	152		5715	0.400	ng/ul	0.00
4) Naphthalene-d8	10.613	136		17454	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.457	164		10626	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.197	188		21003	0.400	ng/ul	0.00
17) Chrysene-d12	21.407	240		10943	0.400	ng/ul	0.01
23) Perylene-d12	23.736	264		5978m	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.173	96		41879	5.694	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.219	152		8469	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.231	212		18038	0.445	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
Data File : BN019456.D
Acq On : 15 Apr 2022 11:13
Operator : CG/JU
Sample : PB144123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK123

Manual IntegrationsAPPROVED

Quant Time: Apr 18 05:01:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 14:35:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

