




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
 Data File : BN019465.D
 Acq On : 15 Apr 2022 16:38
 Operator : CG/JU
 Sample : N2280-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFC1

Manual IntegrationsAPPROVED

Quant Time: Apr 18 05:03:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

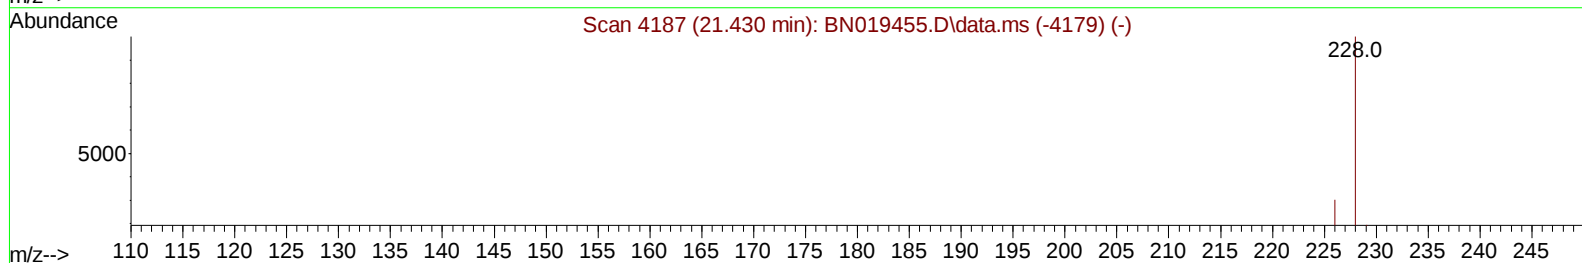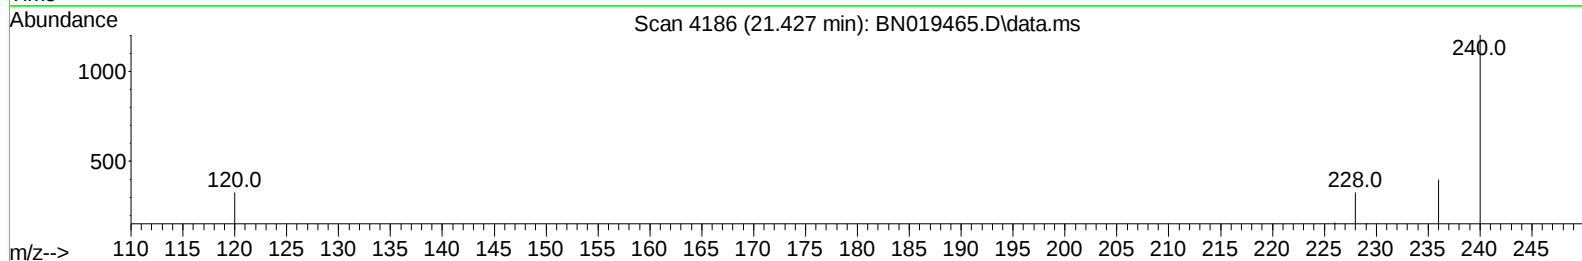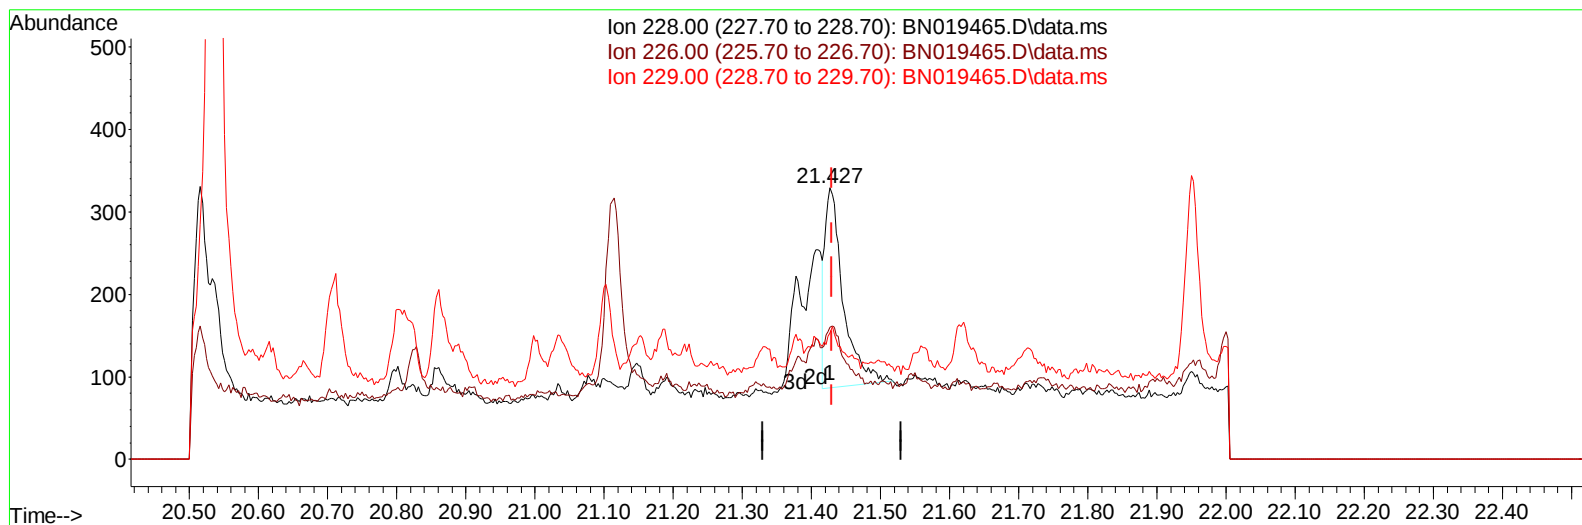

TIC: BN019465.D\data.ms

(22) Chrysene

21.427min (-0.003) 0.01 ng/u1

response 444

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	48.63#
229.00	20.00	46.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
 Data File : BN019465.D
 Acq On : 15 Apr 2022 16:38
 Operator : CG/JU
 Sample : N2280-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFC1

Manual IntegrationsAPPROVED

Quant Time: Apr 18 05:03:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

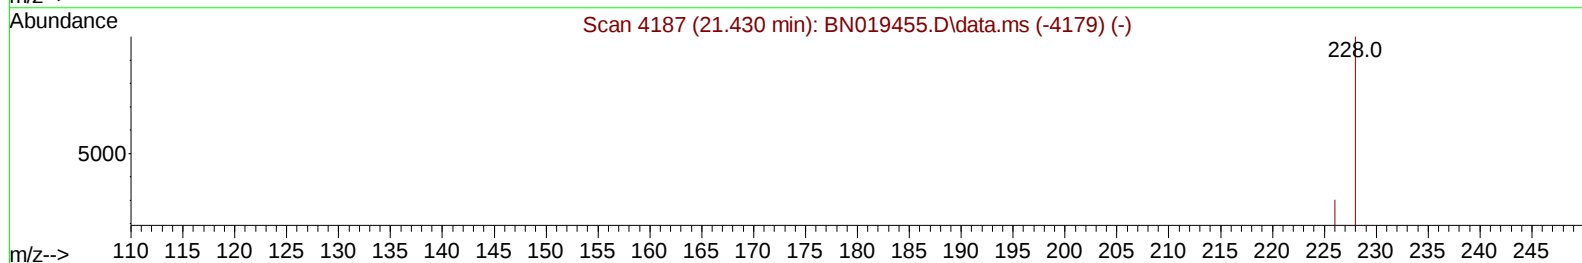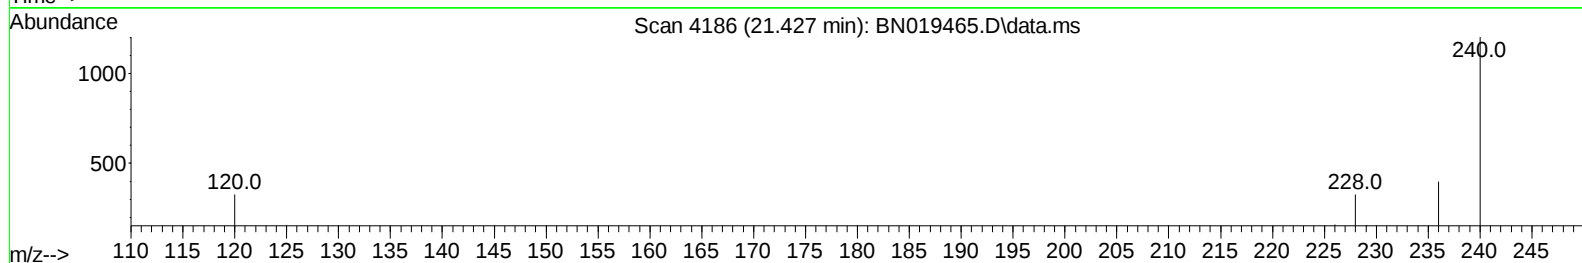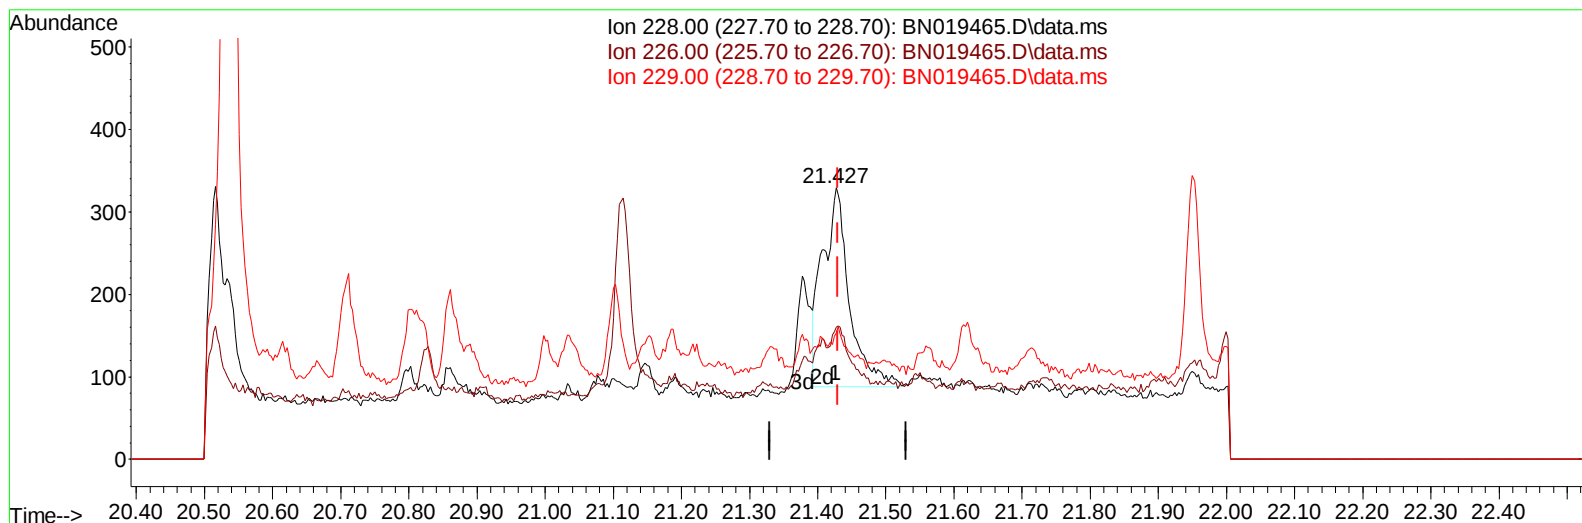

TIC: BN019465.D\data.ms

(22) Chrysene

21.427min (-0.003) 0.02 ng/u1 m

response 670

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.20	48.63#
229.00	20.00	46.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
Data File : BN019465.D
Acq On : 15 Apr 2022 16:38
Operator : CG/JU
Sample : N2280-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFC1

Manual IntegrationsAPPROVED

Quant Time: Apr 18 05:03:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 14:35:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

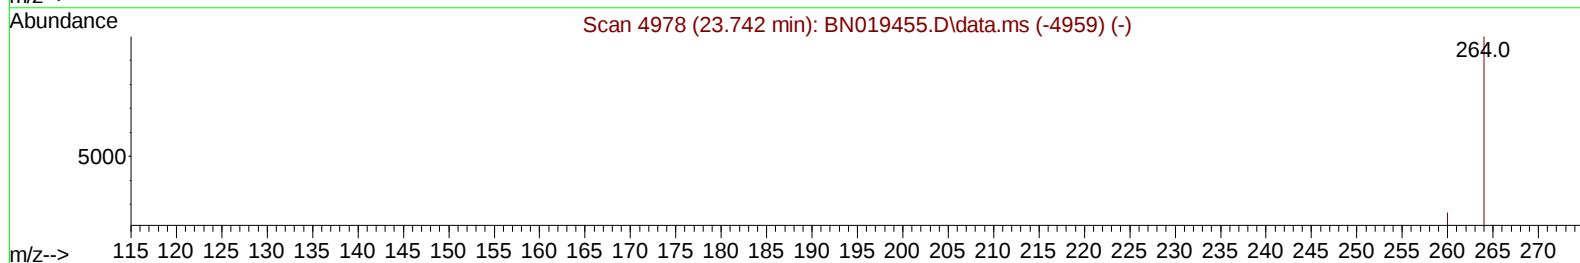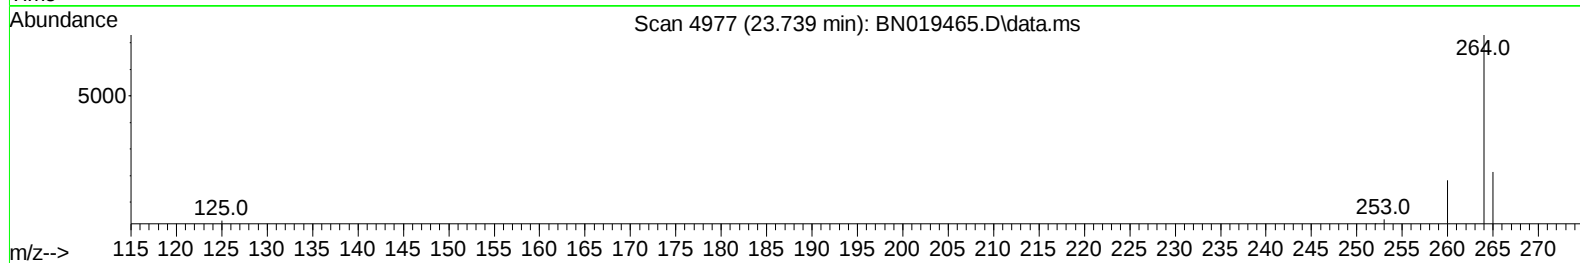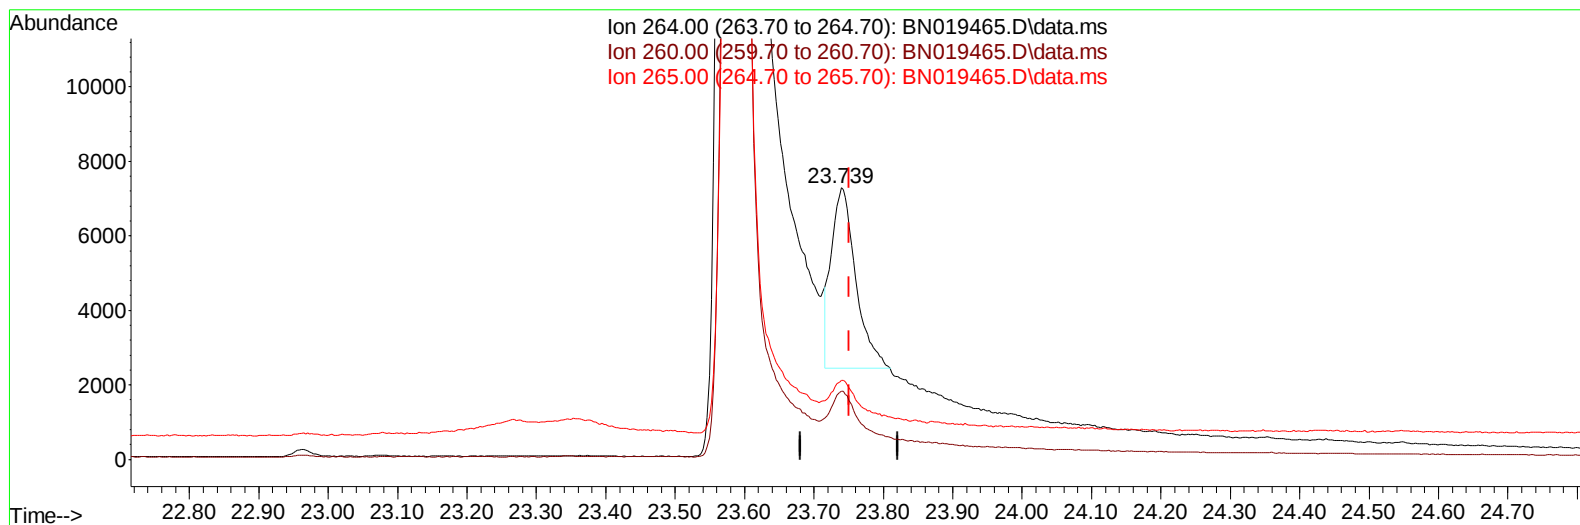

TIC: BN019465.D\data.ms

(23) Perylene-d12 (I)

23.739min (-0.012) 0.40 ng/u1

response 11846

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	25.22
265.00	45.70	29.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
 Data File : BN019465.D
 Acq On : 15 Apr 2022 16:38
 Operator : CG/JU
 Sample : N2280-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFC1

Manual IntegrationsAPPROVED

Quant Time: Apr 18 05:03:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

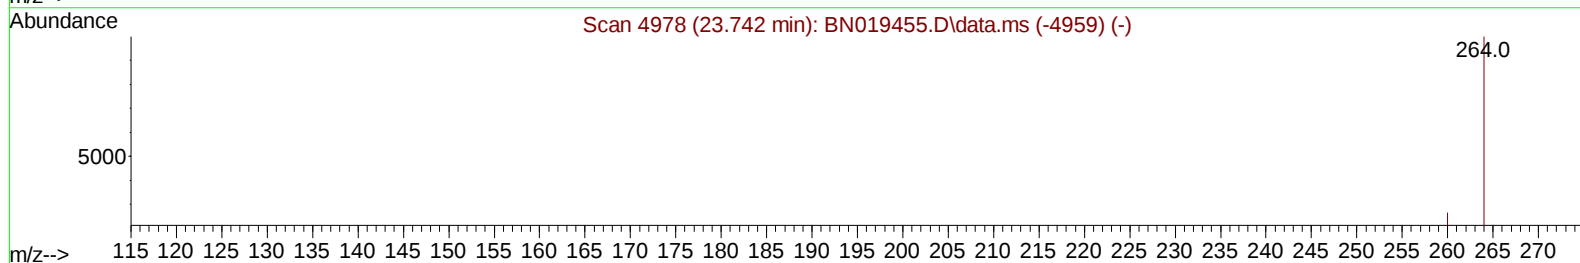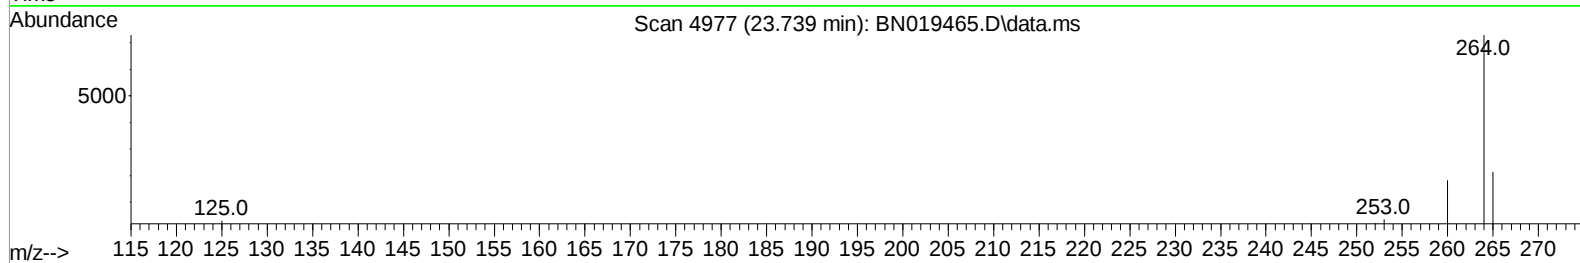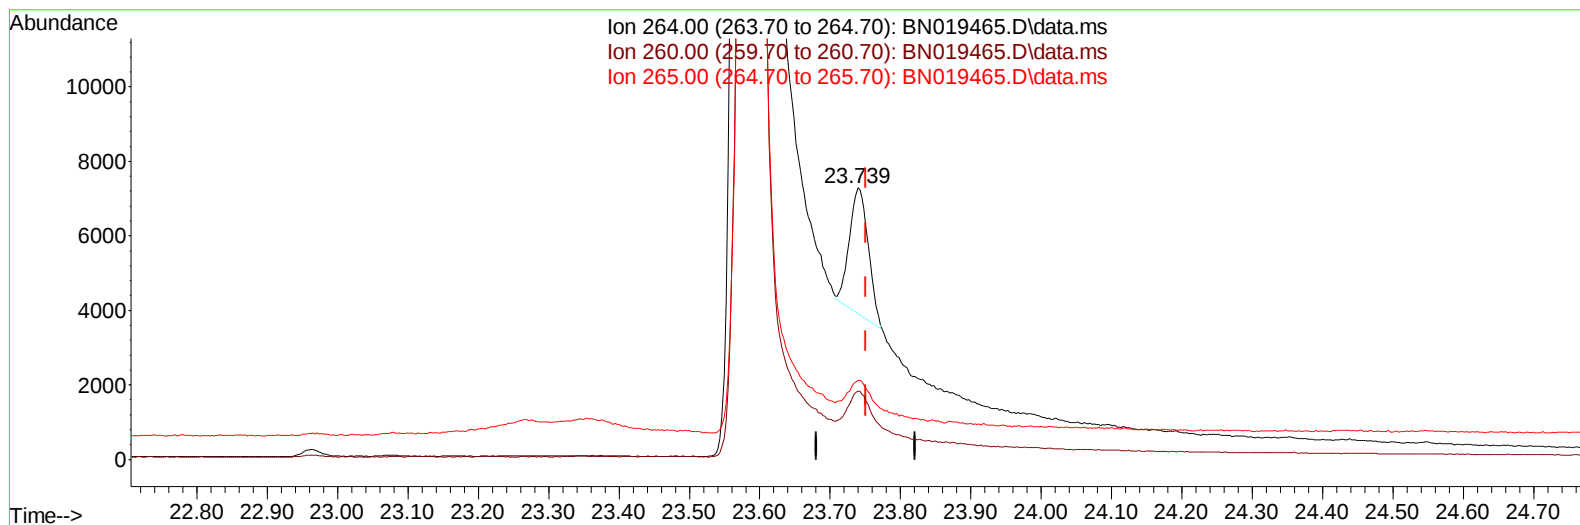

TIC: BN019465.D\data.ms

(23) Perylene-d12 (I)

23.739min (-0.012) 0.40 ng/ul m

response 6232

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	25.22
265.00	45.70	29.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
 Data File : BN019465.D
 Acq On : 15 Apr 2022 16:38
 Operator : CG/JU
 Sample : N2280-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFC1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

Quant Time: Apr 18 05:03:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.814	152	4344	0.400	ng/ul	0.00
4) Naphthalene-d8	10.618	136	13365	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164	8281	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.197	188	16728	0.400	ng/ul	0.00
17) Chrysene-d12	21.395	240	11070	0.400	ng/ul	0.00
23) Perylene-d12	23.739	264	6232m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.173	96	11533	2.063	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.213	152	3720	0.197	ng/ul	0.00
18) Fluoranthene-d10	19.231	212	9088	0.222	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.868	266	91	0.034	ng/ul#	89
19) Fluoranthene	19.259	202	2477	0.045	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041522\
Data File : BN019465.D
Acq On : 15 Apr 2022 16:38
Operator : CG/JU
Sample : N2280-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFC1

Manual IntegrationsAPPROVED

Quant Time: Apr 18 05:03:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 14:35:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

