

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
 Data File : BN030947.D
 Acq On : 15 Apr 2024 20:50
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Apr 16 00:17:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 17:03:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.653	152	4376	0.400	ng	0.00
7) Naphthalene-d8	10.431	136	13365	0.400	ng	0.00
13) Acenaphthene-d10	14.295	164	7566	0.400	ng	0.00
19) Phenanthrene-d10	17.040	188	17241	0.400	ng	0.00
29) Chrysene-d12	21.240	240	15488	0.400	ng	# 0.00
35) Perylene-d12	23.457	264	15785	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.248	112	3656	0.375	ng	0.00
5) Phenol-d6	6.822	99	4375	0.371	ng	0.00
8) Nitrobenzene-d5	8.798	82	3412	0.369	ng	0.00
11) 2-Methylnaphthalene-d10	12.024	152	7705	0.375	ng	0.00
14) 2,4,6-Tribromophenol	15.786	330	1002	0.341	ng	0.00
15) 2-Fluorobiphenyl	12.915	172	10174	0.400	ng	0.01
27) Fluoranthene-d10	19.075	212	17274	0.372	ng	0.00
31) Terphenyl-d14	19.683	244	13600	0.378	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.190	88	1989	0.370	ng	99
3) n-Nitrosodimethylamine	3.507	42	1904	0.378	ng	# 96
6) bis(2-Chloroethyl)ether	7.082	93	4245	0.364	ng	99
9) Naphthalene	10.474	128	14159	0.384	ng	100
10) Hexachlorobutadiene	10.762	225	2946	0.398	ng	# 98
12) 2-Methylnaphthalene	12.100	142	9208	0.376	ng	99
16) Acenaphthylene	14.006	152	11989	0.359	ng	100
17) Acenaphthene	14.348	154	8971	0.381	ng	99
18) Fluorene	15.342	166	11883	0.381	ng	99
20) 4,6-Dinitro-2-methylph...	15.428	198	712	0.375	ng	94
21) 4-Bromophenyl-phenylether	16.233	248	3832	0.374	ng	97
22) Hexachlorobenzene	16.345	284	4651	0.389	ng	99
23) Atrazine	16.519	200	2574	0.347	ng	# 88
24) Pentachlorophenol	16.692	266	1215	0.384	ng	98
25) Phenanthrene	17.077	178	19294	0.379	ng	100
26) Anthracene	17.177	178	15061	0.358	ng	100
28) Fluoranthene	19.107	202	22571	0.370	ng	100
30) Pyrene	19.469	202	22971	0.382	ng	100
32) Benzo(a)anthracene	21.222	228	19822	0.367	ng	99
33) Chrysene	21.276	228	22430	0.382	ng	99
34) Bis(2-ethylhexyl)phtha...	21.159	149	8569	0.347	ng	98
36) Indeno(1,2,3-cd)pyrene	25.688	276	27858	0.379	ng	98
37) Benzo(b)fluoranthene	22.787	252	25609	0.393	ng	96
38) Benzo(k)fluoranthene	22.831	252	24501	0.384	ng	98
39) Benzo(a)pyrene	23.357	252	21674	0.400	ng	# 94
40) Dibenzo(a,h)anthracene	25.705	278	22098	0.376	ng	100
41) Benzo(g,h,i)perylene	26.366	276	24118	0.373	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030947.D
Acq On : 15 Apr 2024 20:50
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Quant Time: Apr 16 00:17:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 17:03:47 2024
Response via : Initial Calibration

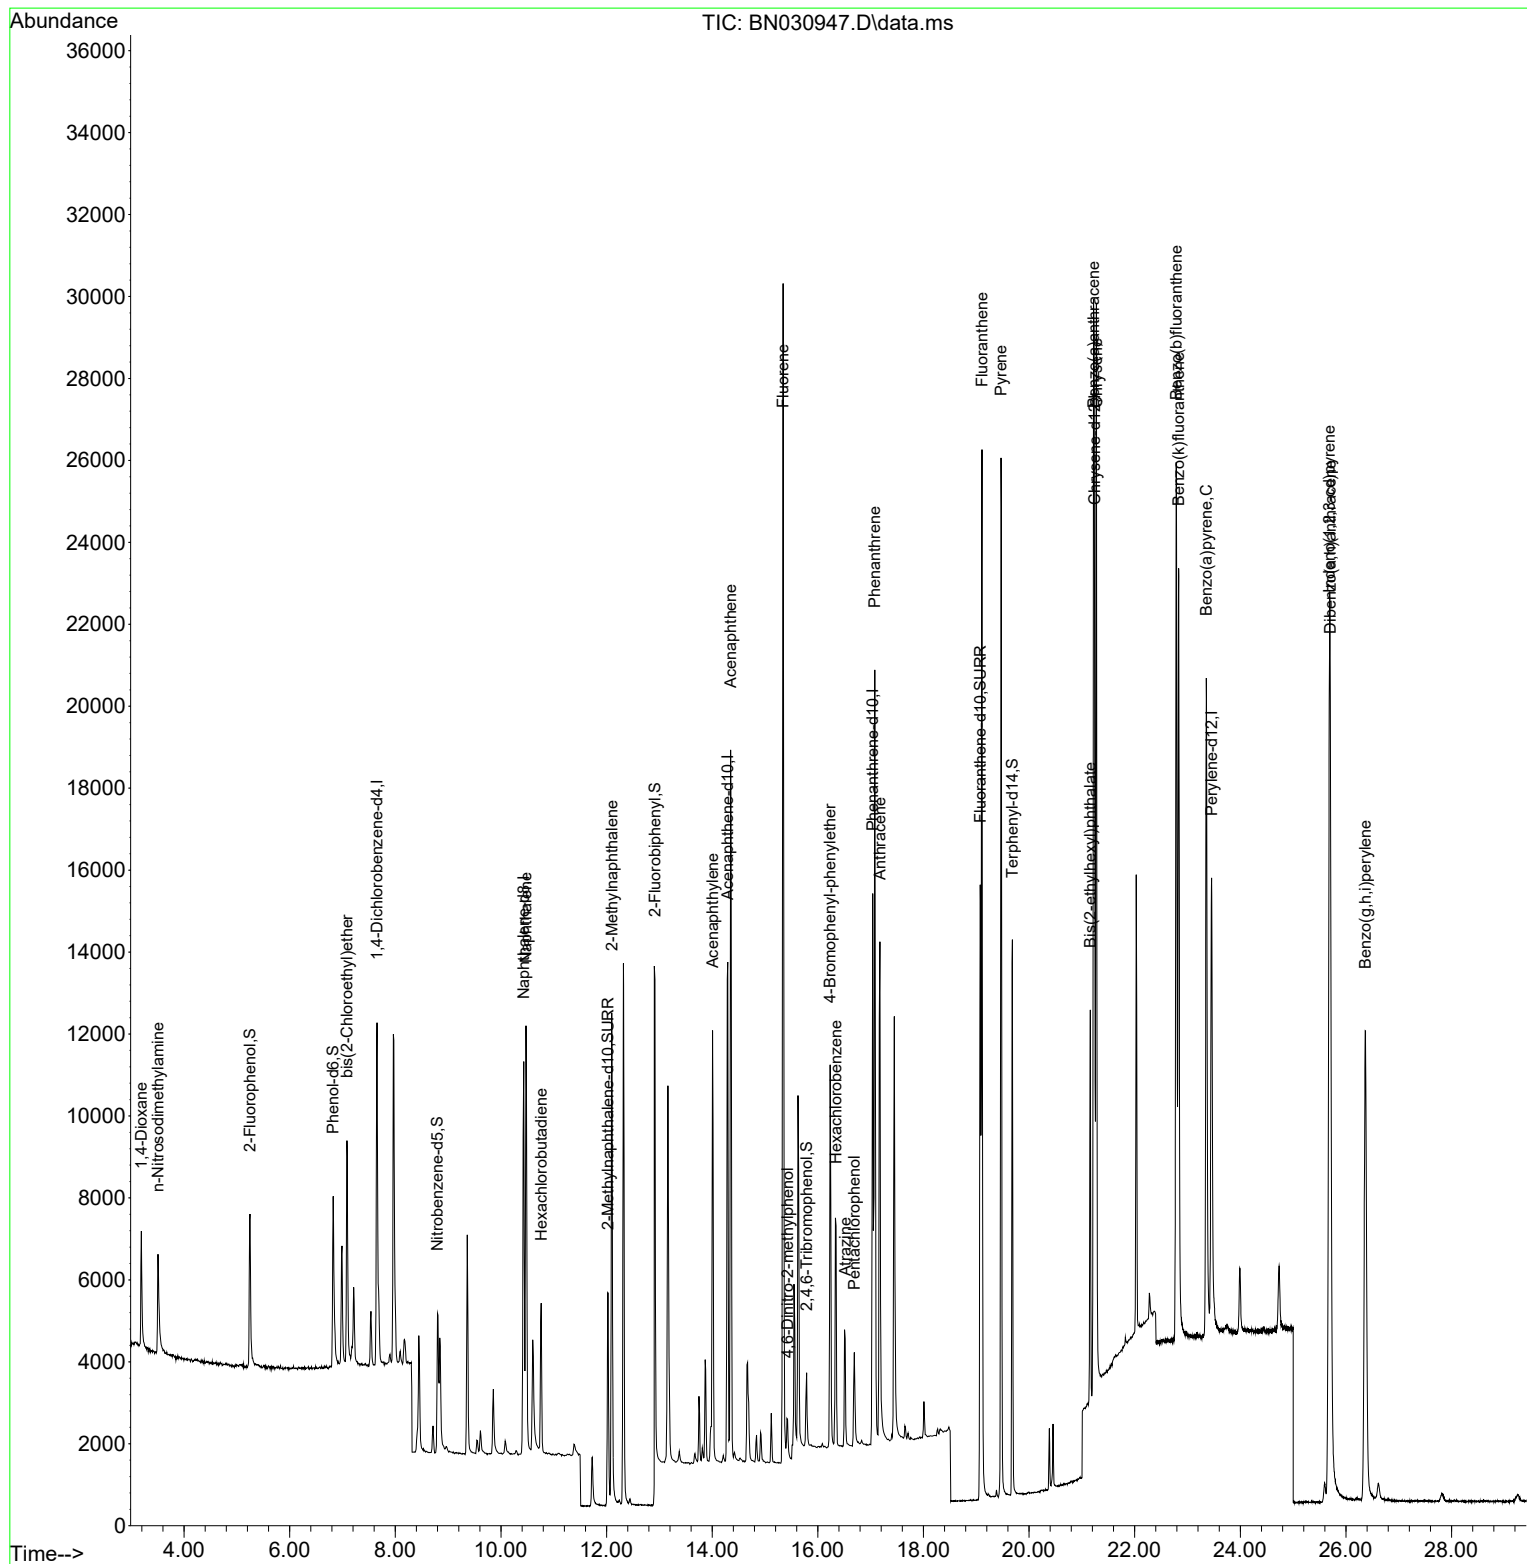






#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.653 min Scan# 64
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC





Tgt Ion:152 Resp: 4376
Ion Ratio Lower Upper
152 100
150 150.4 121.7 182.5
115 59.5 47.8 71.8

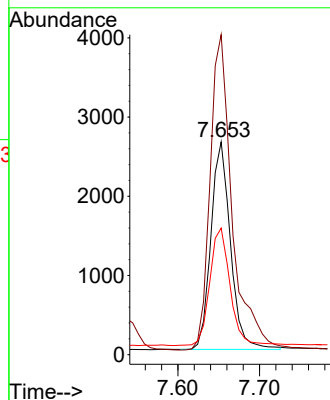


#2
1,4-Dioxane
Concen: 0.370 ng
RT: 3.190 min Scan# 29
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50



Tgt Ion: 88 Resp: 1989
Ion Ratio Lower Upper
88 100
43 30.4 23.7 35.5
58 70.4 55.7 83.5

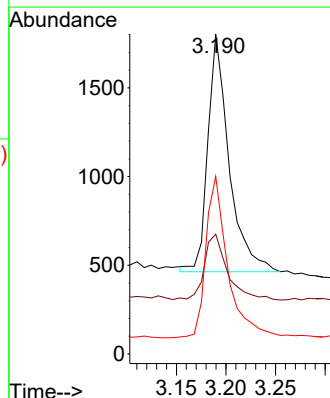



#3

n-Nitrosodimethylamine

Concen: 0.378 ng

RT: 3.507 min Scan# 71

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion: 42 Resp: 1904

Ion Ratio Lower Upper

42 100

74 124.6 103.1 154.7

44 11.9 7.0 10.6#

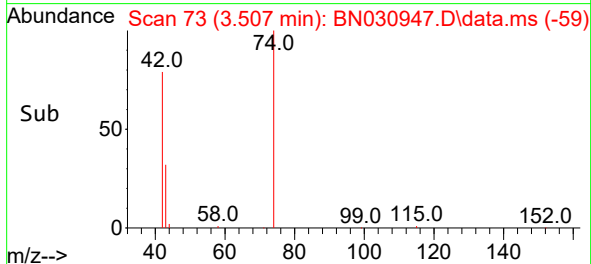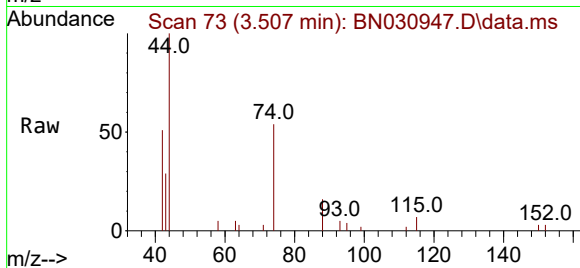

#4

2-Fluorophenol

Concen: 0.375 ng

RT: 5.248 min Scan# 314

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50




Tgt Ion: 112 Resp: 3656


Ion Ratio Lower Upper

112 100

64 53.7 43.4 65.2

63 29.0 22.2 33.2




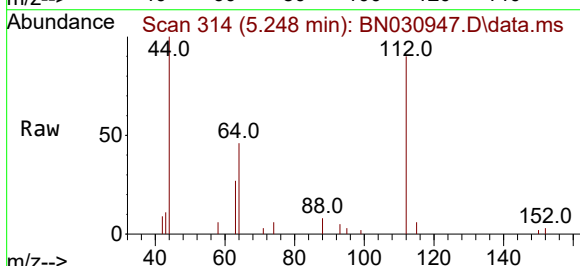




#5
Phenol-d6
Concen: 0.371 ng
RT: 6.822 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 4375
Ion Ratio Lower Upper
99 100
42 19.4 16.4 24.6
71 33.8 26.3 39.5

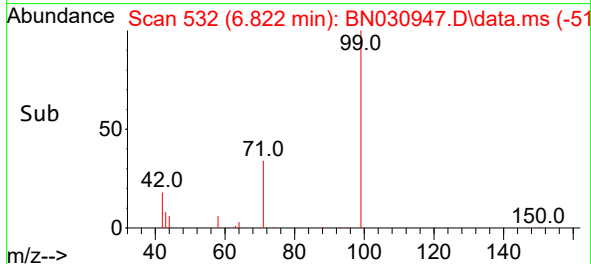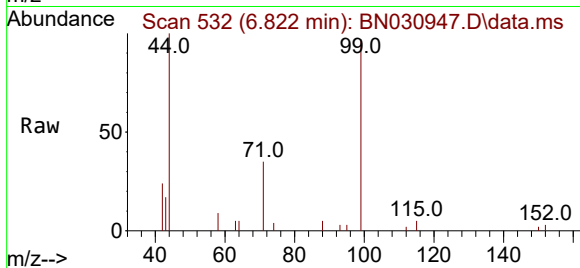

#6
bis(2-Chloroethyl)ether
Concen: 0.364 ng
RT: 7.082 min Scan# 568
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Tgt Ion: 93 Resp: 4245
Ion Ratio Lower Upper
93 100
63 78.3 61.8 92.8
95 35.3 27.4 41.0

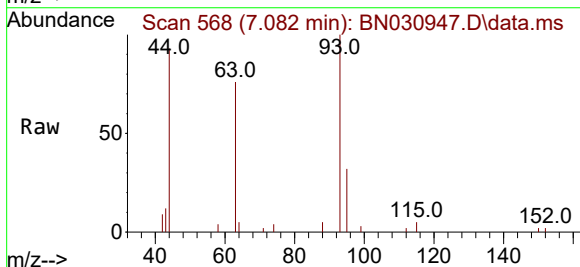



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.431 min Scan# 91

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:136 Resp: 13365





Ion Ratio Lower Upper

136 100

137 11.7 9.4 14.0

54 6.5 5.3 7.9

68 5.6 4.7 7.1



#8

Nitrobenzene-d5

Concen: 0.369 ng

RT: 8.798 min Scan# 784

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50




Tgt Ion: 82 Resp: 3412


Ion Ratio Lower Upper

82 100

128 38.5 33.7 50.5

54 54.5 43.7 65.5









#9
Naphthalene
Concen: 0.384 ng
RT: 10.474 min Scan# 941
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:128 Resp: 14159
Ion Ratio Lower Upper
128 100
129 11.7 9.4 14.0
127 13.6 10.9 16.3

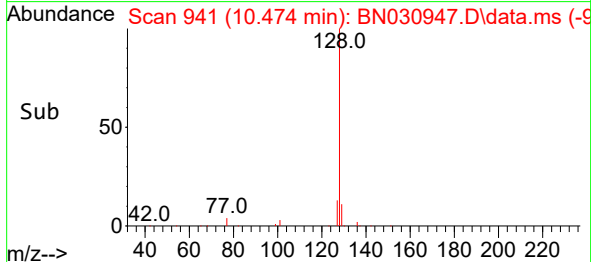

#10
Hexachlorobutadiene
Concen: 0.398 ng
RT: 10.762 min Scan# 968
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Tgt Ion:225 Resp: 2946
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 65.5 51.3 76.9


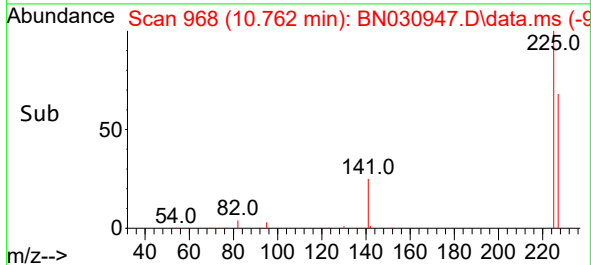






#11
2-Methylnaphthalene-d10
Concen: 0.375 ng
RT: 12.024 min Scan# 1174
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 7705
Ion Ratio Lower Upper
152 100
151 20.9 16.7 25.1

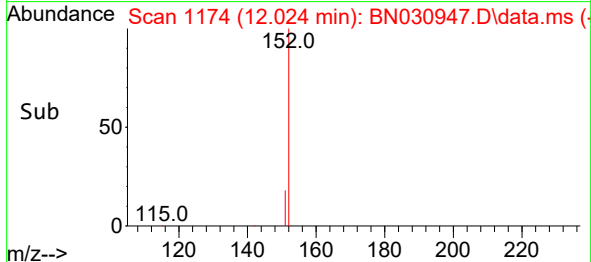

#12
2-Methylnaphthalene
Concen: 0.376 ng
RT: 12.100 min Scan# 1194
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Tgt Ion:142 Resp: 9208
Ion Ratio Lower Upper
142 100
141 88.1 69.8 104.8
115 36.4 28.3 42.5

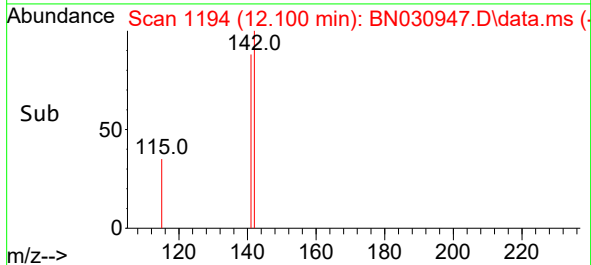



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.295 min Scan# 1537

Delta R.T. -0.000 min

Lab File: BN030947.D


Acq: 15 Apr 2024 20:50

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC






Tgt Ion:164 Resp: 7566

Ion Ratio Lower Upper

164 100

162 102.0 80.6 121.0

160 50.4 40.7 61.1



#14

2,4,6-Tribromophenol

Concen: 0.341 ng

RT: 15.786 min Scan# 1673

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50




Tgt Ion:330 Resp: 1002


Ion Ratio Lower Upper

330 100

332 93.8 74.2 111.2

141 47.7 37.2 55.8







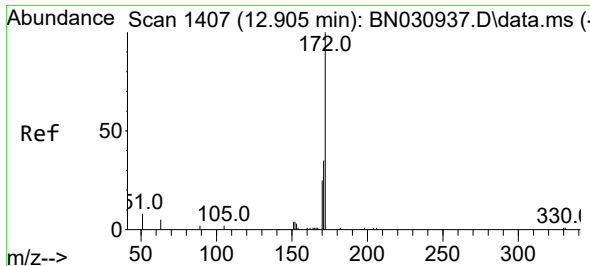

#15
2-Fluorobiphenyl
Concen: 0.400 ng
RT: 12.915 min Scan# 1408
Delta R.T. 0.010 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172 Resp: 10174
Ion Ratio Lower Upper
172 100
171 33.8 28.3 42.5
170 22.8 19.8 29.8

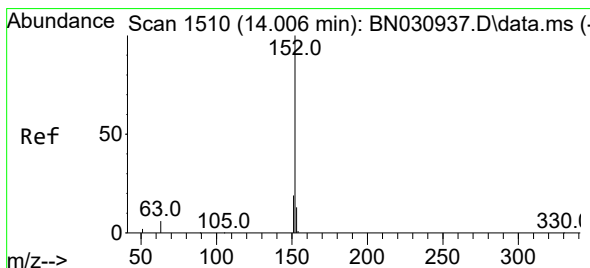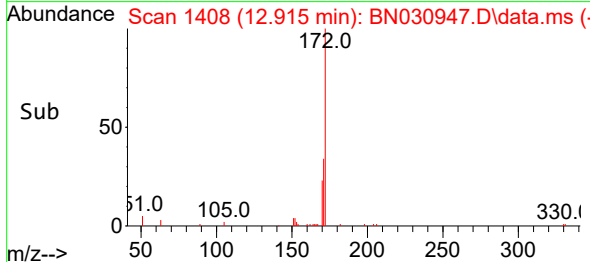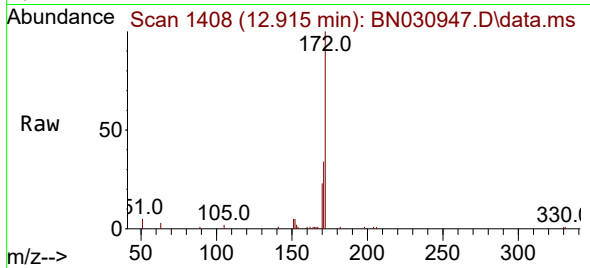

#16
Acenaphthylene
Concen: 0.359 ng
RT: 14.006 min Scan# 1510
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Tgt Ion:152 Resp: 11989
Ion Ratio Lower Upper
152 100
151 19.0 15.3 22.9
153 13.1 10.4 15.6


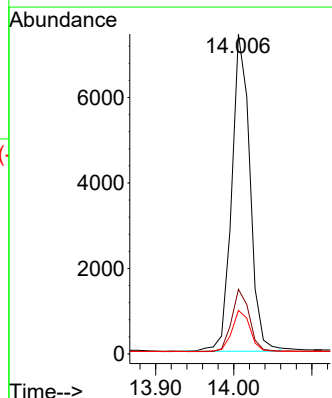
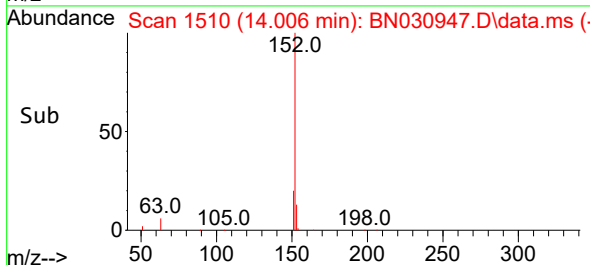
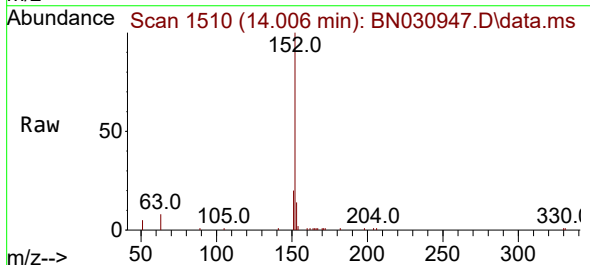




#17
Acenaphthene
Concen: 0.381 ng
RT: 14.348 min Scan# 1542
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 8971
Ion Ratio Lower Upper
154 100
153 113.9 91.1 136.7
152 60.6 47.6 71.4

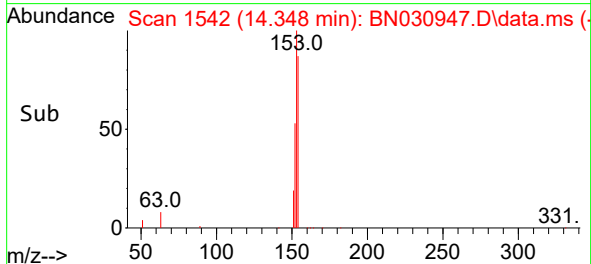

#18
Fluorene
Concen: 0.381 ng
RT: 15.342 min Scan# 1635
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Tgt Ion:166 Resp: 11883
Ion Ratio Lower Upper
166 100
165 97.0 78.3 117.5
167 13.6 11.1 16.7





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.040 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:188 Resp: 17241

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.7 7.4 11.2



#20

4,6-Dinitro-2-methylphenol

Concen: 0.375 ng

RT: 15.428 min Scan# 1643

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50




Tgt Ion:198 Resp: 712


Ion Ratio Lower Upper

198 100

51 85.2 65.2 97.8

105 57.3 41.0 61.4


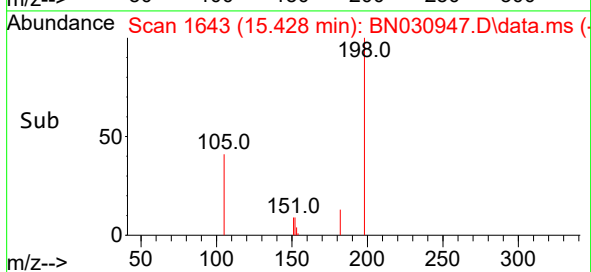






#21
4-Bromophenyl-phenylether
Concen: 0.374 ng
RT: 16.233 min Scan# 1709
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 3832
Ion Ratio Lower Upper
248 100
250 93.5 76.1 114.1
141 92.7 71.1 106.7

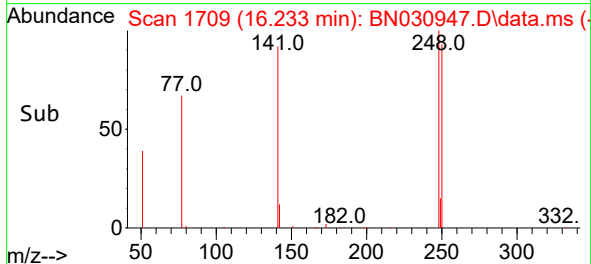

#22
Hexachlorobenzene
Concen: 0.389 ng
RT: 16.345 min Scan# 1718
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Tgt Ion:284 Resp: 4651
Ion Ratio Lower Upper
284 100
142 41.2 33.0 49.4
249 32.8 25.5 38.3


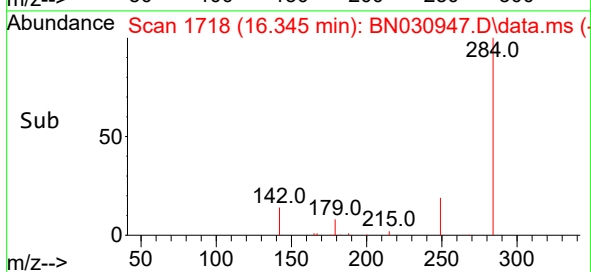

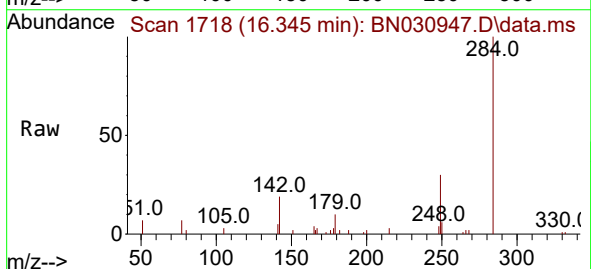




#23
Atrazine
Concen: 0.347 ng
RT: 16.519 min Scan# 1732
Delta R.T. 0.012 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:200 Resp: 2574
Ion Ratio Lower Upper
200 100
173 23.3 29.9 44.9#
215 50.5 38.7 58.1

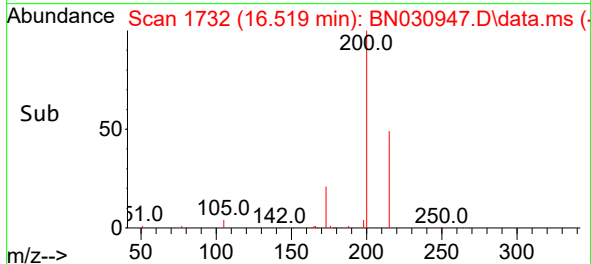

#24
Pentachlorophenol
Concen: 0.384 ng
RT: 16.692 min Scan# 1746
Delta R.T. -0.001 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Tgt Ion:266 Resp: 1215
Ion Ratio Lower Upper
266 100
264 64.2 50.2 75.2
268 64.2 52.3 78.5





#25

Phenanthrene

Concen: 0.379 ng

RT: 17.077 min Scan# 1777

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:178 Resp: 19294

Ion Ratio Lower Upper

178 100

176 19.0 15.1 22.7

179 15.1 12.2 18.2

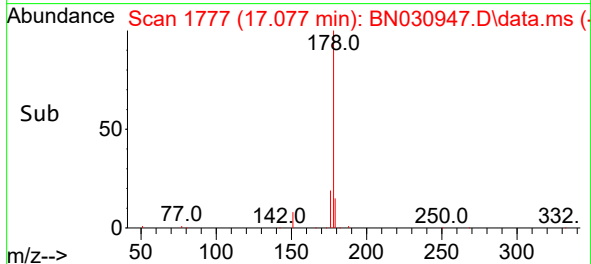

#26

Anthracene

Concen: 0.358 ng

RT: 17.177 min Scan# 1785

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50




Tgt Ion:178 Resp: 15061


Ion Ratio Lower Upper

178 100

176 18.1 14.6 22.0

179 15.5 12.3 18.5




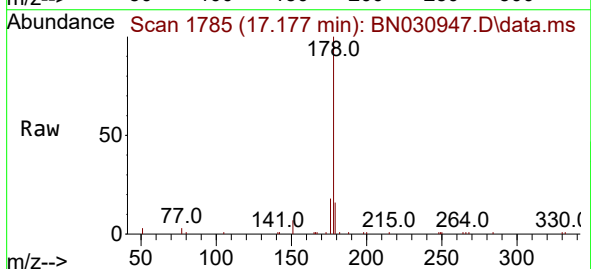




#27
Fluoranthene-d10
Concen: 0.372 ng
RT: 19.075 min Scan# 2014
Delta R.T. -0.005 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 17274
Ion Ratio Lower Upper
212 100
106 14.9 12.0 18.0
104 8.4 6.7 10.1

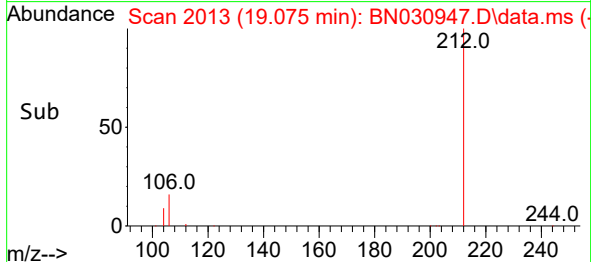

#28
Fluoranthene
Concen: 0.370 ng
RT: 19.107 min Scan# 2020
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Tgt Ion:202 Resp: 22571
Ion Ratio Lower Upper
202 100
101 11.8 9.4 14.2
203 17.2 13.8 20.8

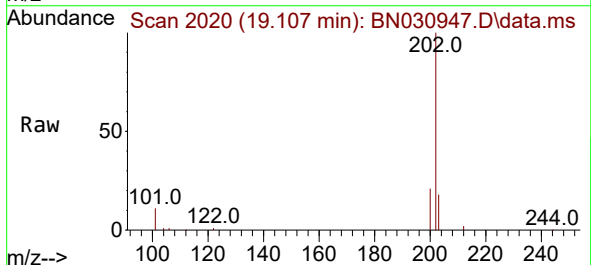



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.240 min Scan# 2455

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:240 Resp: 15488

Ion Ratio Lower Upper

240 100

120 10.5 11.0 16.4#

236 27.3 22.3 33.5

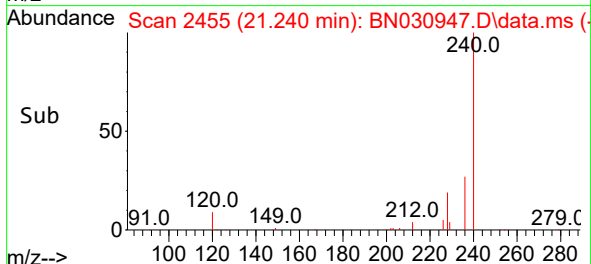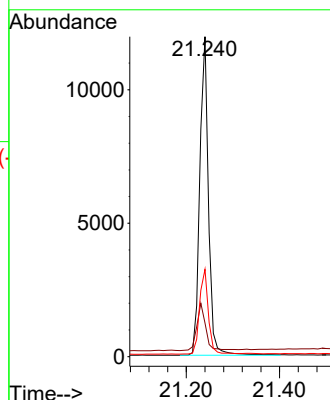

#30

Pyrene

Concen: 0.382 ng

RT: 19.469 min Scan# 2098

Delta R.T. -0.005 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50




Tgt Ion:202 Resp: 22971


Ion Ratio Lower Upper

202 100

200 20.7 16.6 25.0

203 18.0 14.3 21.5



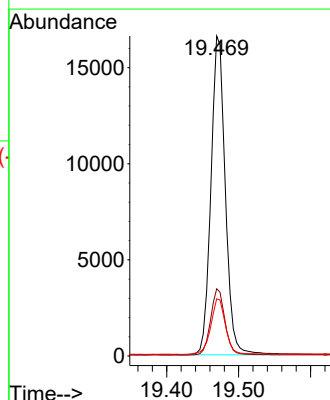





#31
 Terphenyl-d14
 Concen: 0.378 ng
 RT: 19.683 min Scan# 2144
 Delta R.T. -0.000 min
 Lab File: BN030947.D
 Acq: 15 Apr 2024 20:50




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:244 Resp: 13600
 Ion Ratio Lower Upper
 244 100
 212 8.6 7.2 10.8
 122 14.6 12.7 19.1

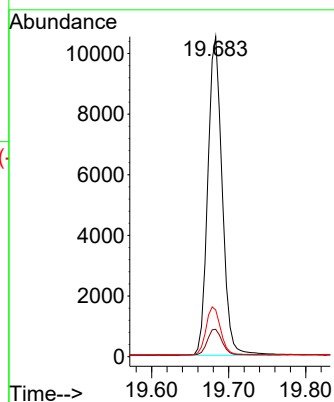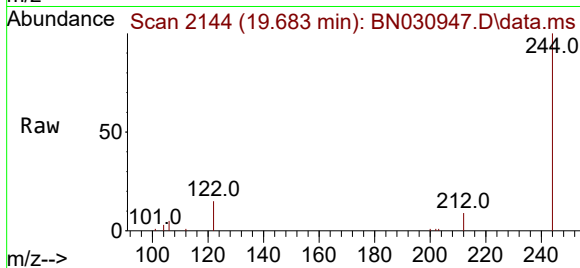

#32
 Benzo(a)anthracene
 Concen: 0.367 ng
 RT: 21.222 min Scan# 2453
 Delta R.T. -0.000 min
 Lab File: BN030947.D
 Acq: 15 Apr 2024 20:50

Tgt Ion:228 Resp: 19822
 Ion Ratio Lower Upper
 228 100
 226 27.2 22.4 33.6
 229 19.4 15.7 23.5

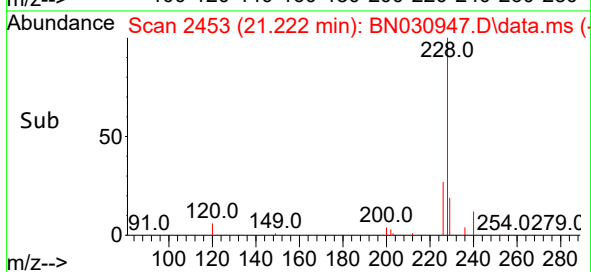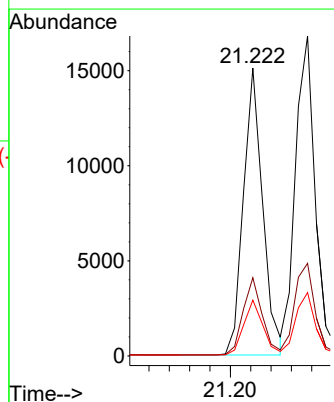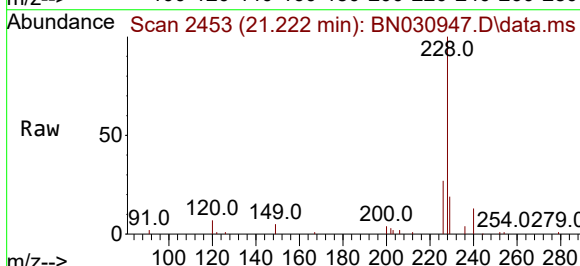

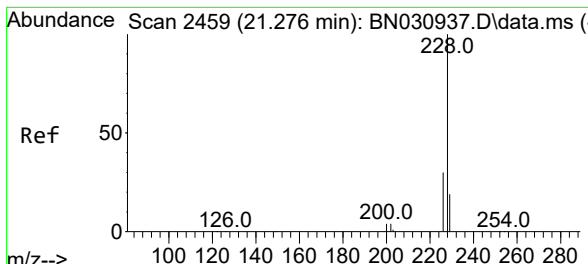

#33

Chrysene

Concen: 0.382 ng

RT: 21.276 min Scan# 2459

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:228 Resp: 22430

Ion Ratio Lower Upper

228 100

226 29.0 23.9 35.9

229 19.8 15.8 23.6

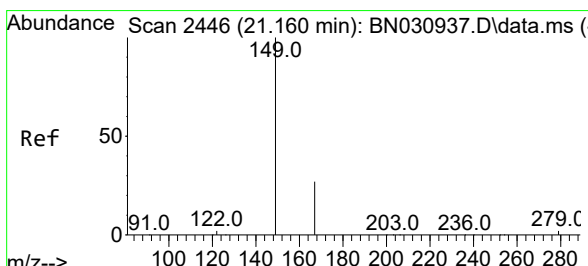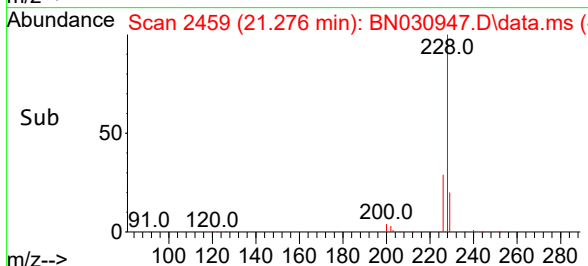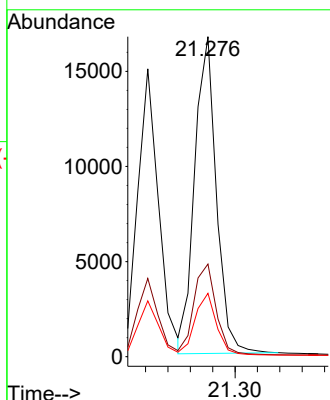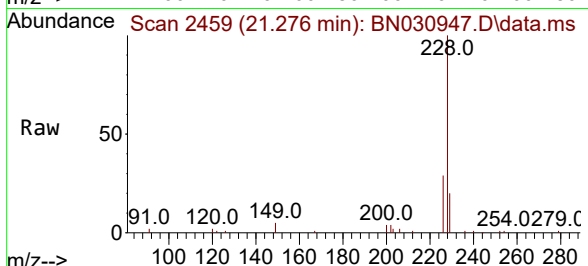

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.347 ng

RT: 21.159 min Scan# 2446

Delta R.T. -0.000 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50




Tgt Ion:149 Resp: 8569


Ion Ratio Lower Upper

149 100

167 27.1 21.0 31.4

279 3.4 2.9 4.3

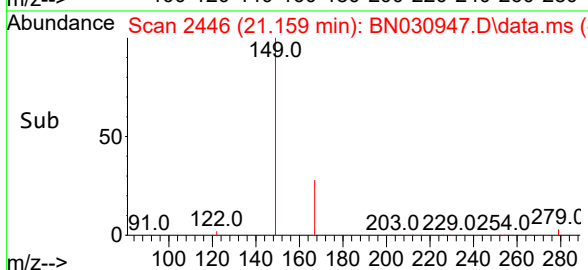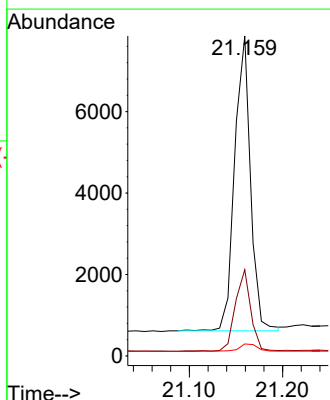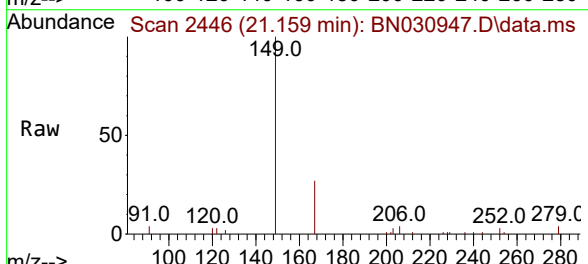



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.457 min Scan# 2945

Delta R.T. -0.003 min

Lab File: BN030947.D


Acq: 15 Apr 2024 20:50

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC






Tgt Ion:264 Resp: 15785

Ion Ratio Lower Upper

264 100

260 25.5 20.6 31.0

265 60.6 53.3 79.9

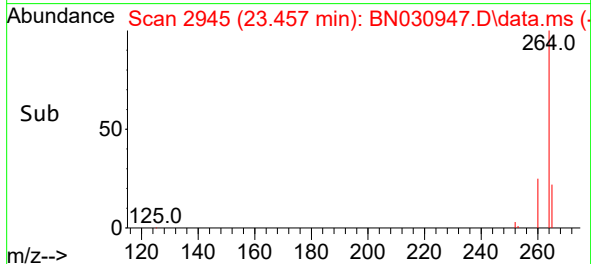

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.379 ng

RT: 25.688 min Scan# 3708

Delta R.T. -0.006 min

Lab File: BN030947.D

Acq: 15 Apr 2024 20:50




Tgt Ion:276 Resp: 27858


Ion Ratio Lower Upper

276 100

138 27.3 23.1 34.7


277 24.8 19.9 29.9







#37
Benzo(b)fluoranthene
Concen: 0.393 ng
RT: 22.787 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:252 Resp: 25609
Ion Ratio Lower Upper
252 100
253 24.2 20.2 30.2
125 19.9 13.4 20.2



#38
Benzo(k)fluoranthene
Concen: 0.384 ng
RT: 22.831 min Scan# 2731
Delta R.T. -0.006 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50


Tgt Ion:252 Resp: 24501
Ion Ratio Lower Upper
252 100
253 24.0 19.9 29.9
125 15.5 13.2 19.8








#39
Benzo(a)pyrene
Concen: 0.400 ng
RT: 23.357 min Scan# 2911
Delta R.T. -0.006 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:252 Resp: 21674
Ion Ratio Lower Upper
252 100
253 26.0 21.4 32.2
125 26.3 16.6 25.0#

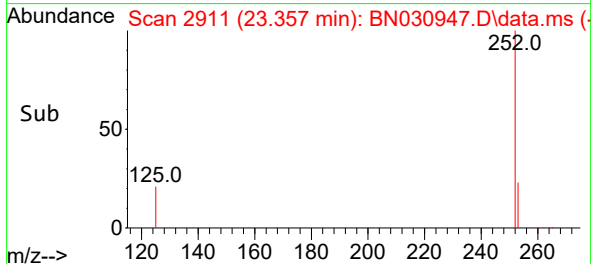

#40
Dibenzo(a,h)anthracene
Concen: 0.376 ng
RT: 25.705 min Scan# 3714
Delta R.T. -0.000 min
Lab File: BN030947.D
Acq: 15 Apr 2024 20:50

Tgt Ion:278 Resp: 22098
Ion Ratio Lower Upper
278 100
139 20.4 16.3 24.5
279 25.7 20.6 31.0



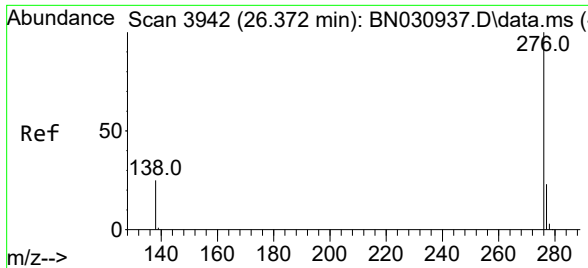

#41

Benzo(g,h,i)perylene

Concen: 0.373 ng

RT: 26.366 min Scan# 3940

Delta R.T. -0.006 min

Lab File: BN030947.D


Acq: 15 Apr 2024 20:50

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

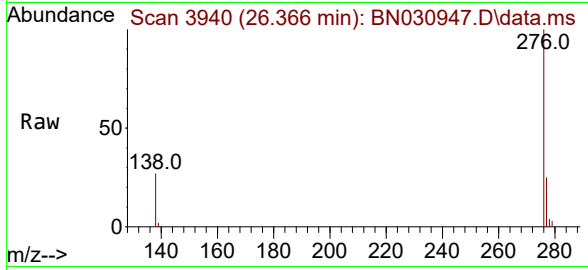

Tgt Ion:276 Resp: 24118

Ion Ratio Lower Upper

276 100

277 24.6 19.4 29.2

138 26.5 21.0 31.4

