
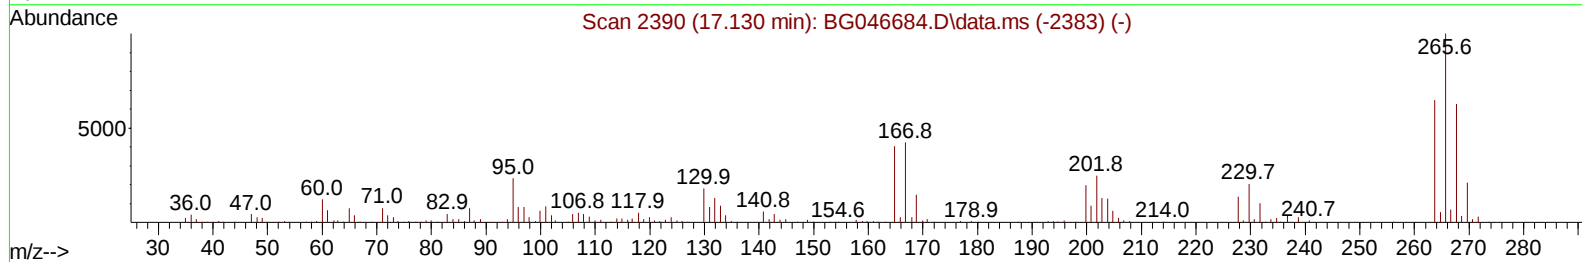
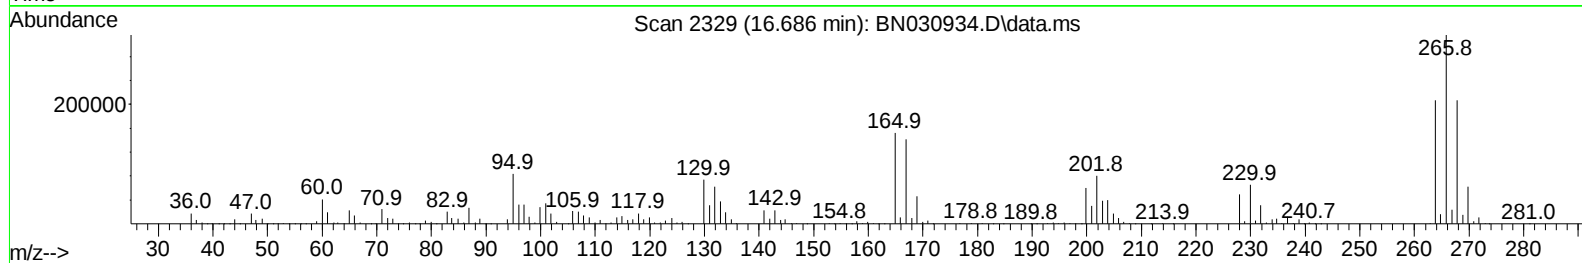


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030934.D
Acq On : 15 Apr 2024 12:03
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 00:45:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 16 00:44:54 2024
Response via : Initial Calibration

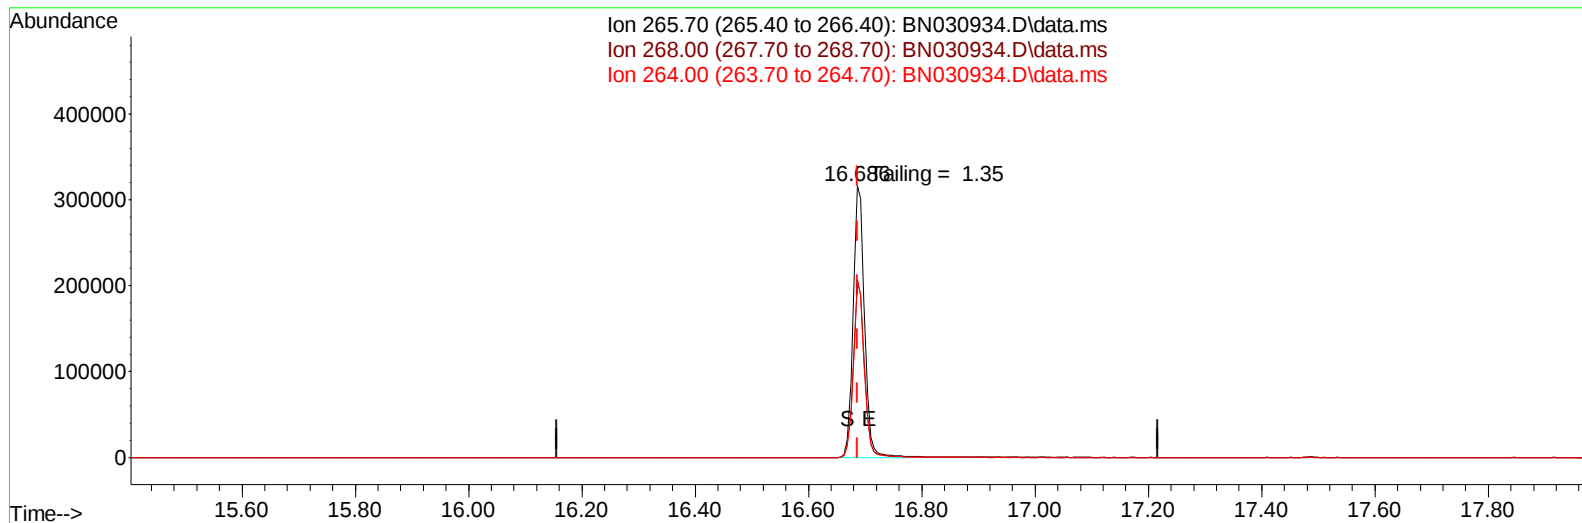




TIC: BN030934.D\data.ms

(70) Pentachlorophenol (C)**16.686min (0.000) 22475.35 ng****response 446420**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.28
264.00	61.60	65.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030934.D
Acq On : 15 Apr 2024 12:03
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 00:45:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 16 00:44:54 2024
Response via : Initial Calibration

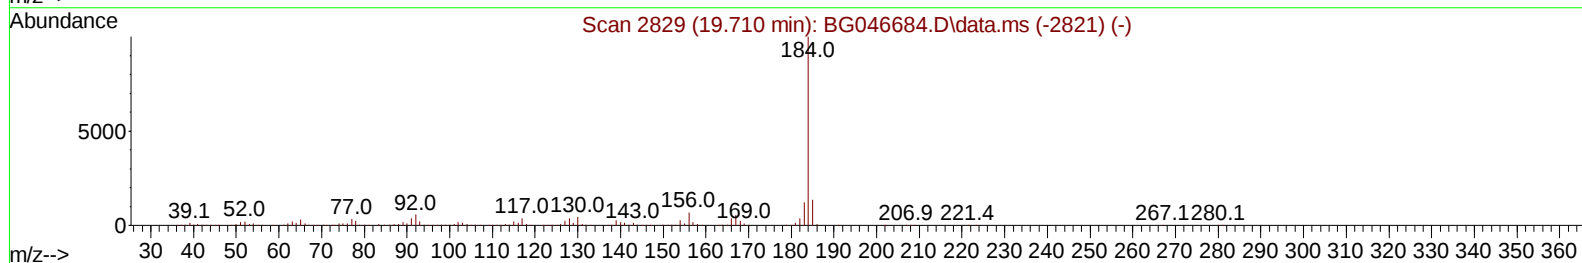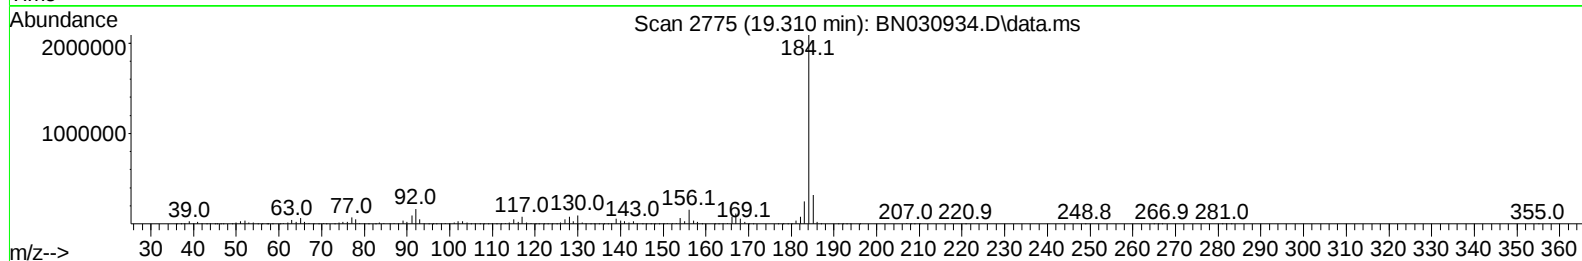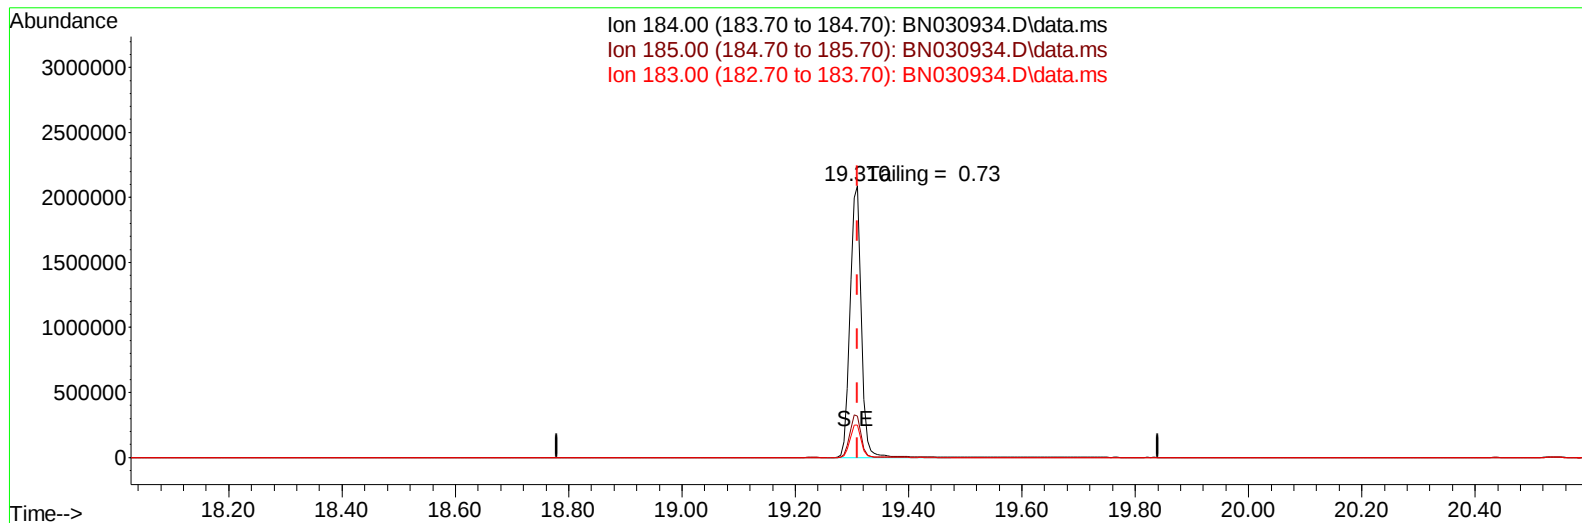

TIC: BN030934.D\data.ms

(77) Benzidine

19.310min (0.000) 0.00 ng

response 2906904

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.30
183.00	13.20	11.98
0.00	0.00	0.00