

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
 Data File : BN030941.D
 Acq On : 15 Apr 2024 16:23
 Operator : MA/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Apr 15 17:14:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 17:03:47 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.653	152	3913	0.400	ng	0.00
7) Naphthalene-d8	10.432	136	11866	0.400	ng	0.00
13) Acenaphthene-d10	14.295	164	7056	0.400	ng	0.00
19) Phenanthrene-d10	17.040	188	15607	0.400	ng	0.00
29) Chrysene-d12	21.240	240	15666	0.400	ng	0.00
35) Perylene-d12	23.460	264	14069	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.241	112	44422	5.095	ng	0.00
5) Phenol-d6	6.823	99	58024	5.496	ng	0.00
8) Nitrobenzene-d5	8.798	82	44246	5.387	ng	0.00
11) 2-Methylnaphthalene-d10	12.024	152	94214	5.158	ng	0.00
14) 2,4,6-Tribromophenol	15.787	330	16381	5.983	ng	0.00
15) 2-Fluorobiphenyl	12.905	172	111718	4.710	ng	0.00
27) Fluoranthene-d10	19.079	212	228845	5.444	ng	0.00
31) Terphenyl-d14	19.683	244	176878	4.864	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.190	88	21178	4.402	ng	99
3) n-Nitrosodimethylamine	3.493	42	23095	5.126	ng	# 98
6) bis(2-Chloroethyl)ether	7.083	93	54194	5.190	ng	96
9) Naphthalene	10.474	128	163268	4.991	ng	98
10) Hexachlorobutadiene	10.763	225	31540	4.801	ng	# 100
12) 2-Methylnaphthalene	12.096	142	111646	5.132	ng	99
16) Acenaphthylene	14.006	152	173070	5.565	ng	100
17) Acenaphthene	14.348	154	112431	5.122	ng	98
18) Fluorene	15.342	166	150412	5.177	ng	99
20) 4,6-Dinitro-2-methylph...	15.428	198	14759	4.995	ng	# 47
21) 4-Bromophenyl-phenylether	16.233	248	48601	5.243	ng	94
22) Hexachlorobenzene	16.345	284	54606	5.043	ng	100
23) Atrazine	16.507	200	38658	5.762	ng	94
24) Pentachlorophenol	16.693	266	25062	4.991	ng	99
25) Phenanthrene	17.078	178	239839	5.207	ng	100
26) Anthracene	17.177	178	216477	5.678	ng	100
28) Fluoranthene	19.107	202	297810	5.390	ng	100
30) Pyrene	19.474	202	304865	5.013	ng	100
32) Benzo(a)anthracene	21.222	228	293487	5.378	ng	99
33) Chrysene	21.276	228	294566	4.965	ng	100
34) Bis(2-ethylhexyl)phtha...	21.160	149	143508	5.739	ng	98
36) Indeno(1,2,3-cd)pyrene	25.694	276	354357	5.415	ng	100
37) Benzo(b)fluoranthene	22.790	252	306813	5.285	ng	# 91
38) Benzo(k)fluoranthene	22.837	252	303378	5.337	ng	# 92
39) Benzo(a)pyrene	23.361	252	261037	5.403	ng	# 87
40) Dibenzo(a,h)anthracene	25.711	278	284479	5.430	ng	96
41) Benzo(g,h,i)perylene	26.375	276	305707	5.299	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030941.D
Acq On : 15 Apr 2024 16:23
Operator : MA/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Apr 15 17:14:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 17:03:47 2024
Response via : Initial Calibration




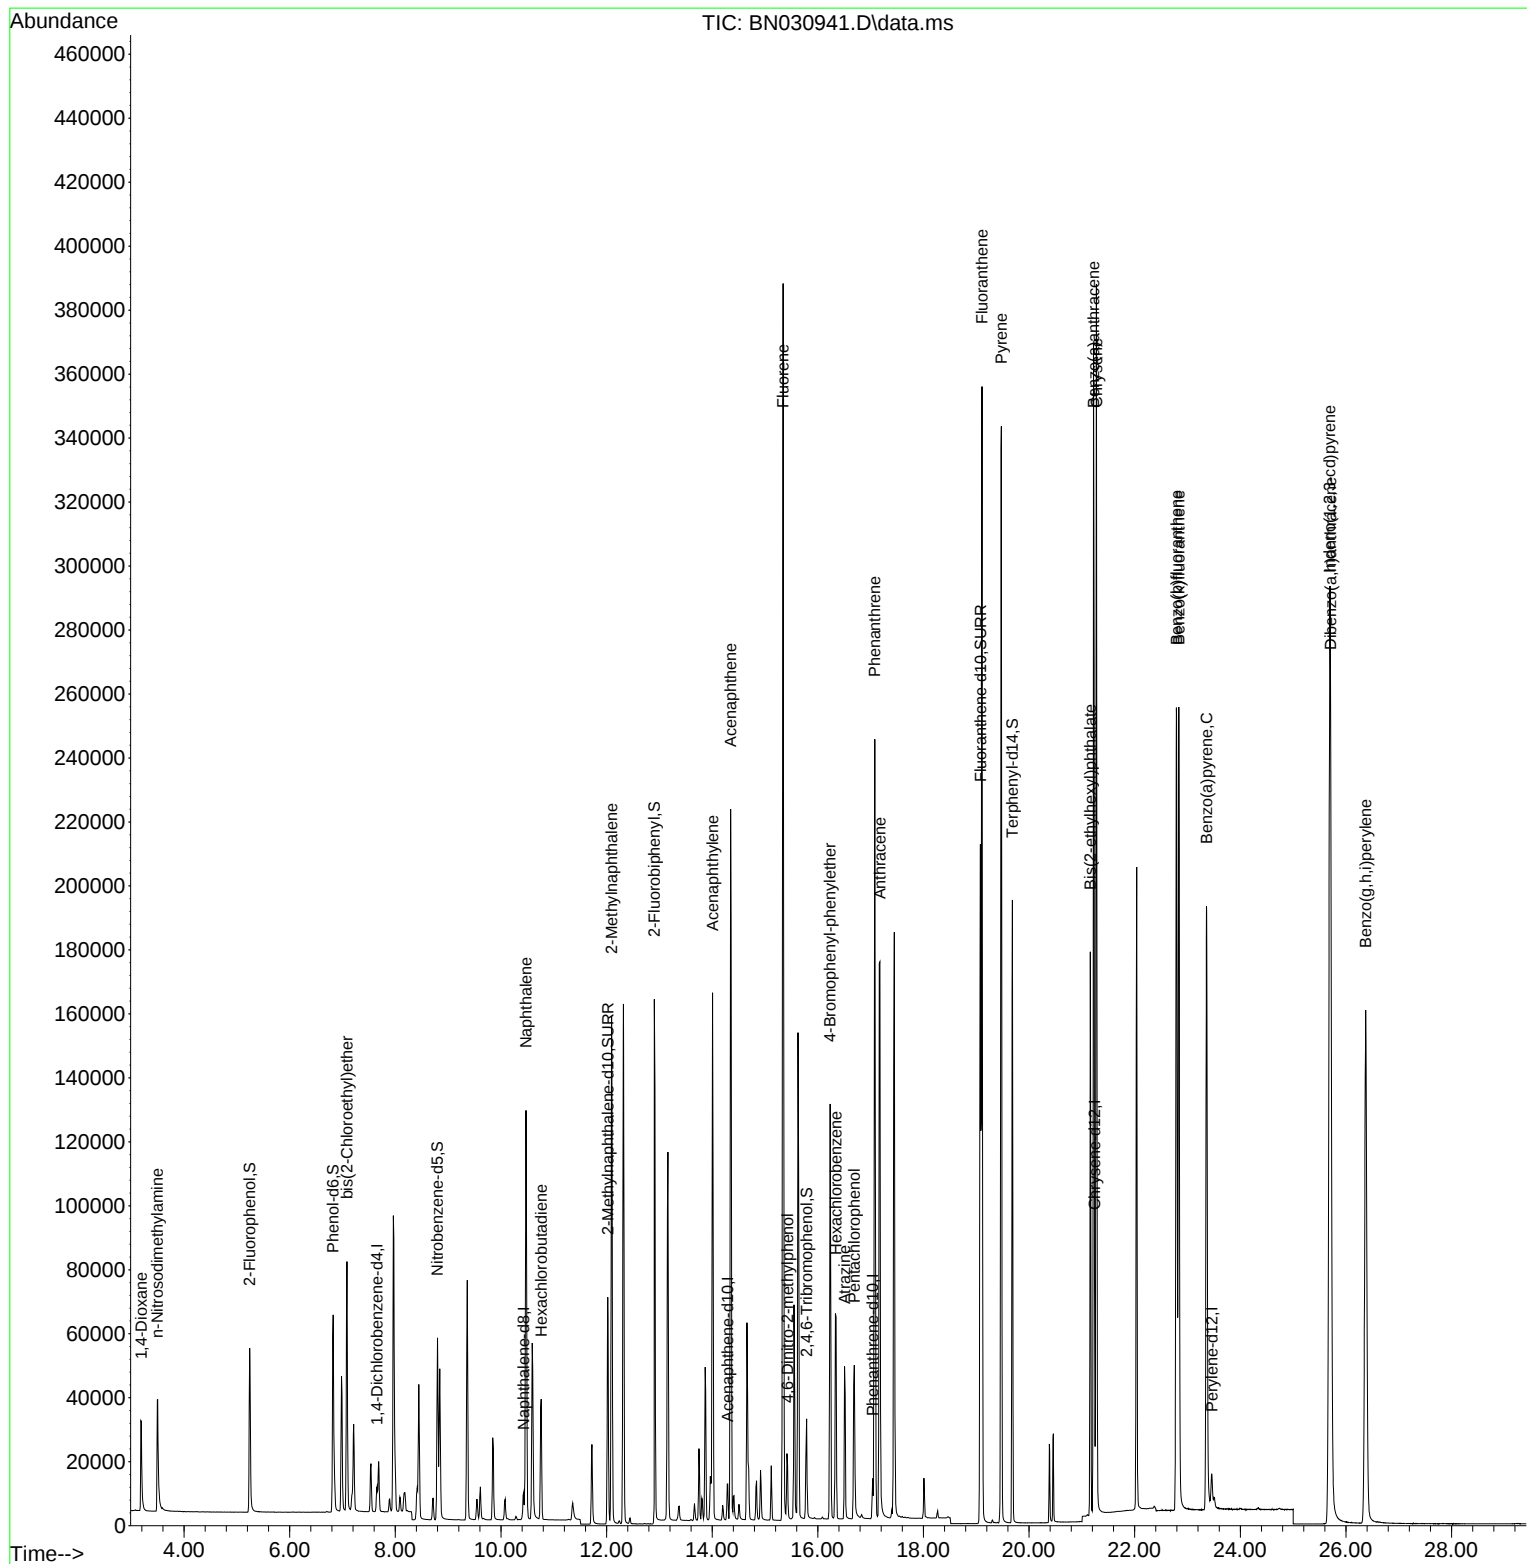


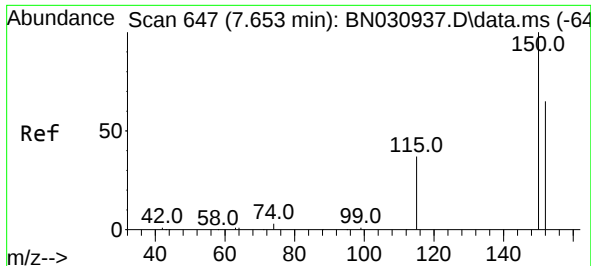

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.653 min Scan# 64
 Delta R.T. 0.000 min
 Lab File: BN030941.D
 Acq: 15 Apr 2024 16:23




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 3913
 Ion Ratio Lower Upper
 152 100
 150 156.3 121.7 182.5
 115 59.0 47.8 71.8

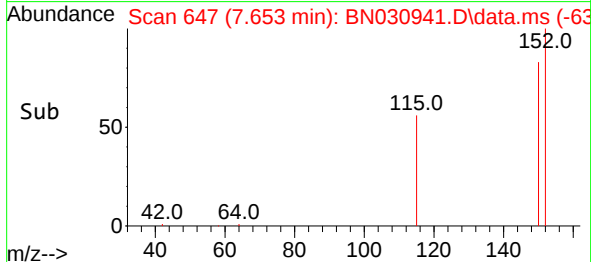

#2
 1,4-Dioxane
 Concen: 4.402 ng
 RT: 3.190 min Scan# 29
 Delta R.T. -0.000 min
 Lab File: BN030941.D
 Acq: 15 Apr 2024 16:23

Tgt Ion: 88 Resp: 21178
 Ion Ratio Lower Upper
 88 100
 43 27.6 23.7 35.5
 58 69.5 55.7 83.5




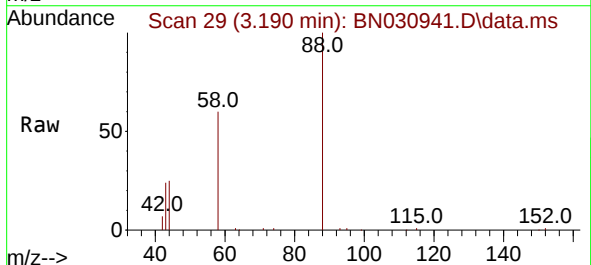




#3
n-Nitrosodimethylamine
Concen: 5.126 ng
RT: 3.493 min Scan# 71
Delta R.T. -0.015 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 23095
Ion Ratio Lower Upper
42 100
74 127.3 103.1 154.7
44 6.4 7.0 10.6#

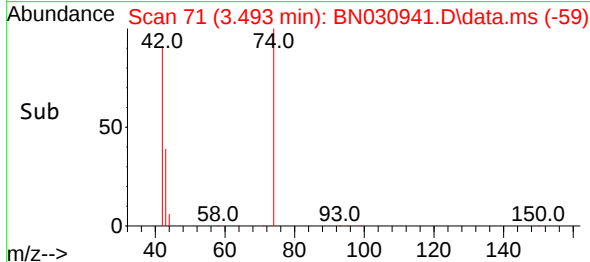

#4
2-Fluorophenol
Concen: 5.095 ng
RT: 5.241 min Scan# 313
Delta R.T. -0.007 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion: 112 Resp: 44422
Ion Ratio Lower Upper
112 100
64 53.1 43.4 65.2
63 27.9 22.2 33.2


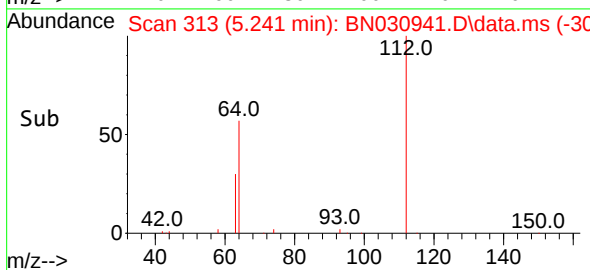

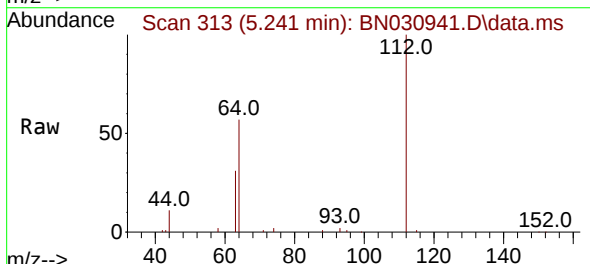




#5
Phenol-d6
Concen: 5.496 ng
RT: 6.823 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 58024
Ion Ratio Lower Upper
99 100
42 19.1 16.4 24.6
71 32.5 26.3 39.5

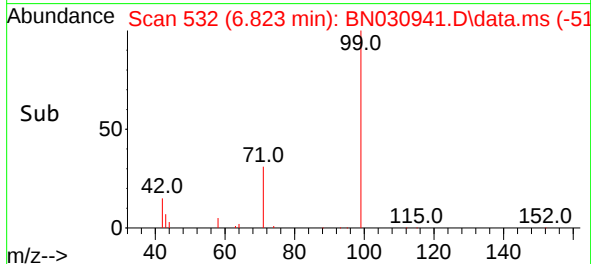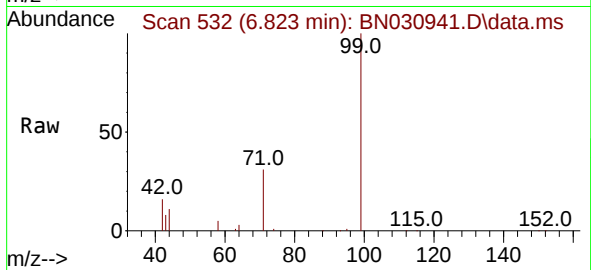

#6
bis(2-Chloroethyl)ether
Concen: 5.190 ng
RT: 7.083 min Scan# 568
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion: 93 Resp: 54194
Ion Ratio Lower Upper
93 100
63 73.5 61.8 92.8
95 33.1 27.4 41.0


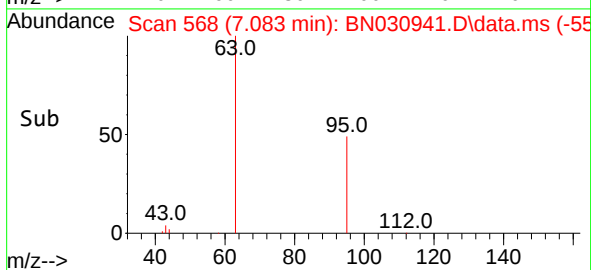




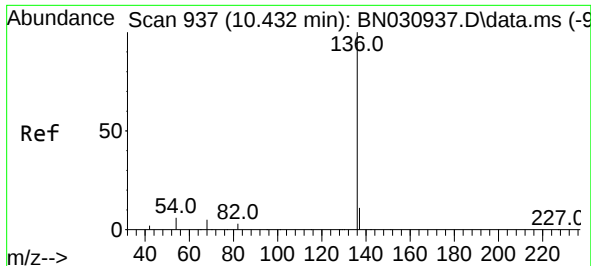

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.432 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	11866
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.4	14.0
54	6.2	5.3	7.9
68	5.6	4.7	7.1

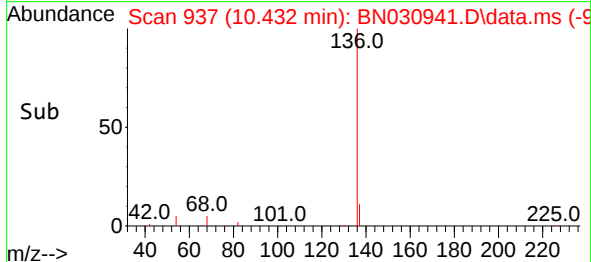

#8
Nitrobenzene-d5
Concen: 5.387 ng
RT: 8.798 min Scan# 784
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:	82	Resp:	44246
Ion	Ratio	Lower	Upper
82	100		
128	40.9	33.7	50.5
54	49.7	43.7	65.5




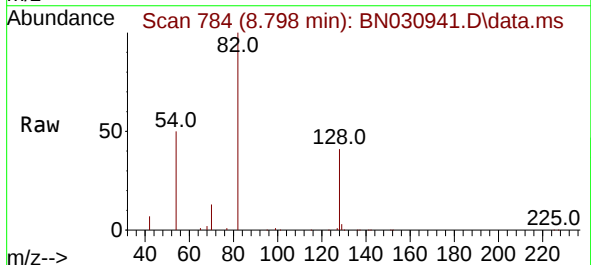


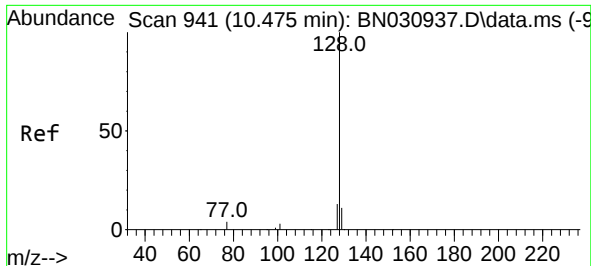

#9
Naphthalene
Concen: 4.991 ng
RT: 10.474 min Scan# 941
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 163268
Ion Ratio Lower Upper
128 100
129 11.0 9.4 14.0
127 13.0 10.9 16.3

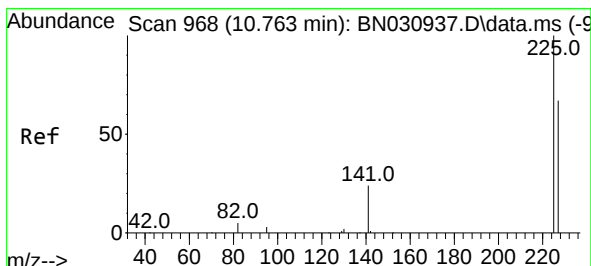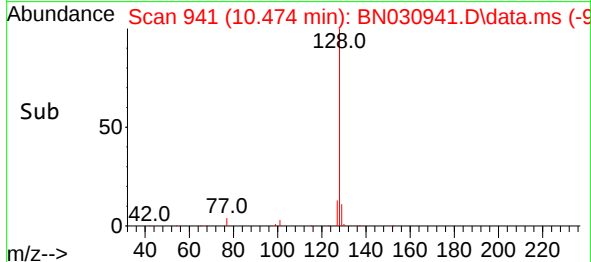

#10
Hexachlorobutadiene
Concen: 4.801 ng
RT: 10.763 min Scan# 968
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:225 Resp: 31540
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.8 51.3 76.9


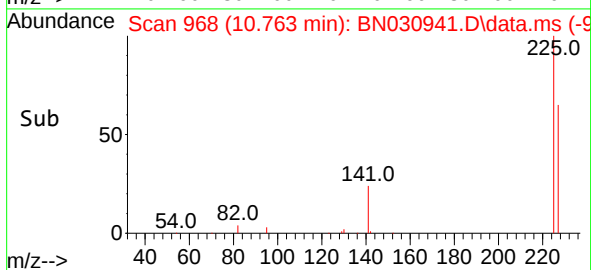

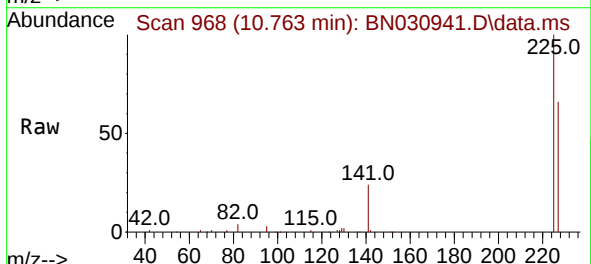




#11
2-Methylnaphthalene-d10
Concen: 5.158 ng
RT: 12.024 min Scan# 1174
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 94214
Ion Ratio Lower Upper
152 100
151 20.7 16.7 25.1

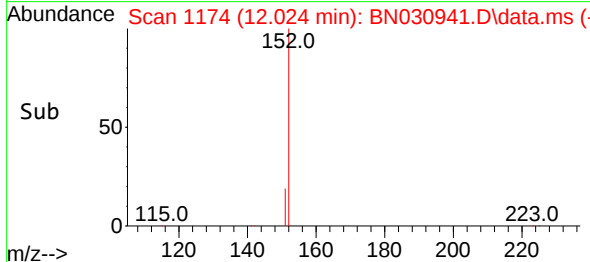

#12
2-Methylnaphthalene
Concen: 5.132 ng
RT: 12.096 min Scan# 1193
Delta R.T. -0.004 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:142 Resp: 111646
Ion Ratio Lower Upper
142 100
141 88.8 69.8 104.8
115 35.2 28.3 42.5


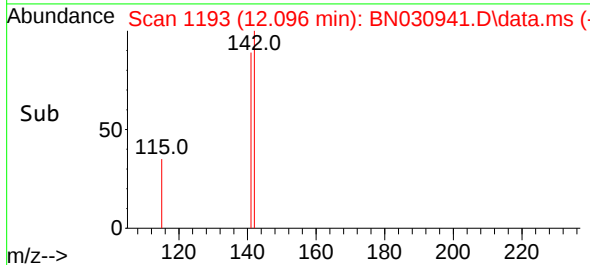

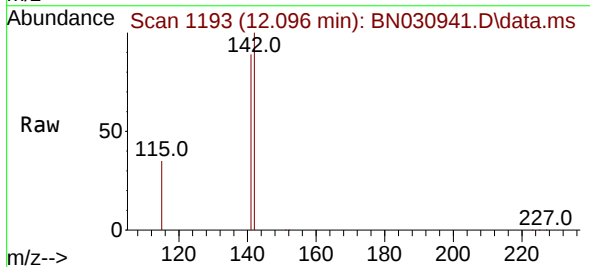




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.295 min Scan# 1537
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 7056
Ion Ratio Lower Upper
164 100
162 99.7 80.6 121.0
160 48.7 40.7 61.1

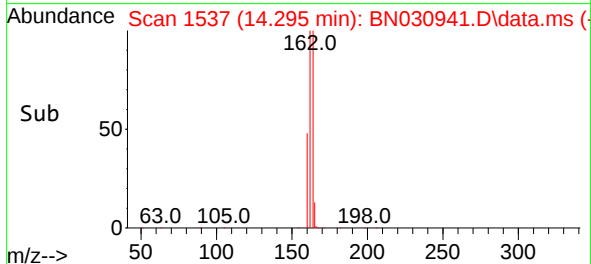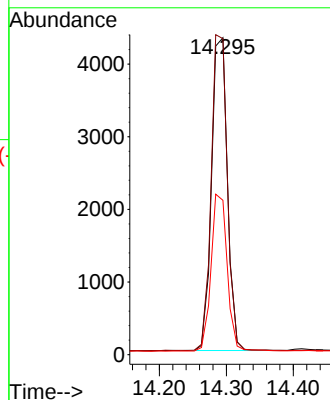

#14
2,4,6-Tribromophenol
Concen: 5.983 ng
RT: 15.787 min Scan# 1673
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:330 Resp: 16381
Ion Ratio Lower Upper
330 100
332 94.4 74.2 111.2
141 46.4 37.2 55.8


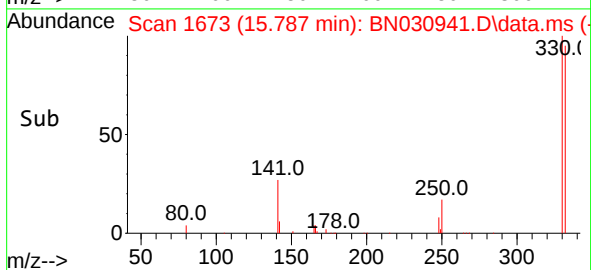
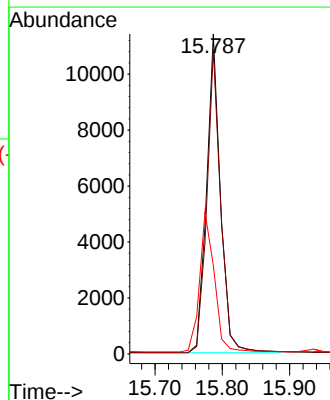





#15
2-Fluorobiphenyl
Concen: 4.710 ng
RT: 12.905 min Scan# 1407
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 111718
Ion Ratio Lower Upper
172 100
171 35.2 28.3 42.5
170 24.2 19.8 29.8

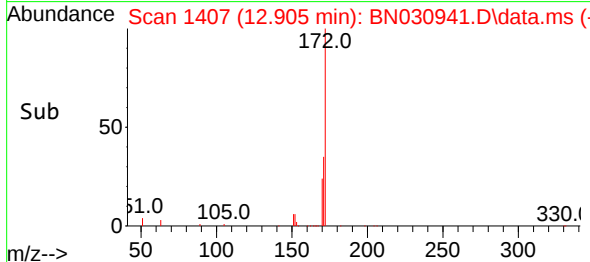

#16
Acenaphthylene
Concen: 5.565 ng
RT: 14.006 min Scan# 1510
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:152 Resp: 173070
Ion Ratio Lower Upper
152 100
151 19.3 15.3 22.9
153 13.0 10.4 15.6


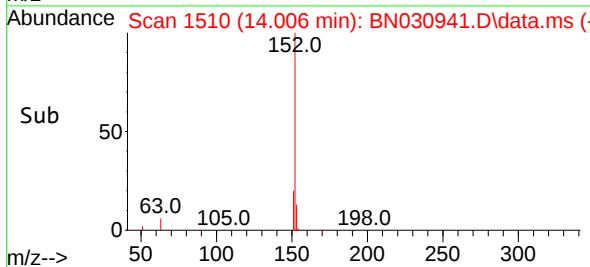

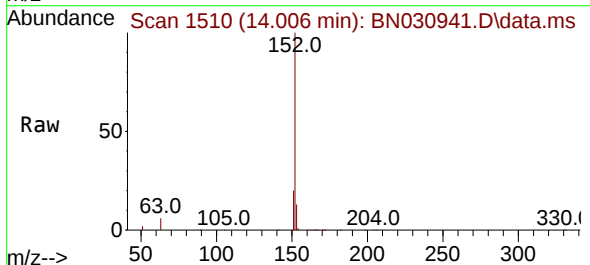


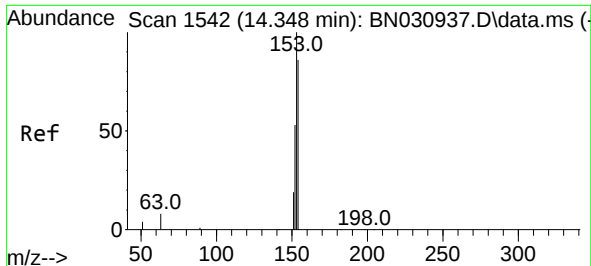

#17
Acenaphthene
Concen: 5.122 ng
RT: 14.348 min Scan# 1542
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 112431
Ion Ratio Lower Upper
154 100
153 112.4 91.1 136.7
152 57.2 47.6 71.4

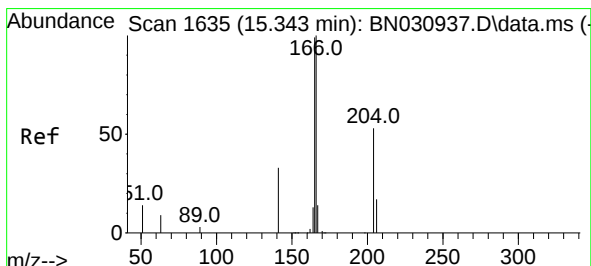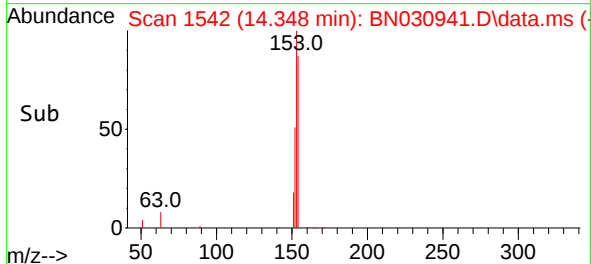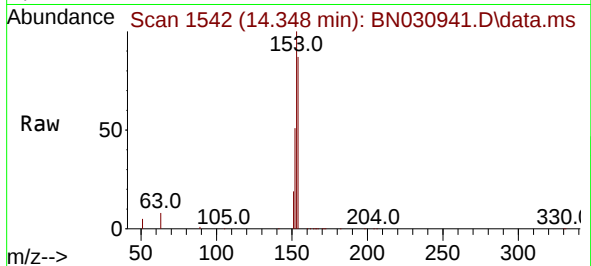

#18
Fluorene
Concen: 5.177 ng
RT: 15.342 min Scan# 1635
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:166 Resp: 150412
Ion Ratio Lower Upper
166 100
165 96.6 78.3 117.5
167 13.5 11.1 16.7


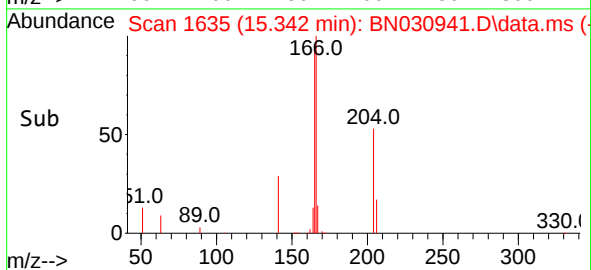

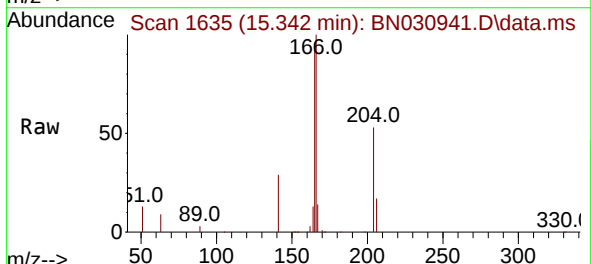




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.040 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 15607
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.2 7.4 11.2

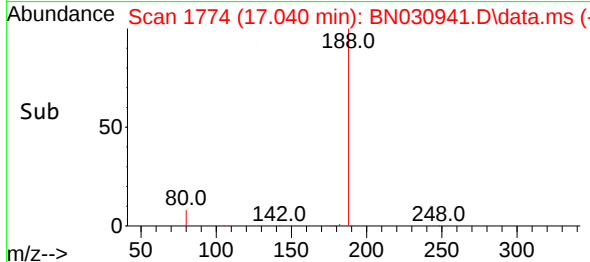

#20
4,6-Dinitro-2-methylphenol
Concen: 4.995 ng
RT: 15.428 min Scan# 1643
Delta R.T. 0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:198 Resp: 14759
Ion Ratio Lower Upper
198 100
51 24.2 65.2 97.8#
105 27.5 41.0 61.4#


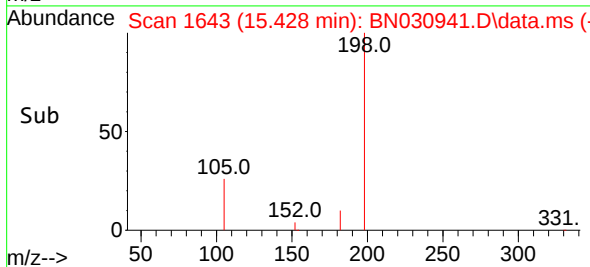

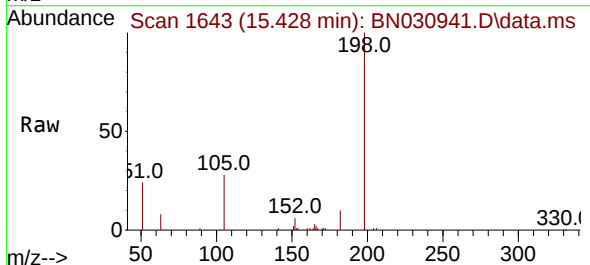




#21
4-Bromophenyl-phenylether
Concen: 5.243 ng
RT: 16.233 min Scan# 1709
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 48601
Ion Ratio Lower Upper
248 100
250 93.2 76.1 114.1
141 80.1 71.1 106.7

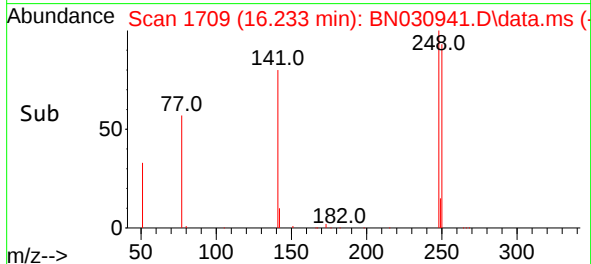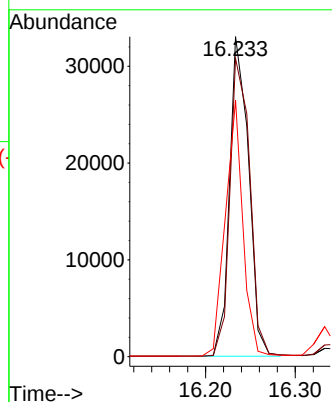

#22
Hexachlorobenzene
Concen: 5.043 ng
RT: 16.345 min Scan# 1718
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:284 Resp: 54606
Ion Ratio Lower Upper
284 100
142 40.7 33.0 49.4
249 31.9 25.5 38.3



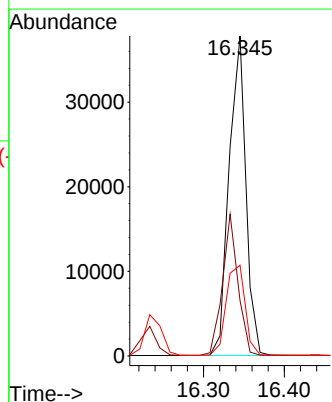





#23
 Atrazine
 Concen: 5.762 ng
 RT: 16.507 min Scan# 1731
 Delta R.T. -0.000 min
 Lab File: BN030941.D
 Acq: 15 Apr 2024 16:23




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:200 Resp: 38658
 Ion Ratio Lower Upper
 200 100
 173 34.1 29.9 44.9
 215 44.4 38.7 58.1

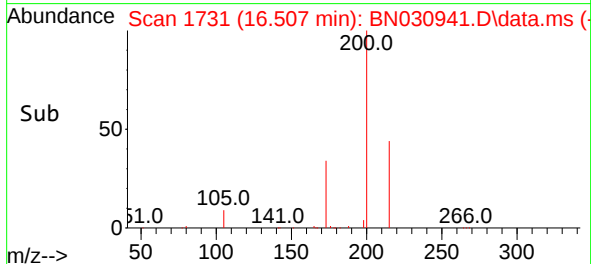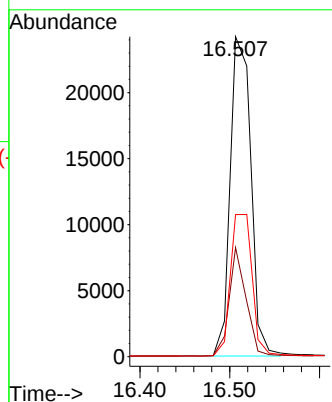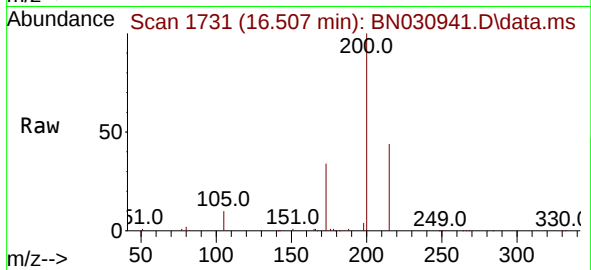

#24
 Pentachlorophenol
 Concen: 4.991 ng
 RT: 16.693 min Scan# 1746
 Delta R.T. -0.000 min
 Lab File: BN030941.D
 Acq: 15 Apr 2024 16:23

Tgt Ion:266 Resp: 25062
 Ion Ratio Lower Upper
 266 100
 264 63.3 50.2 75.2
 268 64.0 52.3 78.5


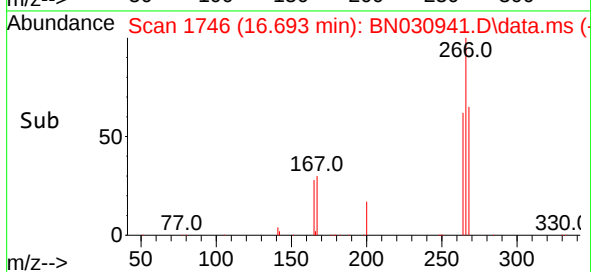
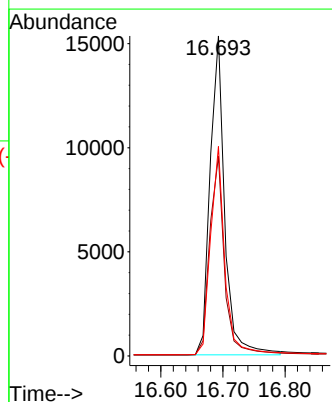
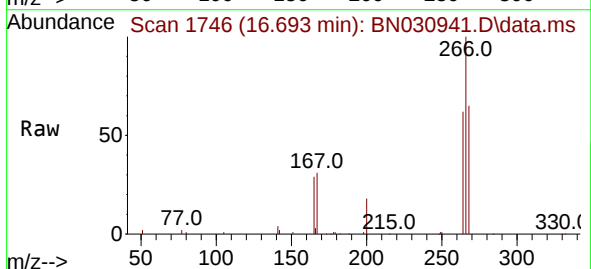




#25
Phenanthrene
Concen: 5.207 ng
RT: 17.078 min Scan# 1777
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 239839
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.2 12.2 18.2

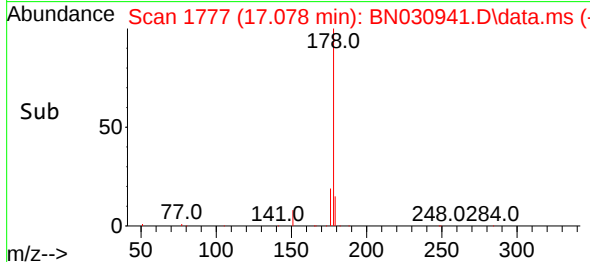

#26
Anthracene
Concen: 5.678 ng
RT: 17.177 min Scan# 1785
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:178 Resp: 216477
Ion Ratio Lower Upper
178 100
176 18.4 14.6 22.0
179 15.3 12.3 18.5


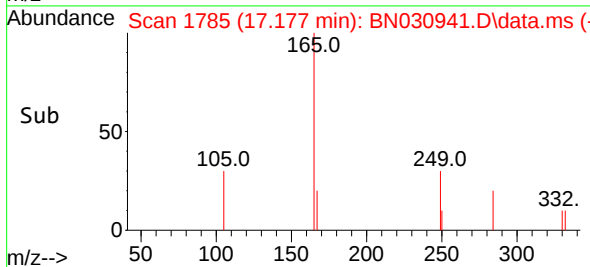

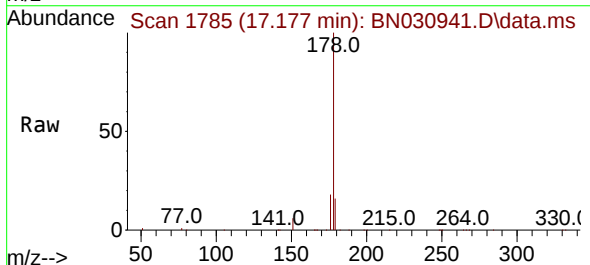




#27
Fluoranthene-d10
Concen: 5.444 ng
RT: 19.079 min Scan# 2014
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 228845
Ion Ratio Lower Upper
212 100
106 14.8 12.0 18.0
104 8.2 6.7 10.1

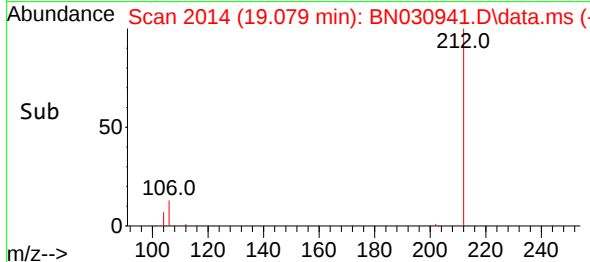

#28
Fluoranthene
Concen: 5.390 ng
RT: 19.107 min Scan# 2020
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:202 Resp: 297810
Ion Ratio Lower Upper
202 100
101 11.7 9.4 14.2
203 17.3 13.8 20.8


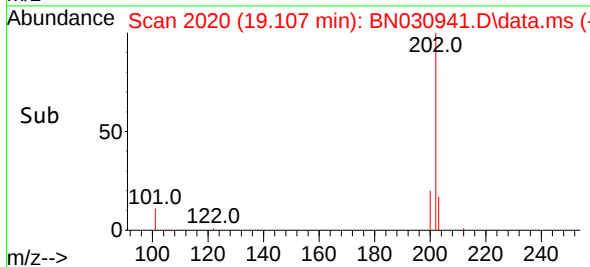

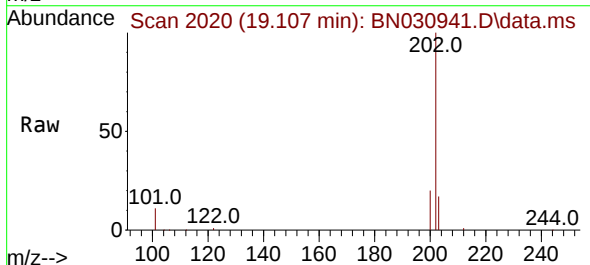




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.240 min Scan# 2455
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 15666
Ion Ratio Lower Upper
240 100
120 13.3 11.0 16.4
236 27.7 22.3 33.5

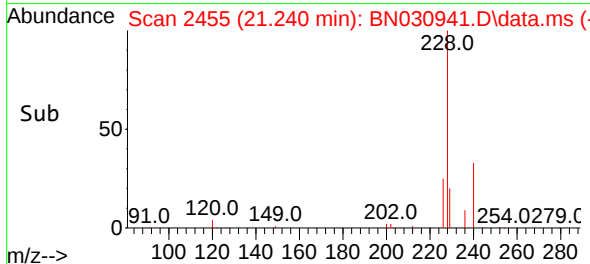

#30
Pyrene
Concen: 5.013 ng
RT: 19.474 min Scan# 2099
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:202 Resp: 304865
Ion Ratio Lower Upper
202 100
200 20.7 16.6 25.0
203 17.8 14.3 21.5


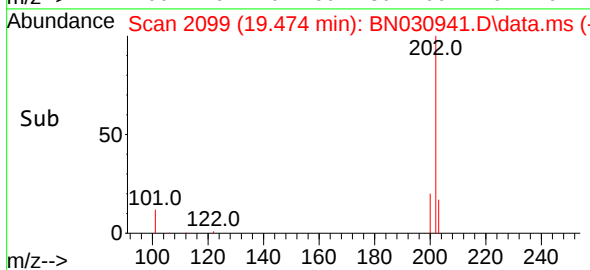

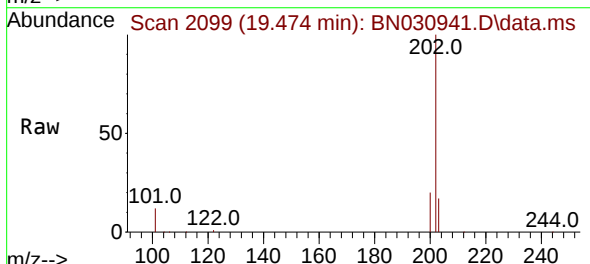




#31
 Terphenyl-d14
 Concen: 4.864 ng
 RT: 19.683 min Scan# 2144
 Delta R.T. -0.000 min
 Lab File: BN030941.D
 Acq: 15 Apr 2024 16:23




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:244 Resp: 176878
 Ion Ratio Lower Upper
 244 100
 212 8.2 7.2 10.8
 122 15.1 12.7 19.1

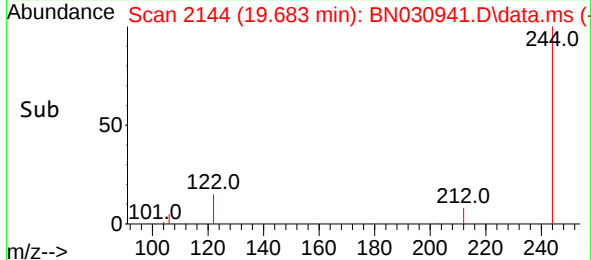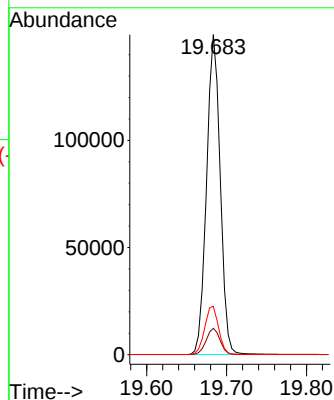

#32
 Benzo(a)anthracene
 Concen: 5.378 ng
 RT: 21.222 min Scan# 2453
 Delta R.T. -0.000 min
 Lab File: BN030941.D
 Acq: 15 Apr 2024 16:23

Tgt Ion:228 Resp: 293487
 Ion Ratio Lower Upper
 228 100
 226 27.3 22.4 33.6
 229 19.2 15.7 23.5



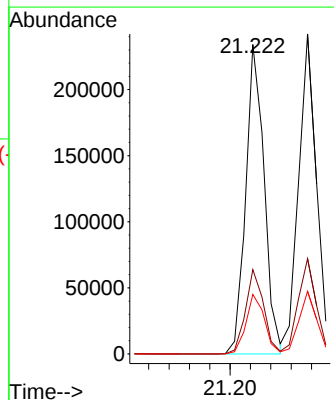
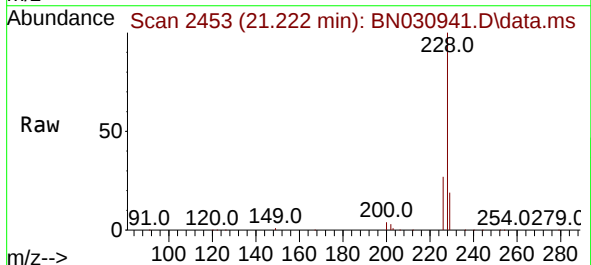




#33
Chrysene
Concen: 4.965 ng
RT: 21.276 min Scan# 2459
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 294566
Ion Ratio Lower Upper
228 100
226 29.8 23.9 35.9
229 19.6 15.8 23.6

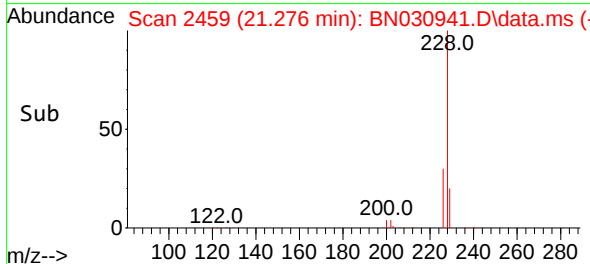

#34
Bis(2-ethylhexyl)phthalate
Concen: 5.739 ng
RT: 21.160 min Scan# 2446
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:149 Resp: 143508
Ion Ratio Lower Upper
149 100
167 27.2 21.0 31.4
279 3.0 2.9 4.3

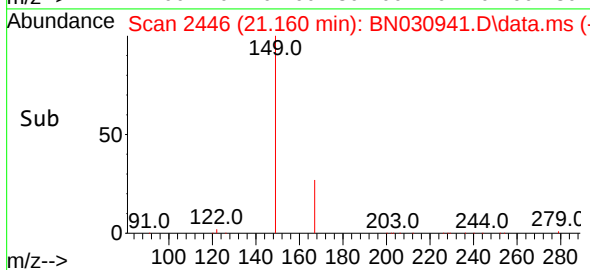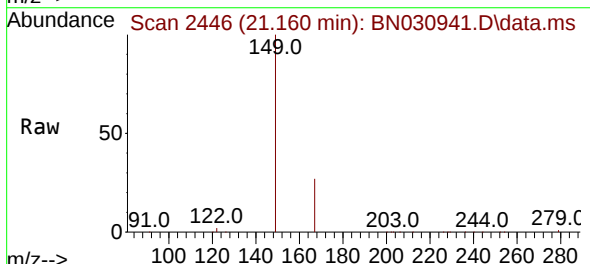




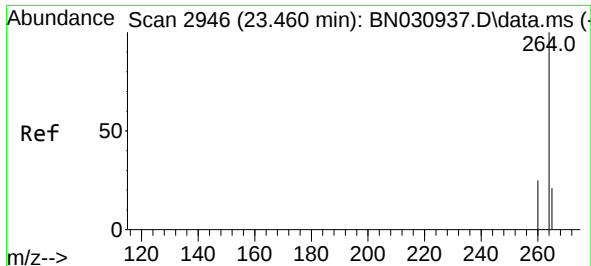


#35
Perylene-d12
Concen: 0.400 ng
RT: 23.460 min Scan# 2946
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:264 Resp: 14069




Ion	Ratio	Lower	Upper
264	100		
260	25.9	20.6	31.0
265	66.6	53.3	79.9

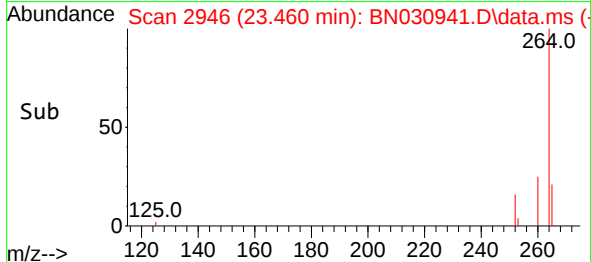


#36
Indeno(1,2,3-cd)pyrene
Concen: 5.415 ng
RT: 25.694 min Scan# 3710
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:276 Resp: 354357

Ion	Ratio	Lower	Upper
276	100		
138	28.9	23.1	34.7
277	24.9	19.9	29.9


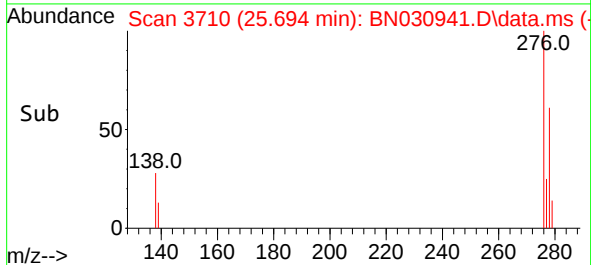




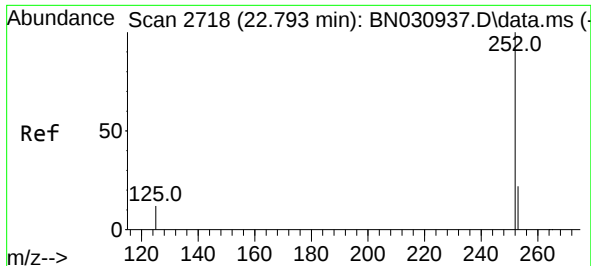

#37
Benzo(b)fluoranthene
Concen: 5.285 ng
RT: 22.790 min Scan# 2718
Delta R.T. -0.003 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 306813
Ion Ratio Lower Upper
252 100
253 21.9 20.2 30.2
125 11.6 13.4 20.2#

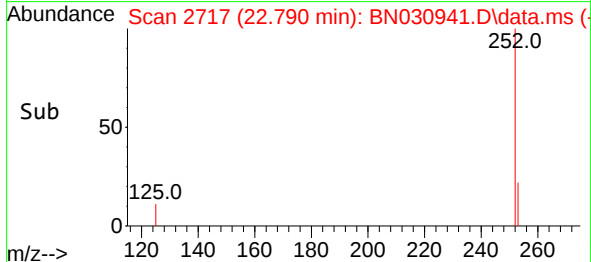

#38
Benzo(k)fluoranthene
Concen: 5.337 ng
RT: 22.837 min Scan# 2733
Delta R.T. -0.000 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:252 Resp: 303378
Ion Ratio Lower Upper
252 100
253 22.0 19.9 29.9
125 11.3 13.2 19.8#


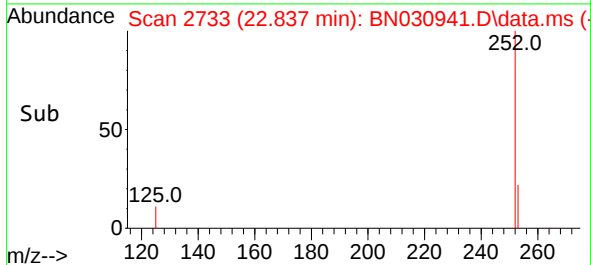






#39
Benzo(a)pyrene
Concen: 5.403 ng
RT: 23.361 min Scan# 2913
Delta R.T. -0.003 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 261037
Ion Ratio Lower Upper
252 100
253 21.8 21.4 32.2
125 12.8 16.6 25.0#

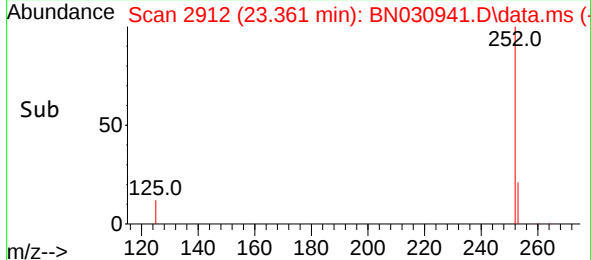

#40
Dibenzo(a,h)anthracene
Concen: 5.430 ng
RT: 25.711 min Scan# 3716
Delta R.T. 0.006 min
Lab File: BN030941.D
Acq: 15 Apr 2024 16:23

Tgt Ion:278 Resp: 284479
Ion Ratio Lower Upper
278 100
139 18.9 16.3 24.5
279 23.5 20.6 31.0

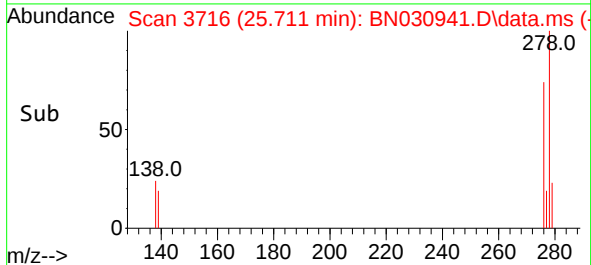

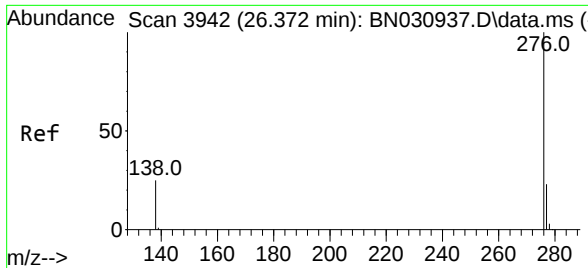

#41
 Benzo(g,h,i)perylene
 Concen: 5.299 ng
 RT: 26.375 min Scan# 3943
 Delta R.T. 0.003 min
 Lab File: BN030941.D
 Acq: 15 Apr 2024 16:23

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:	276	Resp:	305707
Ion	Ratio	Lower	Upper
276	100		
277	23.4	19.4	29.2
138	25.1	21.0	31.4

