
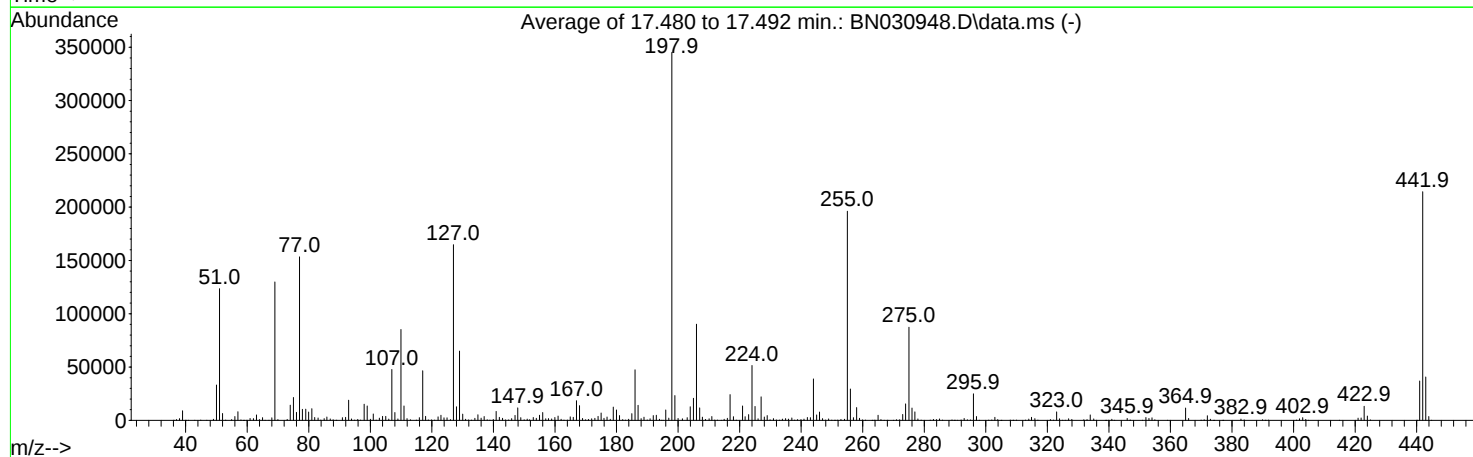


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030948.D
Acq On : 15 Apr 2024 22:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 15 17:03:47 2024

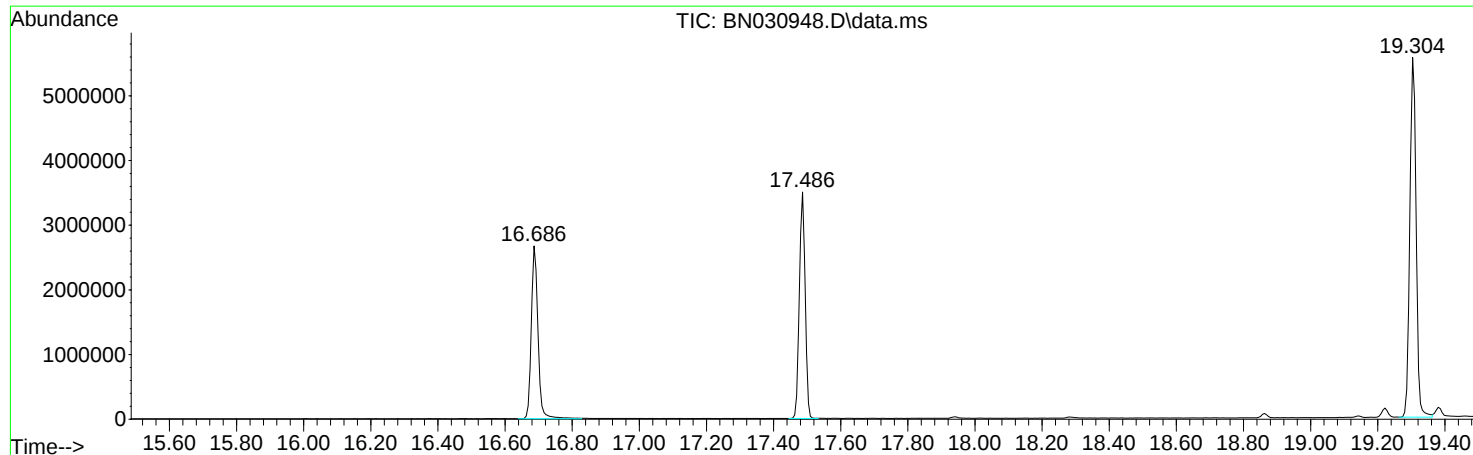




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	123528	PASS
68	69	0.00	2	1.8	2339	PASS
69	198	0.00	100	37.6	129859	PASS
70	69	0.00	2	0.6	735	PASS
127	198	10	80	47.7	164752	PASS
197	198	0.00	2	0.6	2168	PASS
198	198	100	100	100.0	345045	PASS
199	198	5	9	6.7	23205	PASS
275	198	10	60	25.3	87288	PASS
365	198	1	100	3.3	11526	PASS
441	198	0.01	100	10.7	36872	PASS
442	442	50	100	100.0	214400	PASS
443	442	15	24	18.9	40611	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030948.D
Acq On : 15 Apr 2024 22:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 16 00:46:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 16 00:44:54 2024
Response via : Initial Calibration

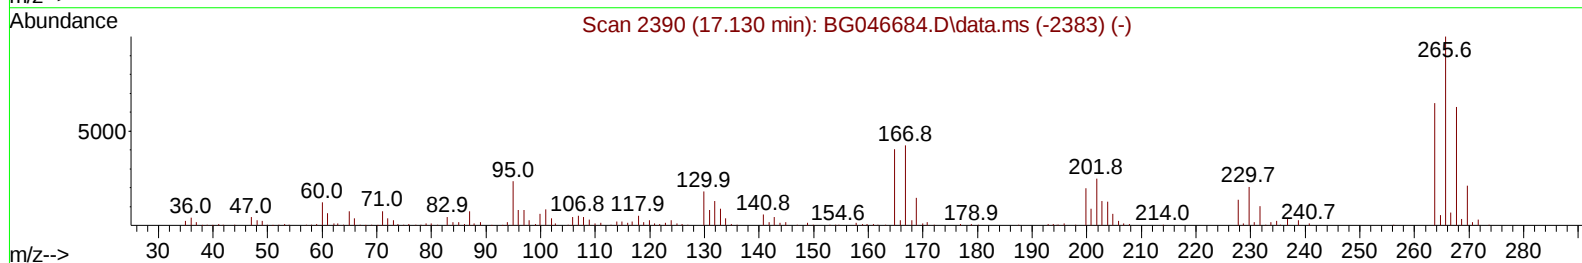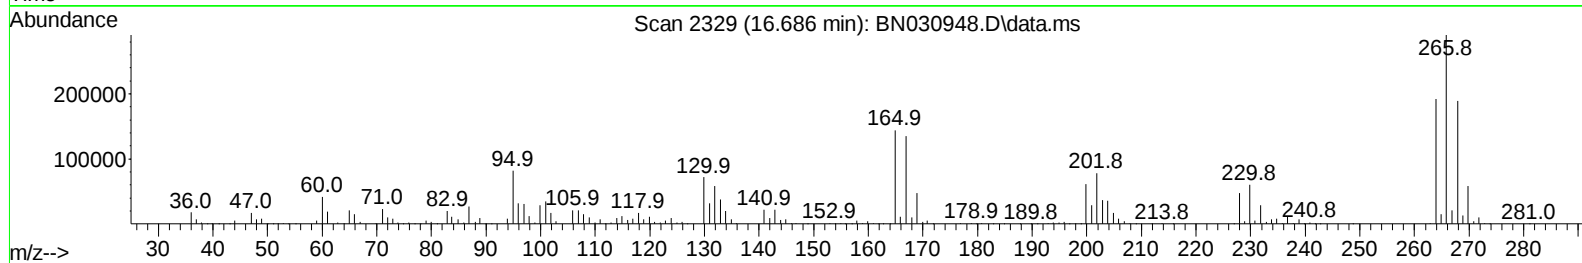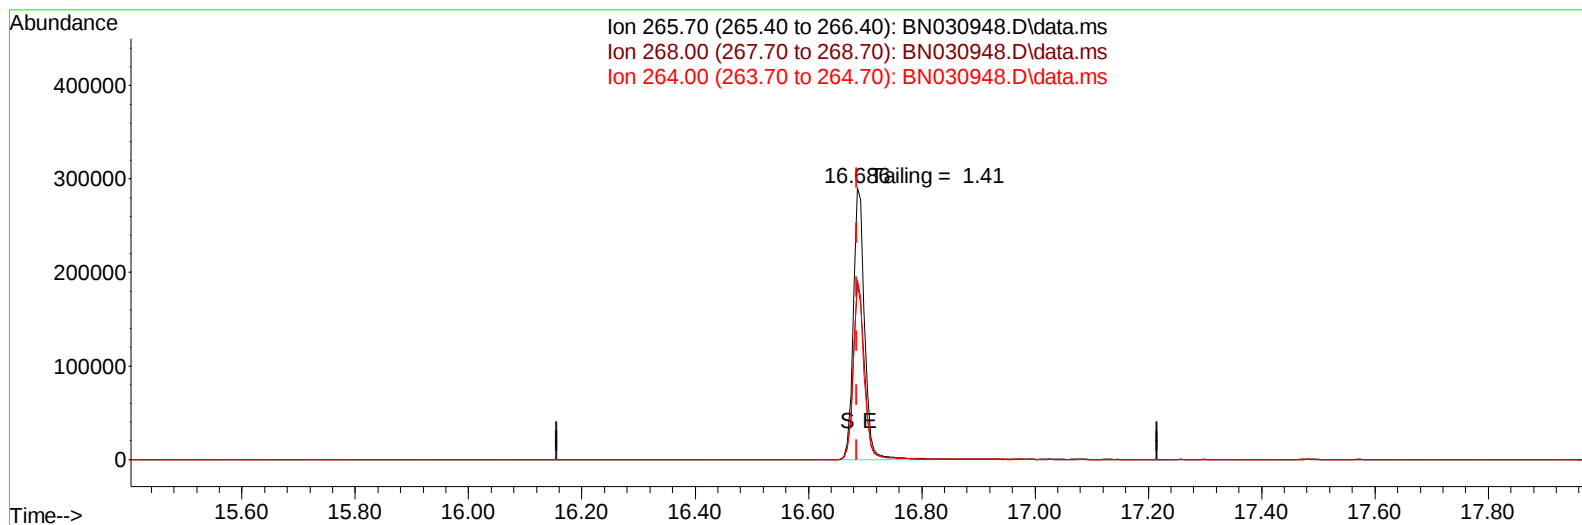

TIC: BN030948.D\data.ms

(70) Pentachlorophenol (C)

16.686min (+ 0.000) 22067.06 ng




response 406619

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.20
264.00	61.60	66.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030948.D
Acq On : 15 Apr 2024 22:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 16 00:46:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 16 00:44:54 2024
Response via : Initial Calibration

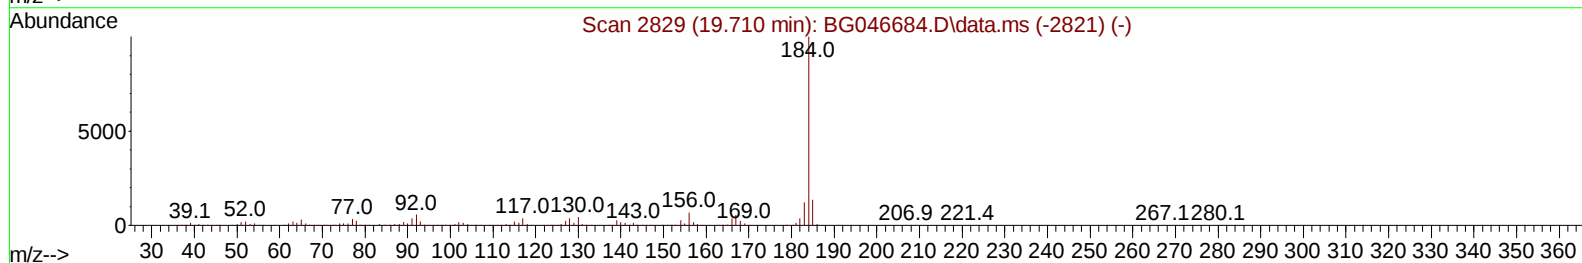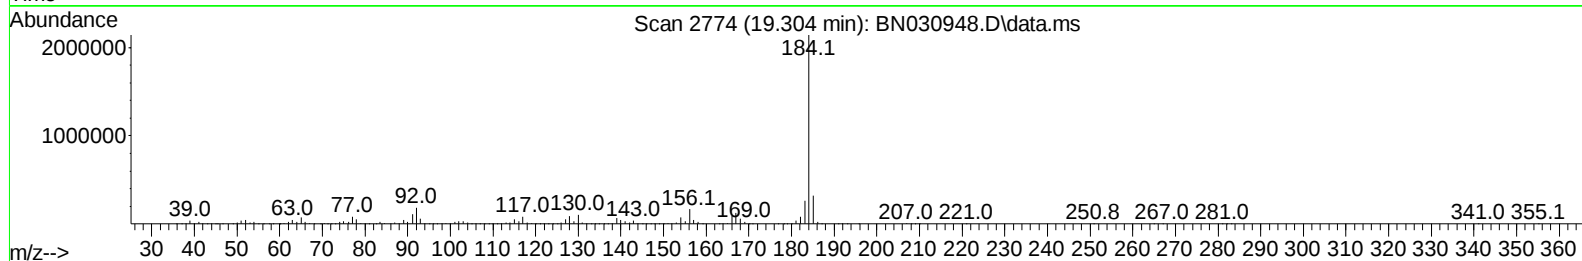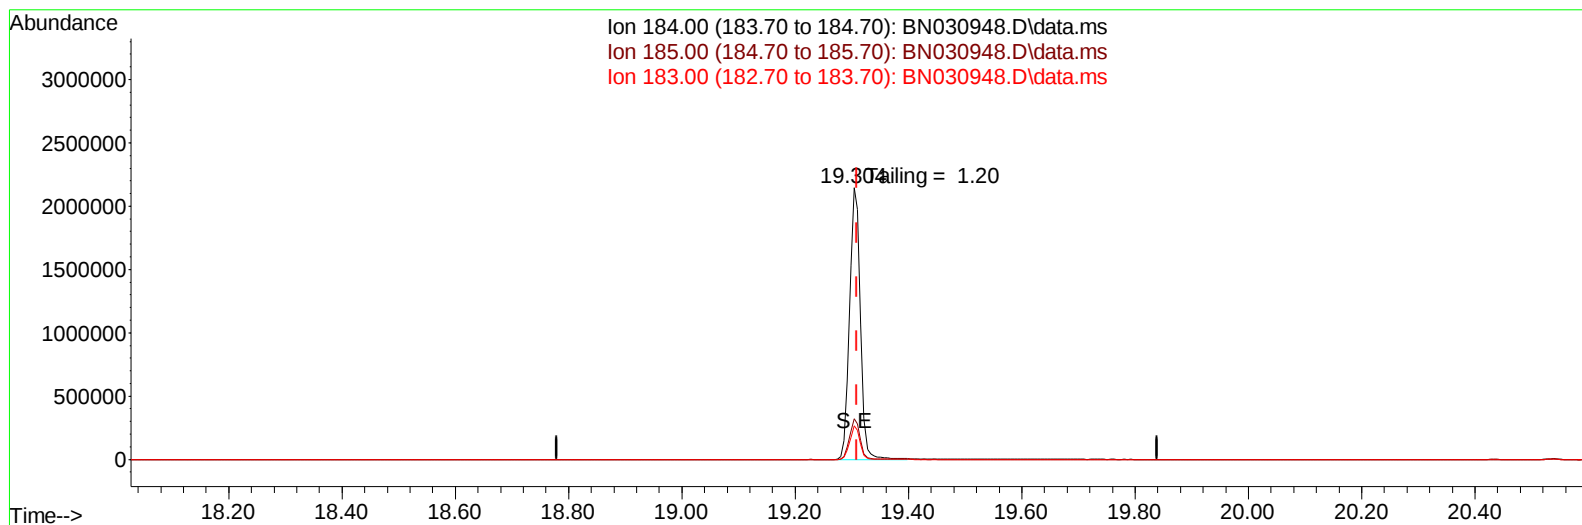

TIC: BN030948.D\data.ms

(77) Benzidine

19.304min (-0.006) 0.00 ng

response 2883503

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.96
183.00	13.20	12.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/15/2024	BNA_N	<u>BN030948.D</u>
Compound Name	Response	Retention Time
DDT	1292261	20.539
DDD	13467	20.145
DDE	0	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13467	1305728	1.03

Instrument :
BNA_N
ClientSampleId :
DFTPP