
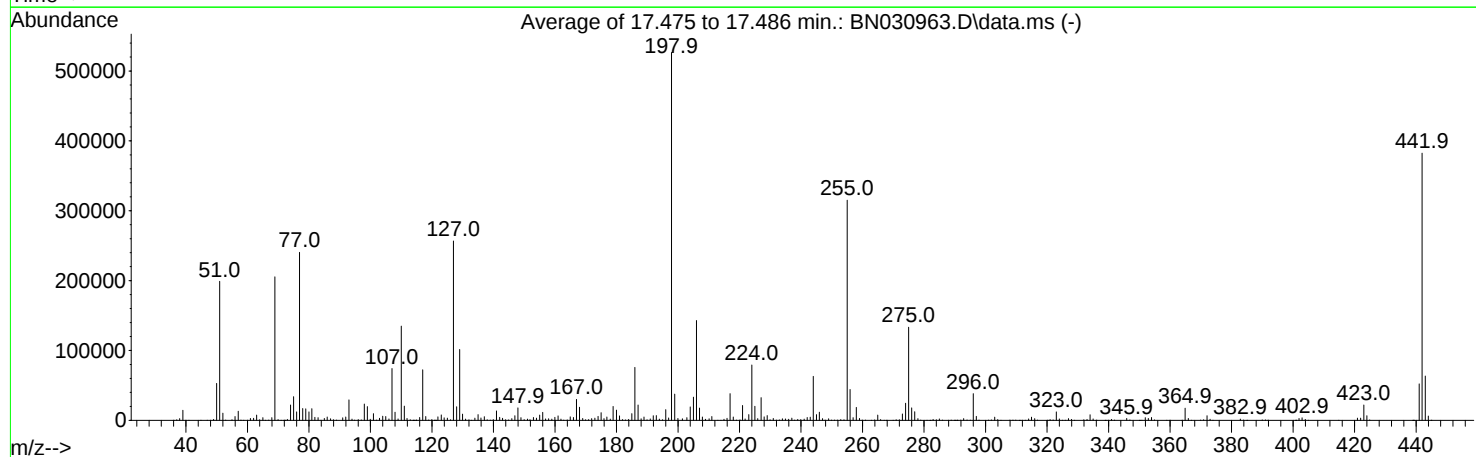


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030963.D
Acq On : 16 Apr 2024 09:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 15 17:03:47 2024

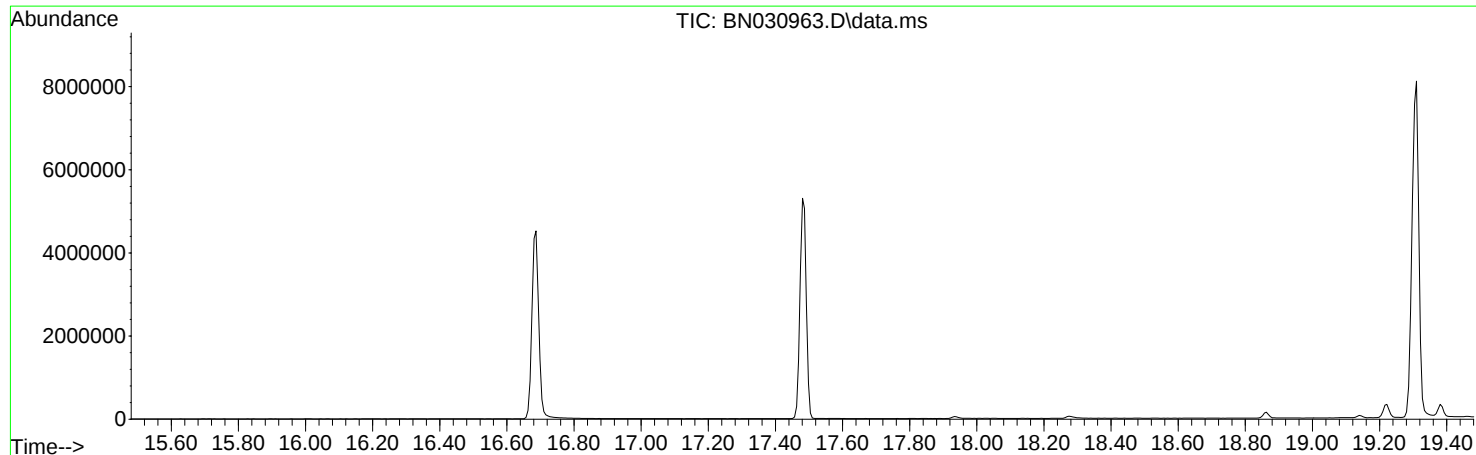




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	198999	PASS
68	69	0.00	2	1.9	3900	PASS
69	198	0.00	100	39.0	205376	PASS
70	69	0.00	2	0.5	1097	PASS
127	198	10	80	48.8	256768	PASS
197	198	0.00	2	0.6	3337	PASS
198	198	100	100	100.0	526528	PASS
199	198	5	9	7.1	37555	PASS
275	198	10	60	25.3	133245	PASS
365	198	1	100	3.3	17347	PASS
441	198	0.01	100	9.9	52301	PASS
442	442	50	100	100.0	382464	PASS
443	442	15	24	16.6	63541	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030963.D
Acq On : 16 Apr 2024 09:01
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTTP

Quant Time: Apr 17 01:56:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

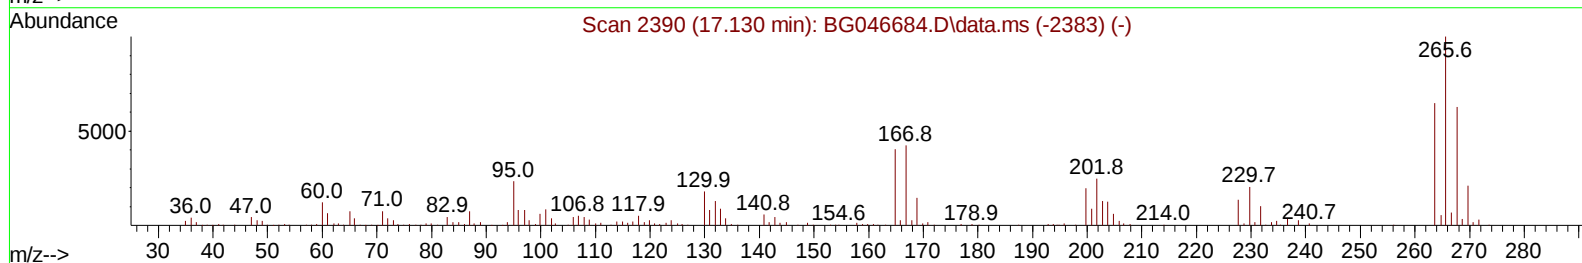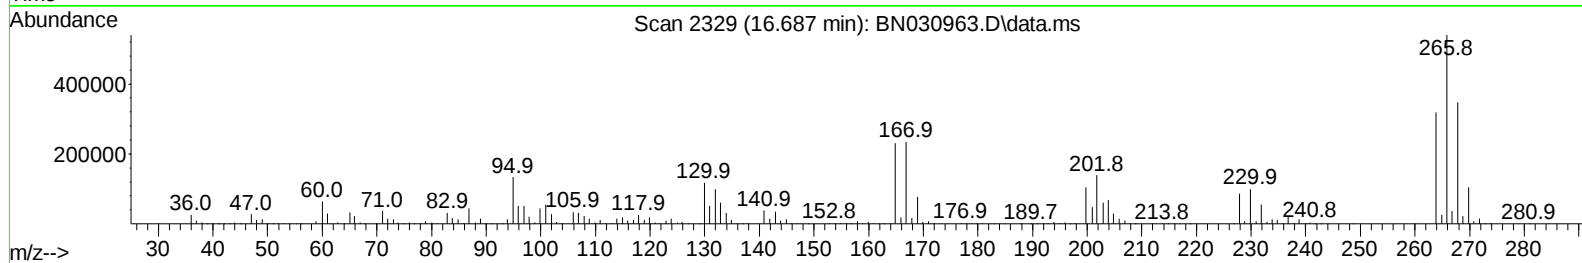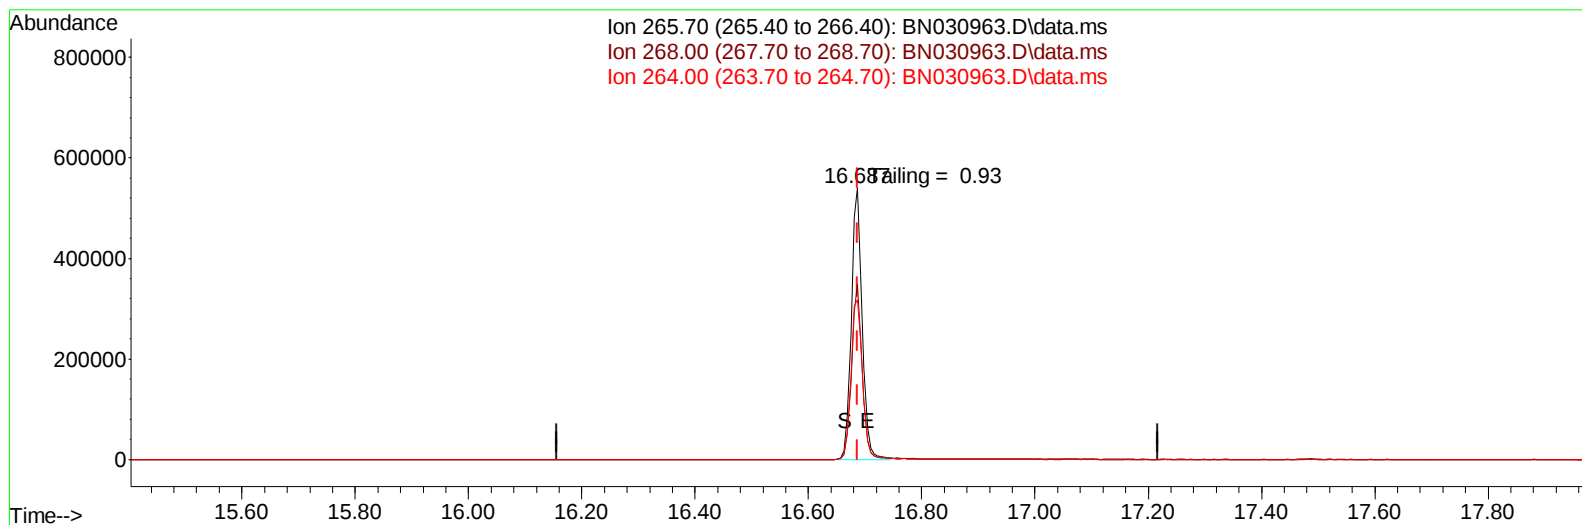

TIC: BN030963.D\data.ms

(70) Pentachlorophenol (C)

16.687min (0.000) 25980.92 ng




response 727078

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.38
264.00	61.60	58.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041524\
Data File : BN030963.D
Acq On : 16 Apr 2024 09:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 17 01:56:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 17 01:56:21 2024
Response via : Initial Calibration

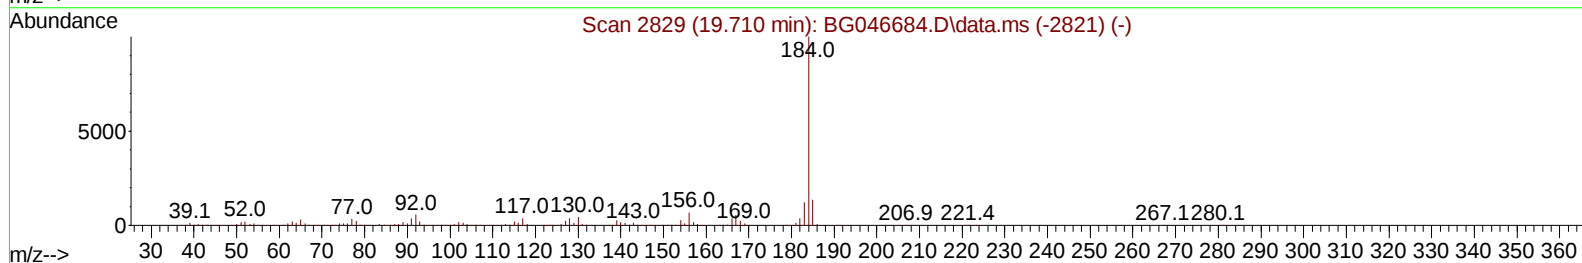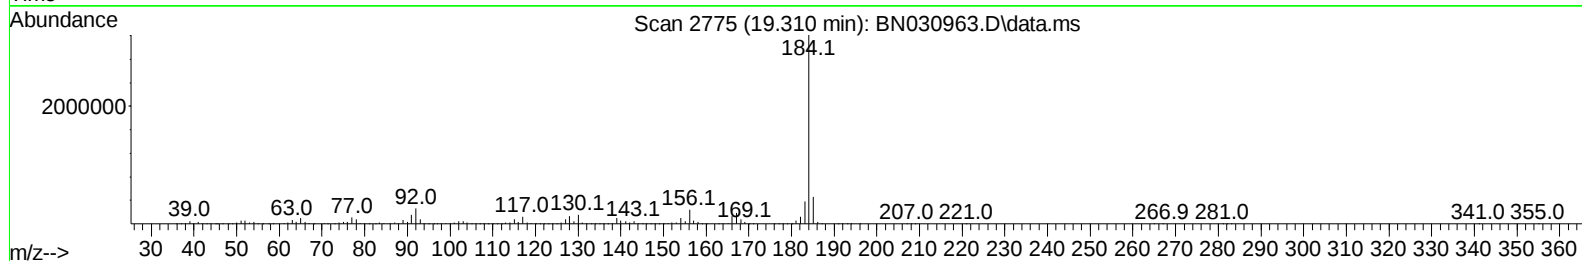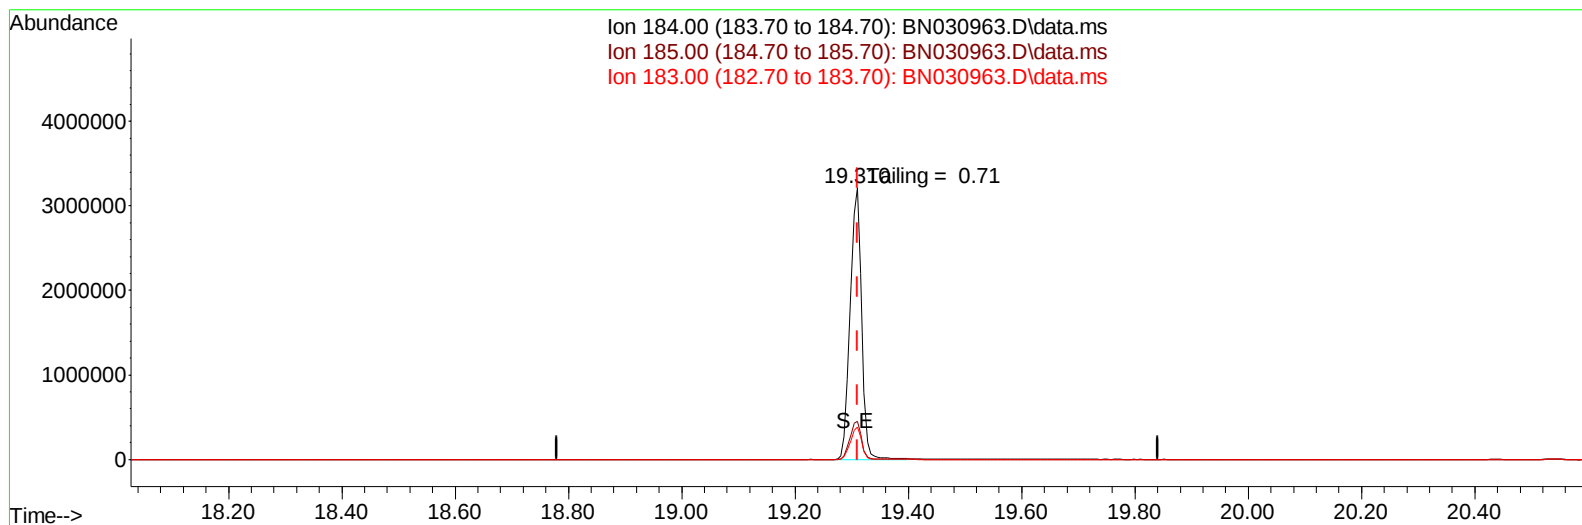

TIC: BN030963.D\data.ms

(77) Benzidine

19.310min (0.000) 0.00 ng

response 4588581

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/15/2024	BNA_N	<u>BN030963.D</u>
Compound Name	Response	Retention Time
DDT	2098980	20.539
DDD	32330	20.145
DDE	605	19.586
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32935	2131915	1.54

Instrument :
BNA_N
ClientSampleId :
DFTPP