

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030975.D
 Acq On : 17 Apr 2024 13:29
 Operator : MA/JU
 Sample : P2006-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R63

Quant Time: Apr 17 22:30:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 17 22:24:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	149547	20.000	ng/ul	0.00
20) Naphthalene-d8	10.422	136	690111	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.287	164	487526	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.034	188	1084423	20.000	ng/ul	0.00
79) Chrysene-d12	21.269	240	1159557	20.000	ng/ul	0.00
88) Perylene-d12	24.174	264	1446600	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.152	96	11814	3.704	ng/uL	0.00
4) Pyridine-d5	3.564	84	51100	5.343	ng/ul	0.00
7) Phenol-d5	6.816	99	55498	4.588	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	238670	31.942	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	204765	22.312	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	123882	12.218	ng/ul	0.00
21) Nitrobenzene-d5	8.799	128	155983	32.583	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	146225	33.389	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	253013	26.389	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	406092	25.728	ng/ul	0.00
46) Dimethylphthalate-d6	13.704	166	1252926	38.492	ng/ul	0.00
49) Acenaphthylene-d8	13.981	160	1292320	34.531	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	26397	4.240	ng/ul	0.00
60) Fluorene-d10	15.281	176	1073233	37.679	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	161905	33.825	ng/ul	0.00
73) Anthracene-d10	17.134	188	1915605	40.999	ng/ul	0.00
81) Pyrene-d10	19.433	212	2390912	38.351	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	2722500	40.844	ng/ul	0.00
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	13.704	165	8260	1.325	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030975.D
Acq On : 17 Apr 2024 13:29
Operator : MA/JU
Sample : P2006-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R63


Quant Time: Apr 17 22:30:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration

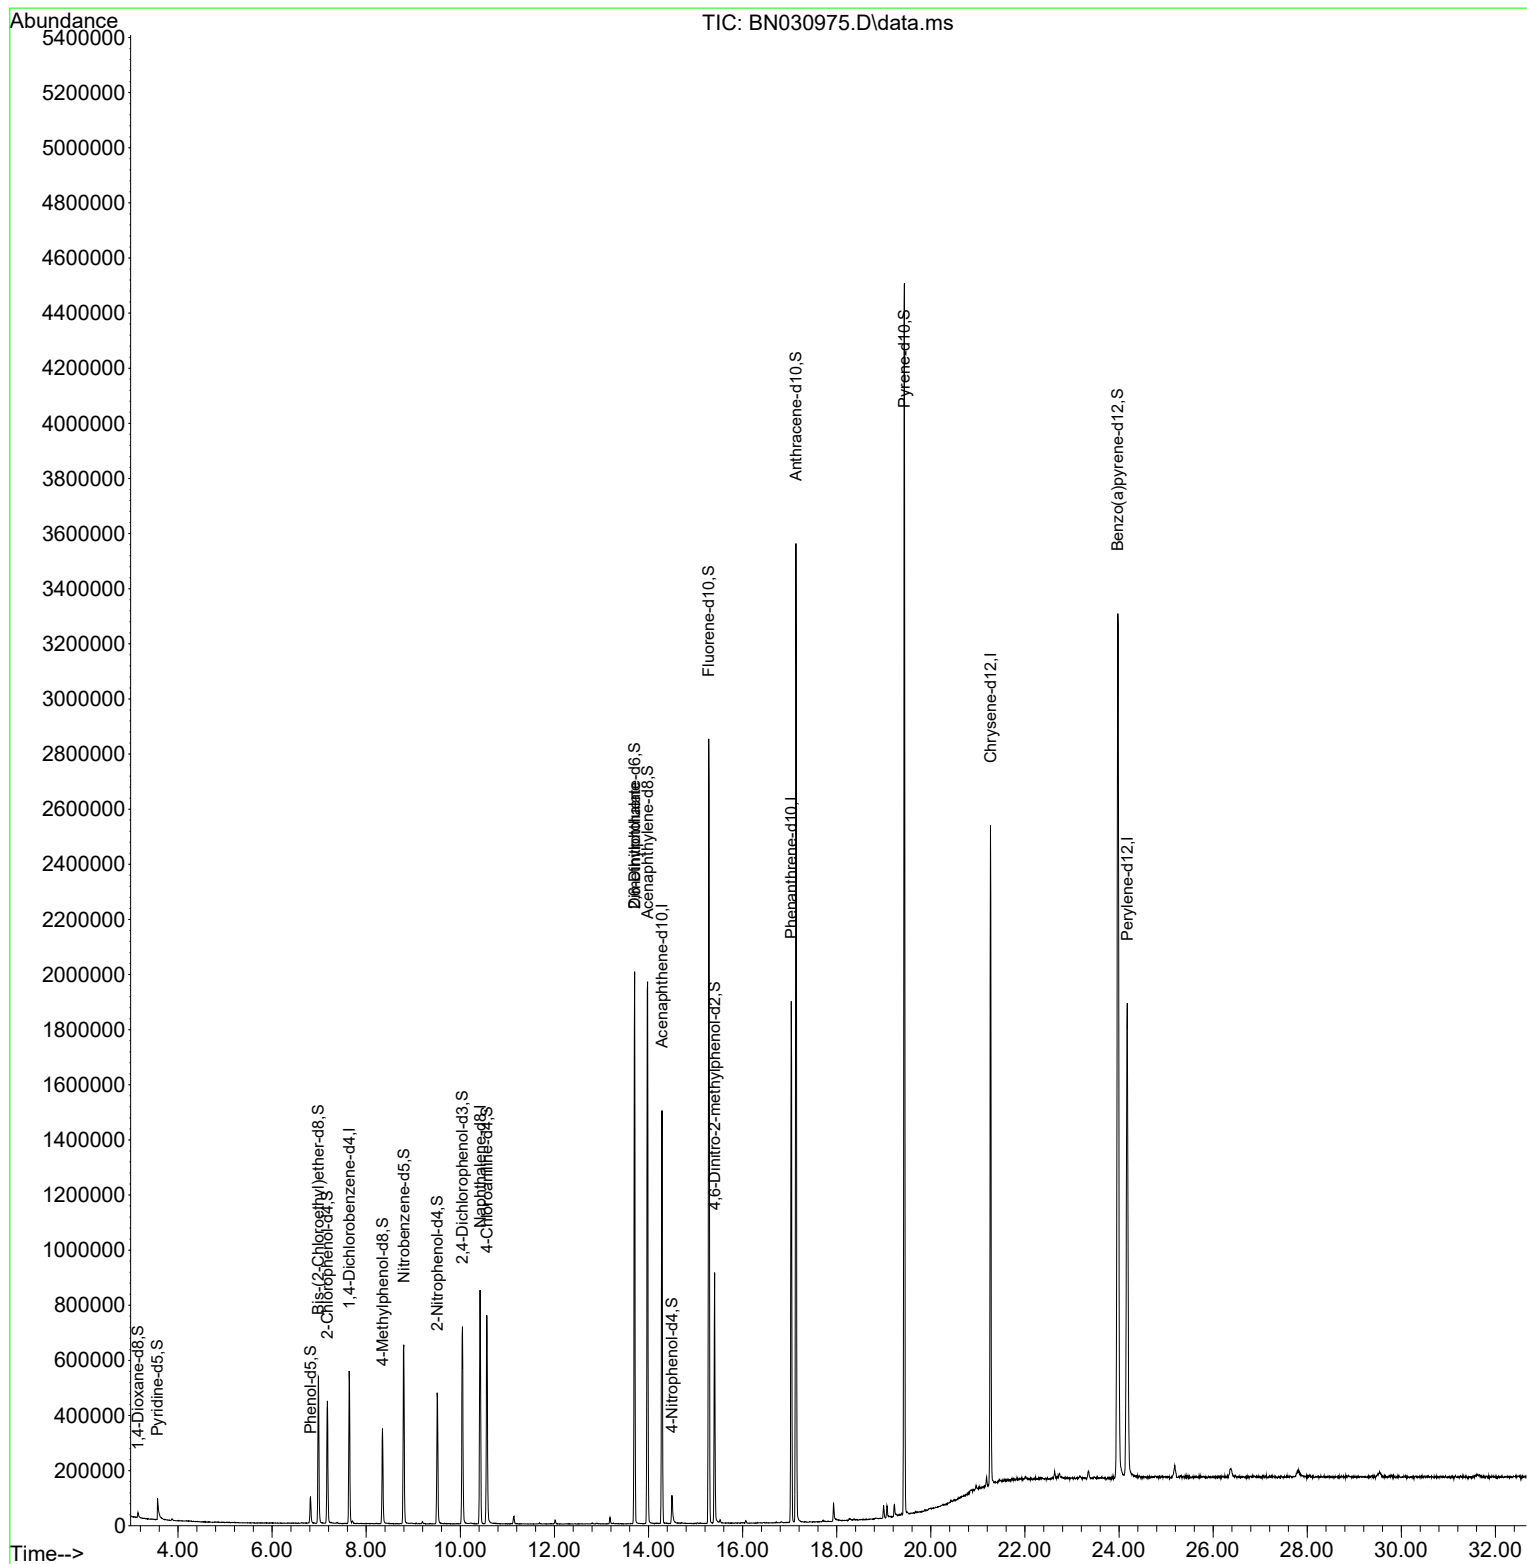

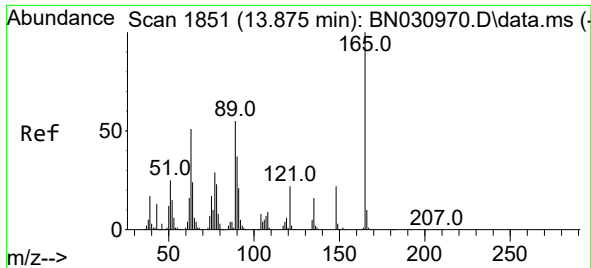

#48
 2,6-Dinitrotoluene
 Concen: 1.325 ng/ul
 RT: 13.704 min Scan# 11
 Delta R.T. -0.171 min
 Lab File: BN030975.D
 Acq: 17 Apr 2024 13:29

Instrument :
 BNA_N
 ClientSampleId :
 MC0R63

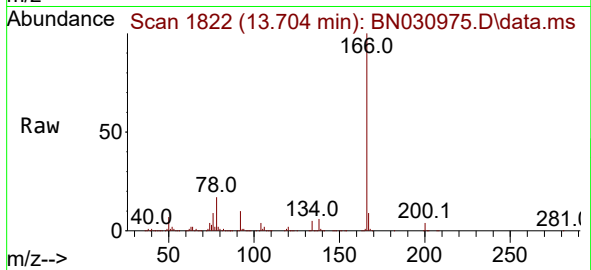

Tgt Ion:165 Resp: 8260
 Ion Ratio Lower Upper
 165 100
 89 0.0 43.5 65.3#
 121 36.9 15.7 23.5#

