

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030976.D
 Acq On : 17 Apr 2024 14:09
 Operator : MA/JU
 Sample : P2006-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R74

Quant Time: Apr 17 22:30:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 17 22:24:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	142361	20.000	ng/ul	0.00
20) Naphthalene-d8	10.422	136	658573	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.287	164	468804	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.034	188	1035388	20.000	ng/ul	0.00
79) Chrysene-d12	21.269	240	1162702	20.000	ng/ul	0.00
88) Perylene-d12	24.174	264	1415748	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.152	96	11546	3.803	ng/uL	0.00
4) Pyridine-d5	3.564	84	54995	6.041	ng/ul	0.00
7) Phenol-d5	6.816	99	54142	4.701	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	207701	29.200	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	186864	21.389	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	113688	11.779	ng/ul	0.00
21) Nitrobenzene-d5	8.799	128	133496	29.221	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	124191	29.716	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	225351	24.630	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	368786	24.483	ng/ul	0.00
46) Dimethylphthalate-d6	13.704	166	1018714	32.547	ng/ul	0.00
49) Acenaphthylene-d8	13.981	160	1084156	30.126	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	24385	4.073	ng/ul	0.00
60) Fluorene-d10	15.281	176	889569	32.478	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	122520	26.809	ng/ul	0.00
73) Anthracene-d10	17.134	188	1561465	35.002	ng/ul	0.00
81) Pyrene-d10	19.439	212	1990570	31.843	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	2381154	36.502	ng/ul	0.00
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	13.710	165	5997	1.000	ng/ul#	40
89) Di-n-octyl phthalate	22.351	149	177953	1.985	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030976.D
Acq On : 17 Apr 2024 14:09
Operator : MA/JU
Sample : P2006-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R74

Quant Time: Apr 17 22:30:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration




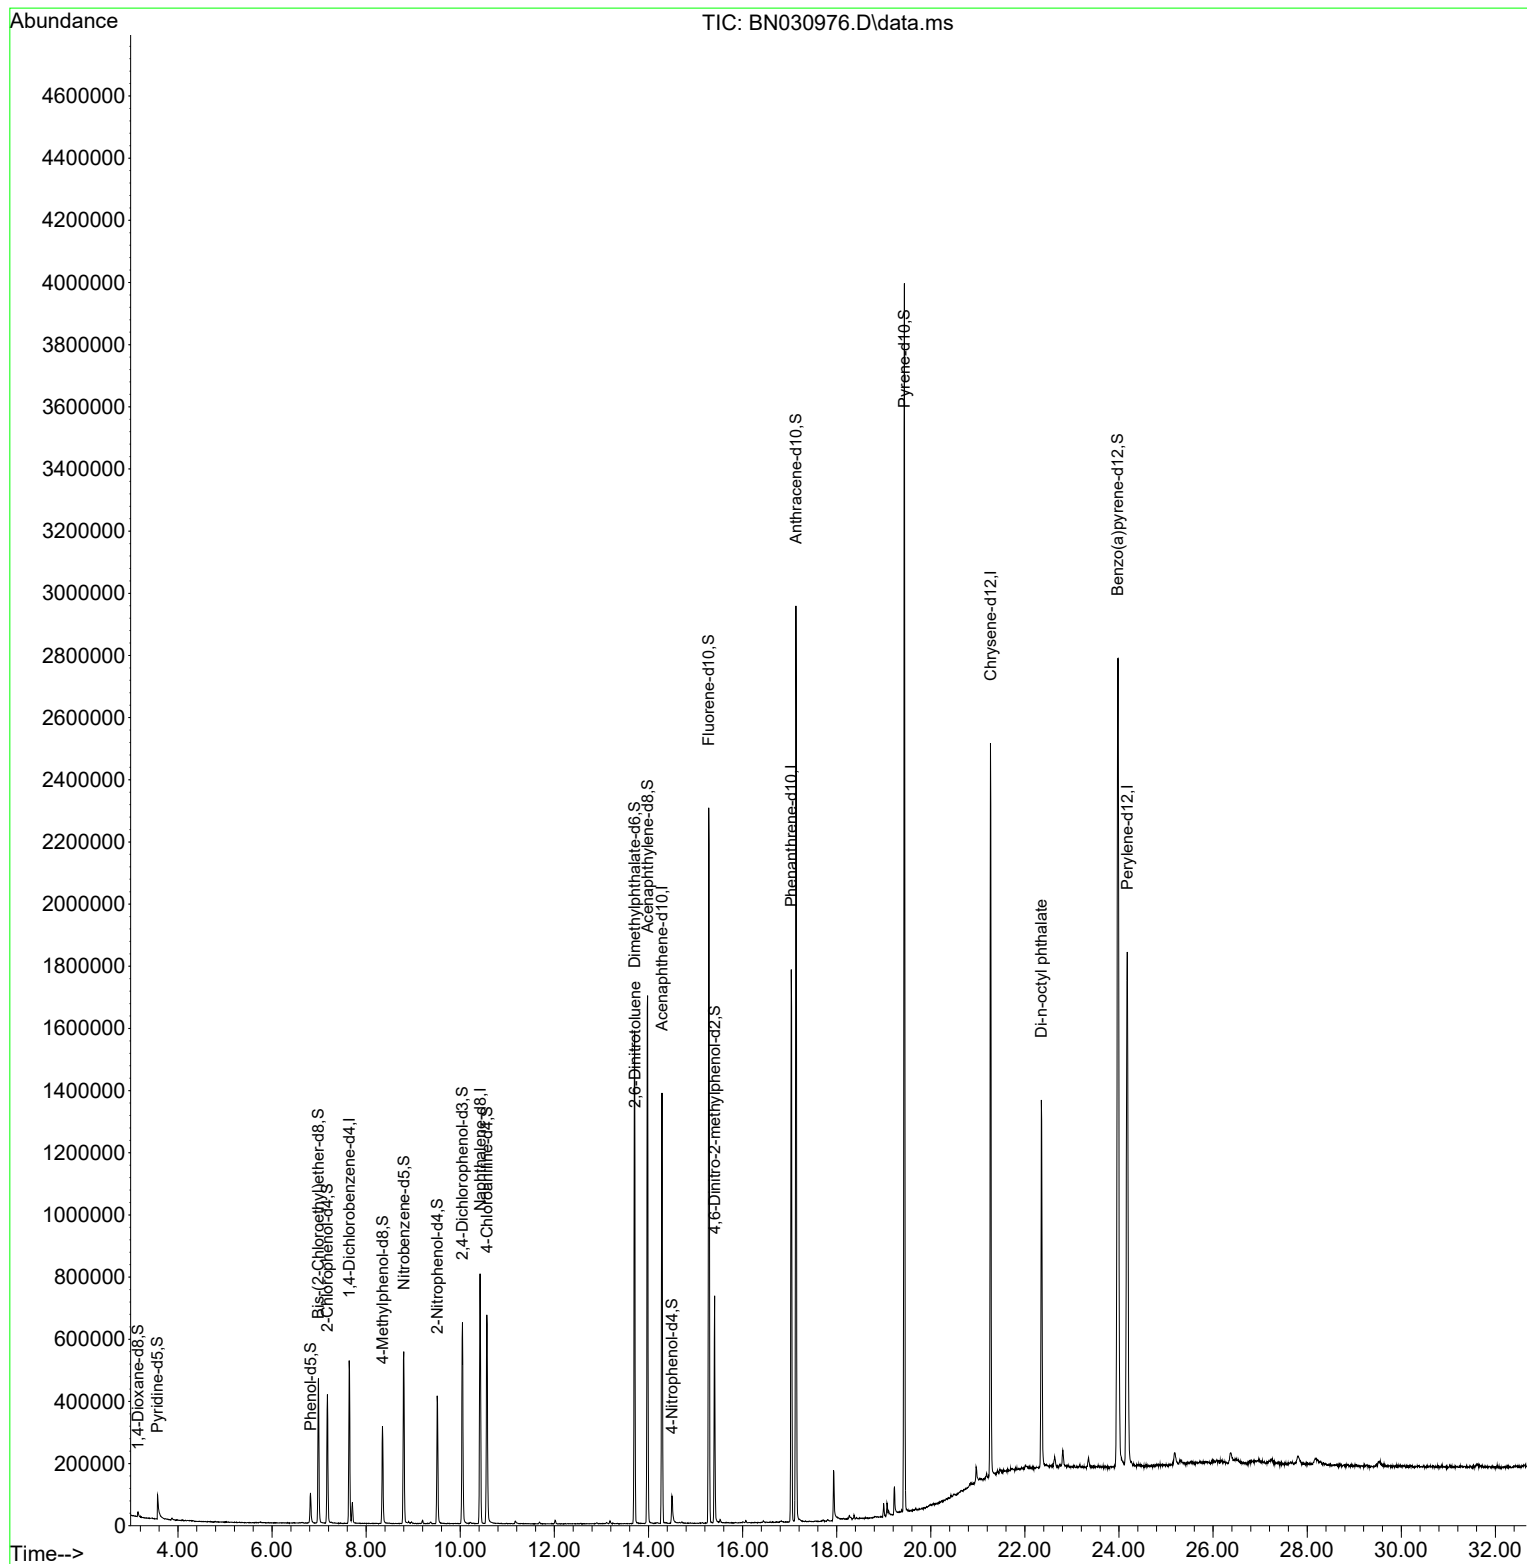


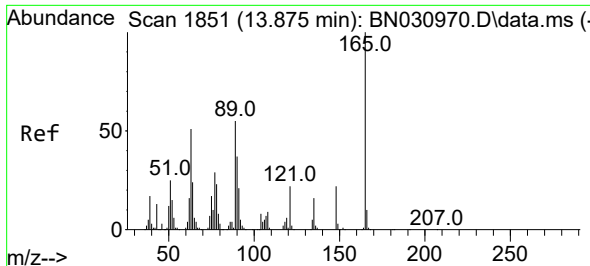

#48
2,6-Dinitrotoluene
Concen: 1.000 ng/ul
RT: 13.710 min Scan# 1851
Delta R.T. -0.165 min
Lab File: BN030976.D
Acq: 17 Apr 2024 14:09

Instrument :
BNA_N
ClientSampleId :
MC0R74

Tgt Ion:165 Resp: 5997
Ion Ratio Lower Upper
165 100
89 0.0 43.5 65.3#
121 27.0 15.7 23.5#

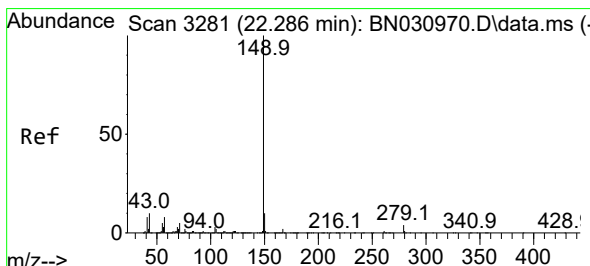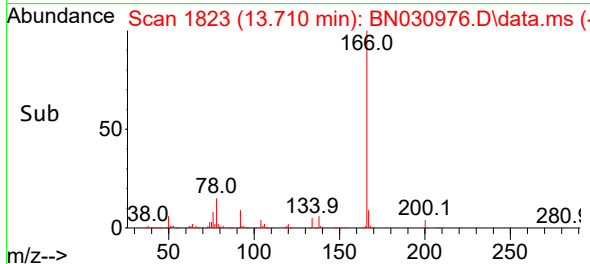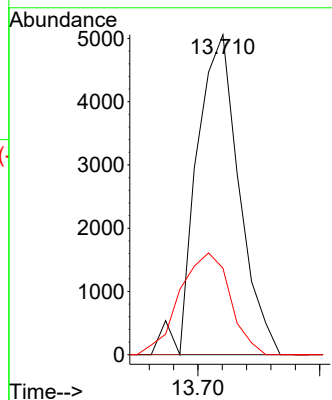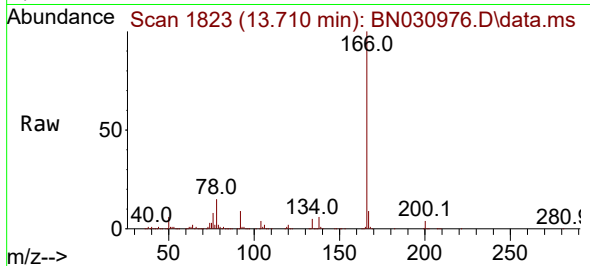

#89
Di-n-octyl phthalate
Concen: 1.985 ng/ul
RT: 22.351 min Scan# 3292
Delta R.T. 0.065 min
Lab File: BN030976.D
Acq: 17 Apr 2024 14:09

Tgt Ion:149 Resp: 177953

