

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030985.D
 Acq On : 17 Apr 2024 21:25
 Operator : MA/JU
 Sample : PB160254BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK254

Quant Time: Apr 17 22:31:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 17 22:24:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	105945	20.000	ng/ul	0.00
20) Naphthalene-d8	10.422	136	501479	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.287	164	355148	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.034	188	809994	20.000	ng/ul	0.00
79) Chrysene-d12	21.269	240	881332	20.000	ng/ul	0.00
88) Perylene-d12	24.169	264	1105667	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	14968	6.624	ng/uL	0.00
4) Pyridine-d5	3.558	84	193144	28.508	ng/ul	0.00
7) Phenol-d5	6.811	99	262515	30.630	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	172994	32.680	ng/ul	0.00
11) 2-Chlorophenol-d4	7.175	132	210131	32.320	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	218925	30.479	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	108143	31.087	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	103877	32.641	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	202073	29.004	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	354306	30.890	ng/ul	0.00
46) Dimethylphthalate-d6	13.704	166	872686	36.804	ng/ul	0.00
49) Acenaphthylene-d8	13.975	160	895506	32.847	ng/ul	0.00
54) 4-Nitrophenol-d4	14.493	143	125408	27.650	ng/ul	0.00
60) Fluorene-d10	15.281	176	705387	33.995	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	85306	23.860	ng/ul	0.00
73) Anthracene-d10	17.134	188	1185324	33.964	ng/ul	0.00
81) Pyrene-d10	19.433	212	1436487	30.316	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.969	264	1783461	35.007	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.710	165	5770	1.271	ng/ul#	Qvalue 44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030985.D
Acq On : 17 Apr 2024 21:25
Operator : MA/JU
Sample : PB160254BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK254


Quant Time: Apr 17 22:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration

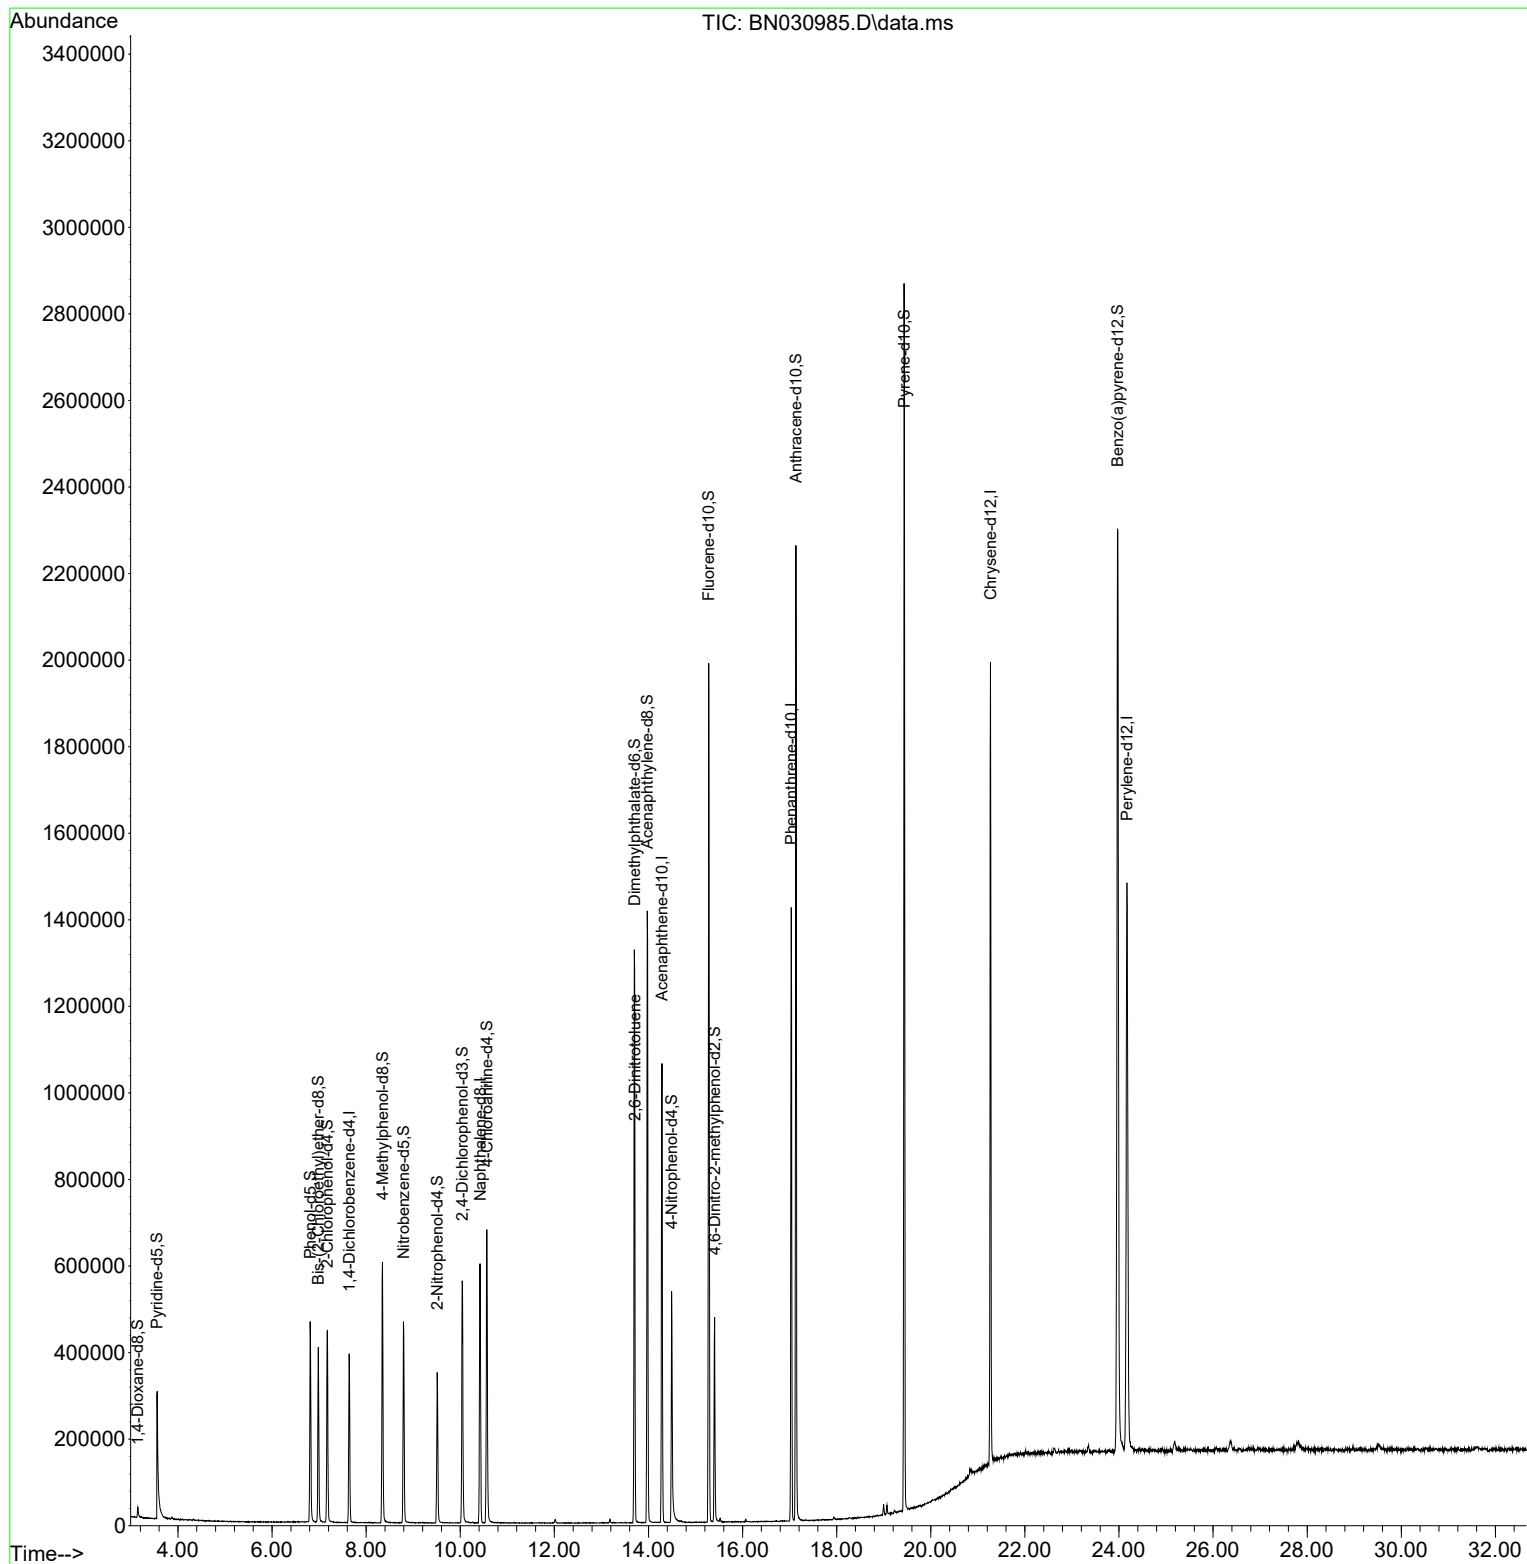

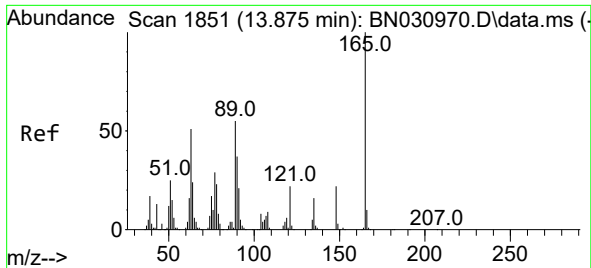

#48
 2,6-Dinitrotoluene
 Concen: 1.271 ng/ul
 RT: 13.710 min Scan# 1851
 Delta R.T. -0.165 min
 Lab File: BN030985.D
 Acq: 17 Apr 2024 21:25

Instrument :
 BNA_N
 ClientSampleId :
 SBLK254

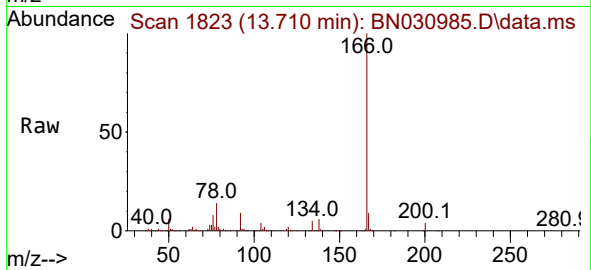

Tgt Ion:165 Resp: 5770
 Ion Ratio Lower Upper
 165 100
 89 0.0 43.5 65.3#
 121 21.1 15.7 23.5

