




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030992.D
Acq On : 18 Apr 2024 02:02
Operator : MA/JU
Sample : P2036-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 02:30:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/30/2024

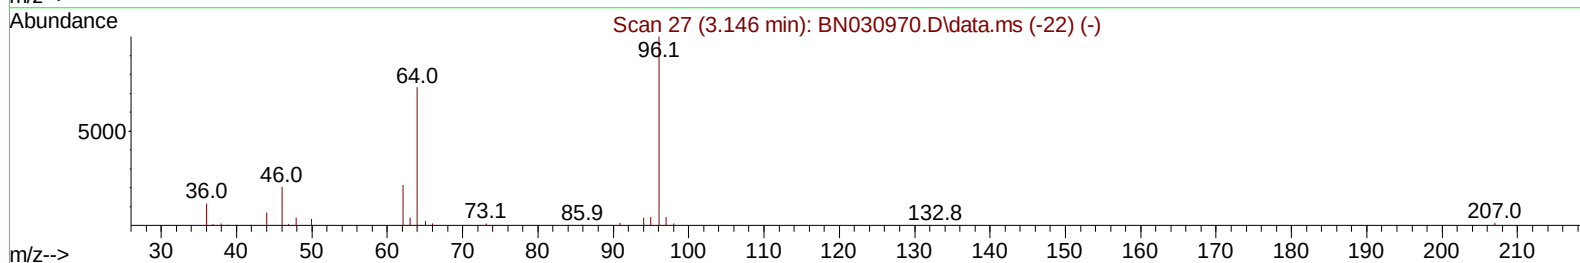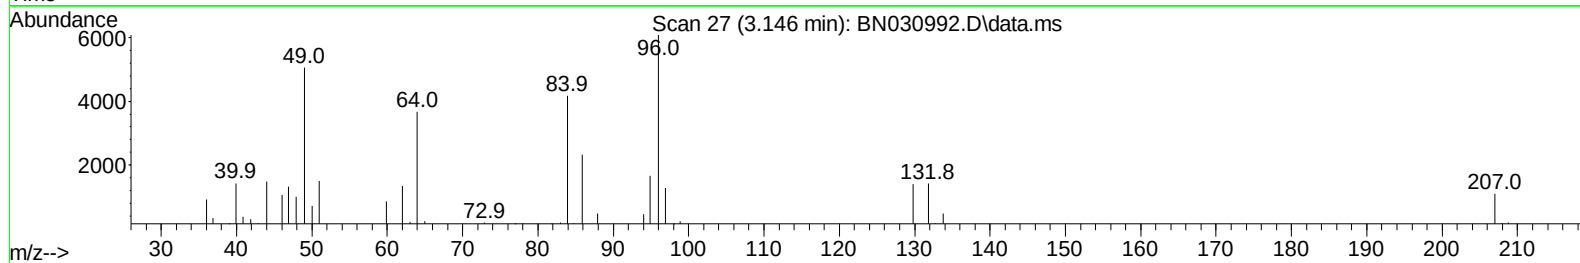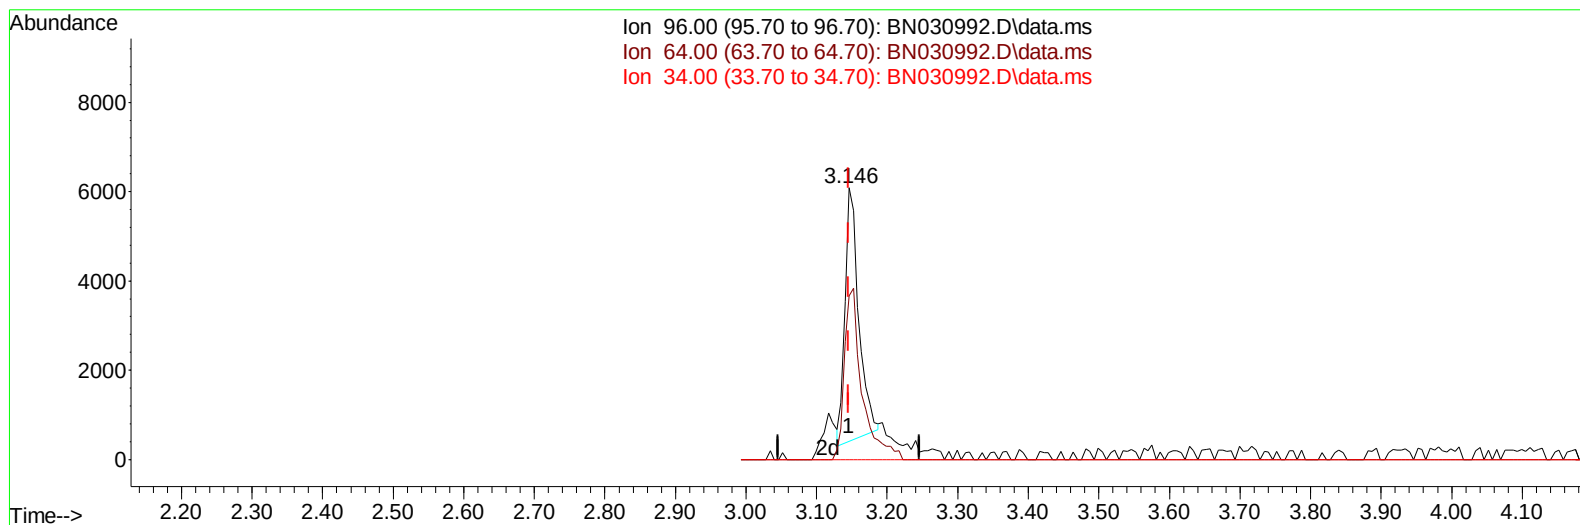

TIC: BN030992.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.146min (+ 0.000) 3.01 ng/uL

response 7748

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	65.50	60.22
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030992.D
 Acq On : 18 Apr 2024 02:02
 Operator : MA/JU
 Sample : P2036-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSY8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 02:30:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 17 22:24:16 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
 Supervised By :mohammad ahmed 04/30/2024

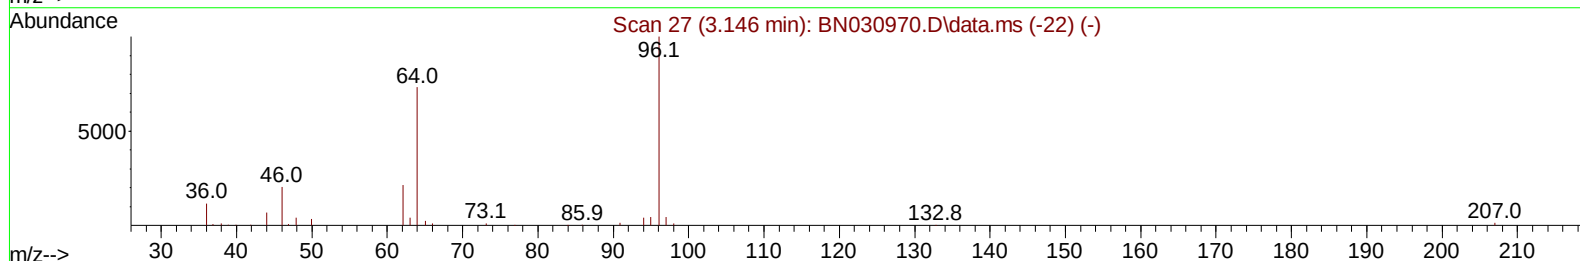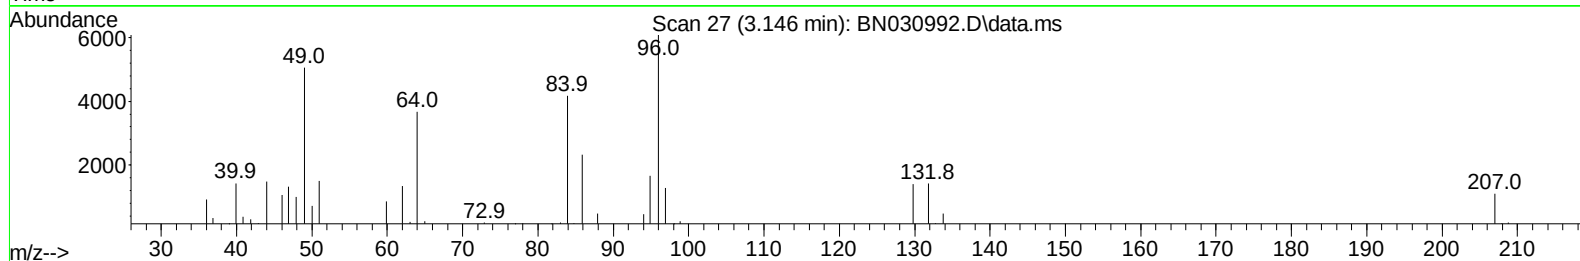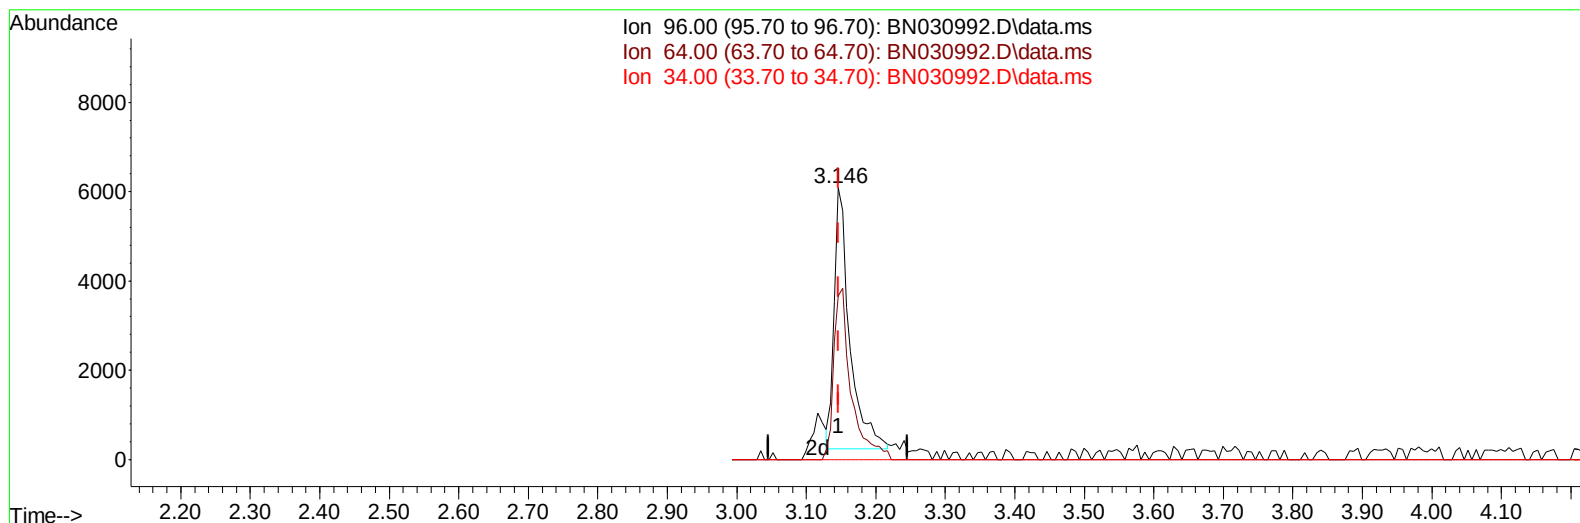

TIC: BN030992.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.146min (+ 0.000) 3.52 ng/uL m

response 9076

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	65.50	60.22
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030992.D
 Acq On : 18 Apr 2024 02:02
 Operator : MA/JU
 Sample : P2036-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSY8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/19/2024
 Supervised By :mohammad ahmed 04/30/2024

Quant Time: Apr 18 02:31:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 17 22:24:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	120725	20.000	ng/ul	0.00
20) Naphthalene-d8	10.422	136	562332	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.281	164	399207	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.034	188	909611	20.000	ng/ul	0.00
79) Chrysene-d12	21.269	240	996737	20.000	ng/ul	0.00
88) Perylene-d12	24.169	264	1226268	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	9076m	3.525	ng/uL	0.00
4) Pyridine-d5	3.564	84	57068	7.392	ng/ul	0.00
7) Phenol-d5	6.816	99	41890	4.289	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	167881	27.832	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	148439	20.036	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	90474	11.054	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	106099	27.199	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	95462	26.751	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.046	165	179347	22.957	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	298230	23.188	ng/ul	0.00
46) Dimethylphthalate-d6	13.704	166	830575	31.162	ng/ul	0.00
49) Acenaphthylene-d8	13.975	160	868804	28.351	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	16225	3.182	ng/ul	0.00
60) Fluorene-d10	15.281	176	746248	31.995	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	91497	22.789	ng/ul	0.00
73) Anthracene-d10	17.134	188	1315877	33.575	ng/ul	0.00
81) Pyrene-d10	19.433	212	1595999	29.782	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	1944627	34.416	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030992.D
Acq On : 18 Apr 2024 02:02
Operator : MA/JU
Sample : P2036-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 02:31:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/30/2024

