




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031007.D
Acq On : 18 Apr 2024 12:33
Operator : MA/JU
Sample : P2060-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CY8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 14:09:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/30/2024

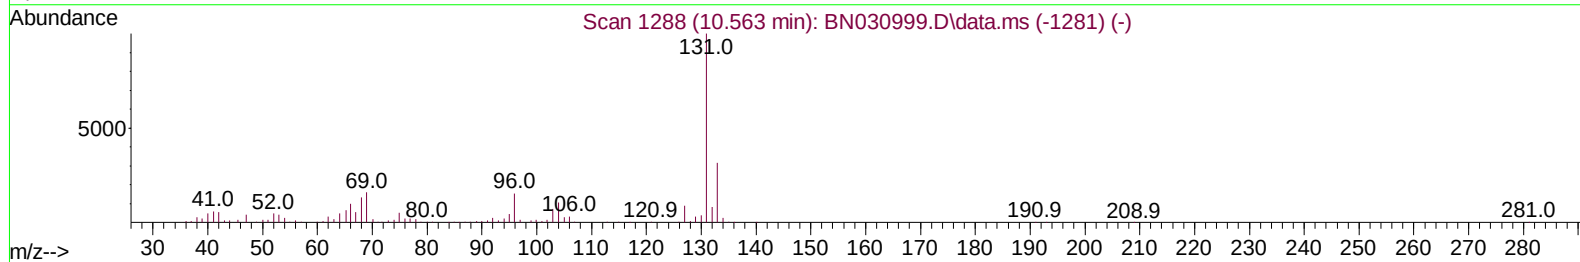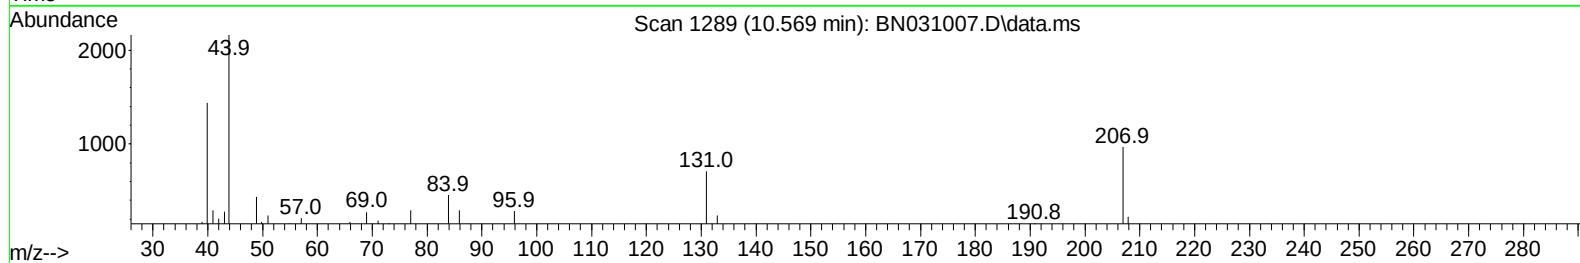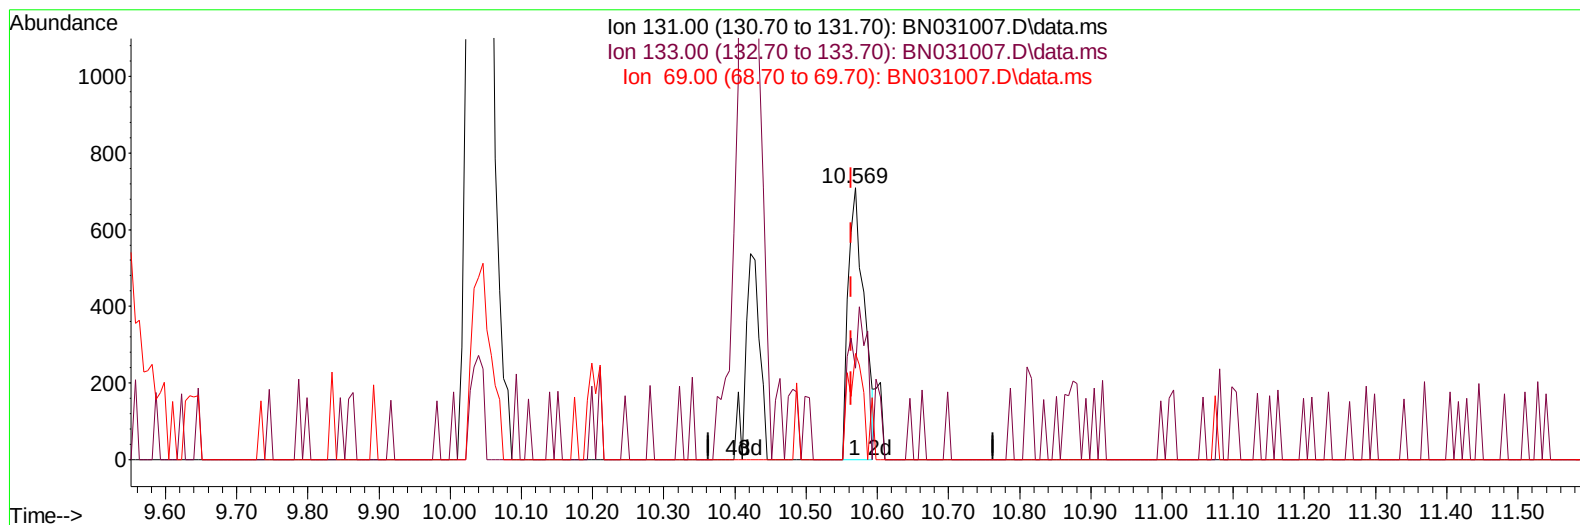

TIC: BN031007.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.569min (+ 0.006) 0.09 ng/ul

response 1112

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.70	33.71
69.00	16.20	38.93#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031007.D
Acq On : 18 Apr 2024 12:33
Operator : MA/JU
Sample : P2060-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CY8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 14:09:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/30/2024

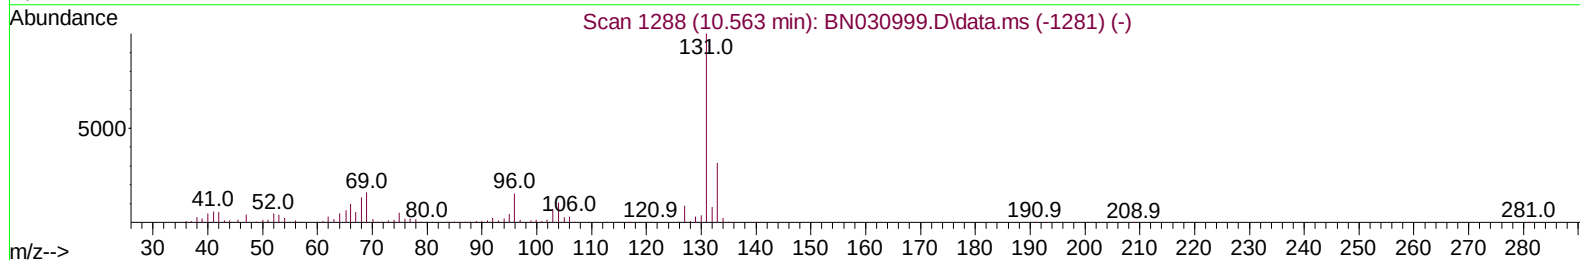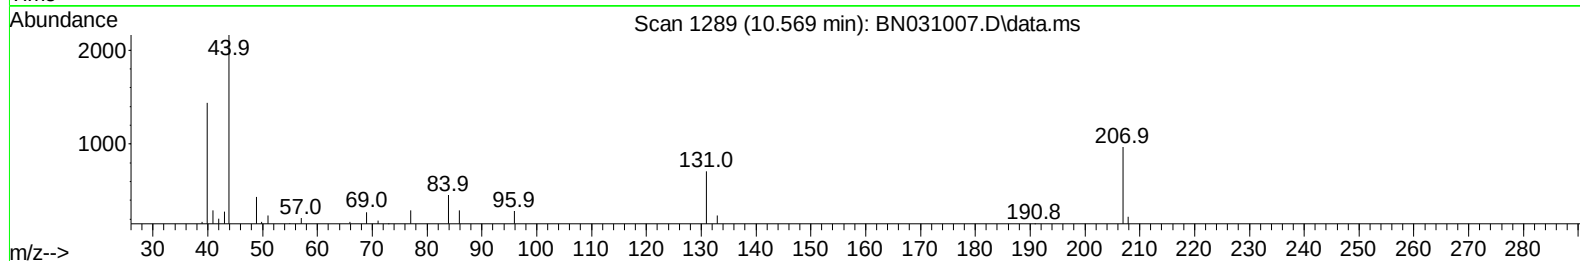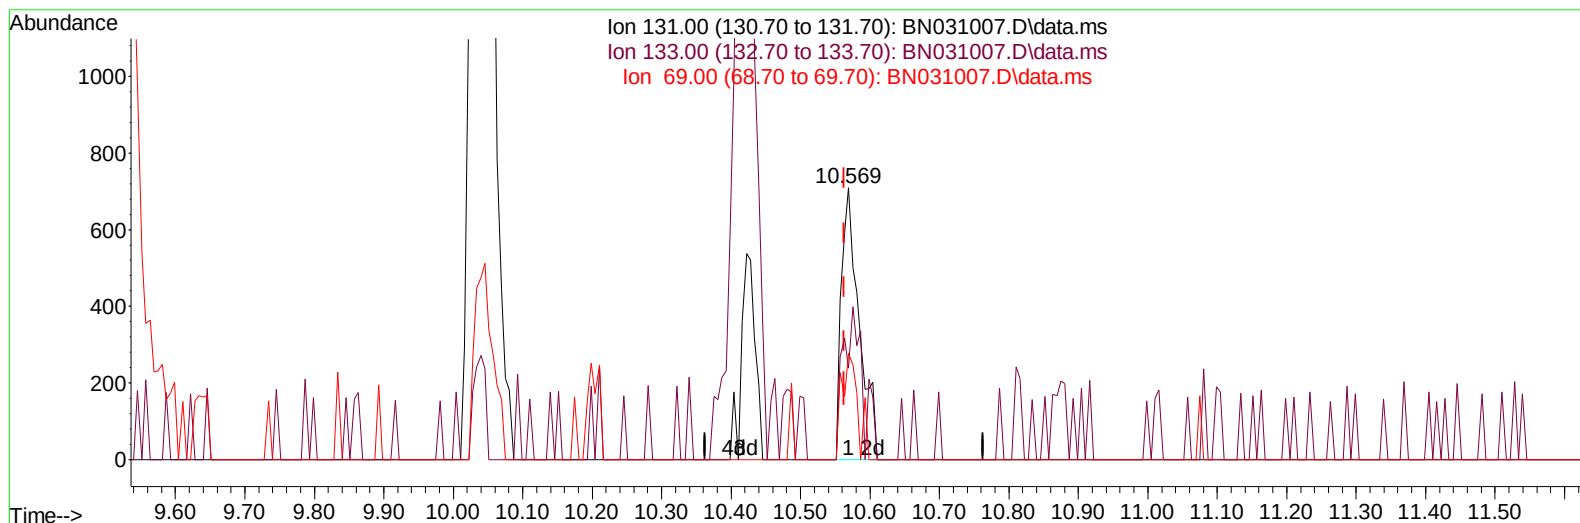

TIC: BN031007.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.569min (+ 0.006) 0.10 ng/ul m

response 1248

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.70	33.71
69.00	16.20	38.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031007.D
 Acq On : 18 Apr 2024 12:33
 Operator : MA/JU
 Sample : P2060-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CY8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/19/2024
 Supervised By :mohammad ahmed 04/30/2024

Quant Time: Apr 18 14:11:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 17 22:24:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	114099	20.000	ng/ul	0.00
20) Naphthalene-d8	10.416	136	524372	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.287	164	369456	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.033	188	832834	20.000	ng/ul	0.00
79) Chrysene-d12	21.269	240	920132	20.000	ng/ul	0.00
88) Perylene-d12	24.168	264	1205371	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	11419	4.692	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.810	99	136691	14.809	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	226011	39.645	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	268205	38.304	ng/ul	0.00
15) 4-Methylphenol-d8	8.346	113	223522	28.895	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	147033	40.421	ng/ul	0.00
24) 2-Nitrophenol-d4	9.510	143	143396	43.092	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	283321	38.891	ng/ul	0.00
31) 4-Chloroaniline-d4	10.569	131	1248m	0.104	ng/ul	0.00
46) Dimethylphthalate-d6	13.698	166	1077796	43.694	ng/ul	0.00
49) Acenaphthylene-d8	13.975	160	1122565	39.581	ng/ul	0.00
54) 4-Nitrophenol-d4	14.492	143	60546	12.832	ng/ul	0.00
60) Fluorene-d10	15.281	176	925323	42.868	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	123533	33.605	ng/ul	0.00
73) Anthracene-d10	17.133	188	1502182	41.862	ng/ul	0.00
81) Pyrene-d10	19.433	212	1946775	39.353	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	2345464	42.230	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031007.D
Acq On : 18 Apr 2024 12:33
Operator : MA/JU
Sample : P2060-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CY8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 14:11:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/19/2024
Supervised By :mohammad ahmed 04/30/2024

