

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030989.D
 Acq On : 18 Apr 2024 00:04
 Operator : MA/JU
 Sample : P2100-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AP2

Quant Time: Apr 18 00:49:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 17 22:24:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	120906	20.000	ng/u1	0.00
20) Naphthalene-d8	10.416	136	567887	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.286	164	404029	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.033	188	936912	20.000	ng/u1	0.00
79) Chrysene-d12	21.268	240	1039531	20.000	ng/u1	0.00
88) Perylene-d12	24.168	264	1290134	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	11865	4.601	ng/uL	0.00
4) Pyridine-d5	3.563	84	54284	7.021	ng/u1	0.00
7) Phenol-d5	6.816	99	70645	7.223	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	230573	38.168	ng/u1	0.00
11) 2-Chlorophenol-d4	7.175	132	218747	29.482	ng/u1	0.00
15) 4-Methylphenol-d8	8.346	113	143775	17.539	ng/u1	0.00
21) Nitrobenzene-d5	8.798	128	149913	38.055	ng/u1	0.00
24) 2-Nitrophenol-d4	9.510	143	142292	39.484	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	272661	34.560	ng/u1	0.00
31) 4-Chloroaniline-d4	10.563	131	338070	26.028	ng/u1	0.00
46) Dimethylphthalate-d6	13.704	166	1177073	43.635	ng/u1	0.00
49) Acenaphthylene-d8	13.975	160	1244693	40.132	ng/u1	0.00
54) 4-Nitrophenol-d4	14.498	143	32383	6.276	ng/u1	0.00
60) Fluorene-d10	15.281	176	1023085	43.341	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	142542	34.468	ng/u1	0.00
73) Anthracene-d10	17.133	188	1729134	42.834	ng/u1	0.00
81) Pyrene-d10	19.433	212	2209953	39.542	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.974	264	2771467	46.621	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.181	88	2768	1.002 ng/uL#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030989.D
Acq On : 18 Apr 2024 00:04
Operator : MA/JU
Sample : P2100-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP2


Quant Time: Apr 18 00:49:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 17 22:24:16 2024
Response via : Initial Calibration

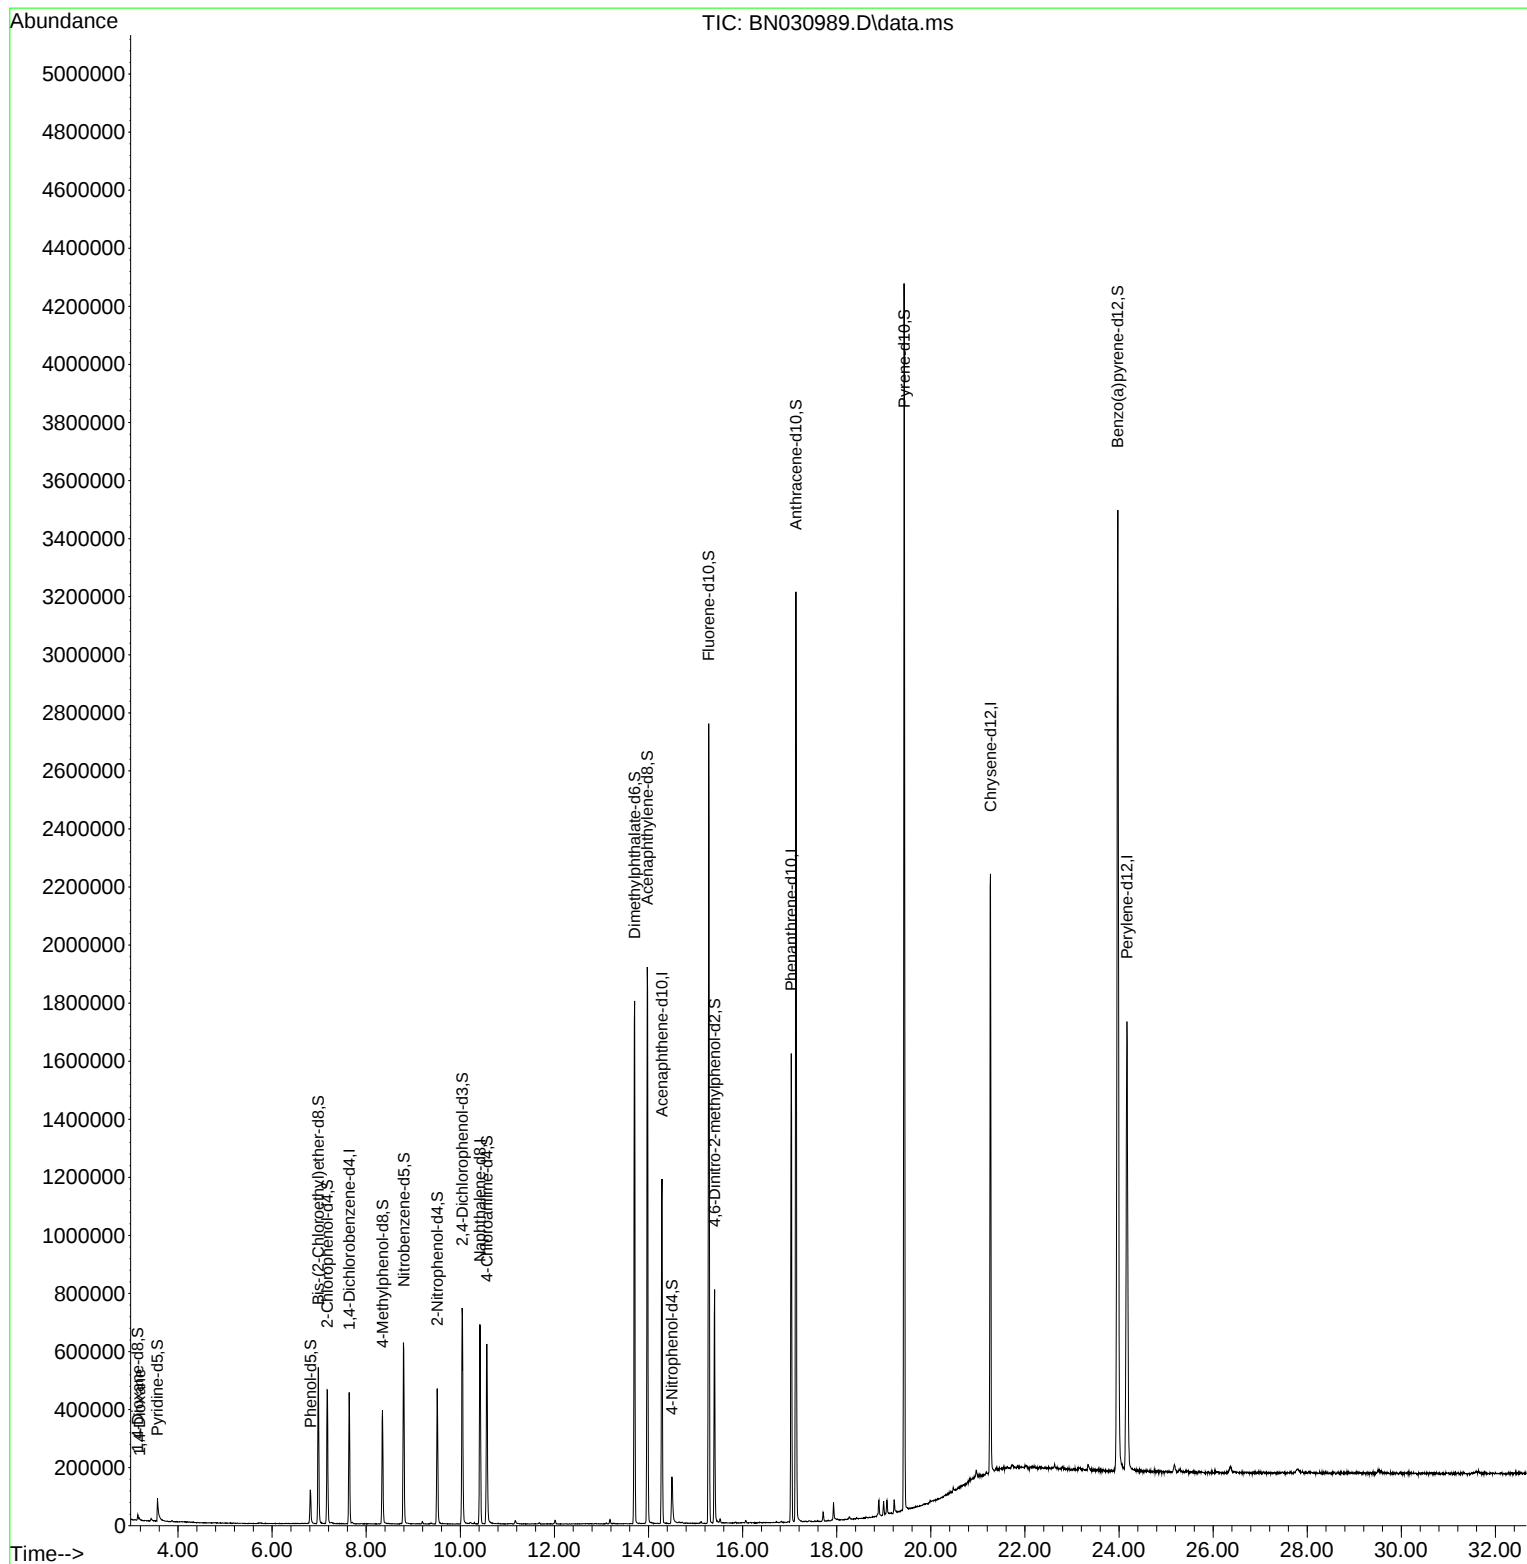

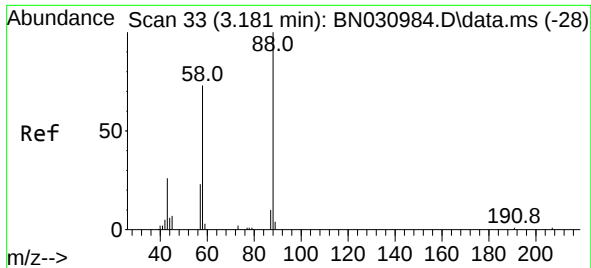

#2
 1,4-Dioxane
 Concen: 1.002 ng/uL
 RT: 3.181 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN030989.D
 Acq: 18 Apr 2024 00:04

Instrument :
 BNA_N
 ClientSampleId :
 C0AP2

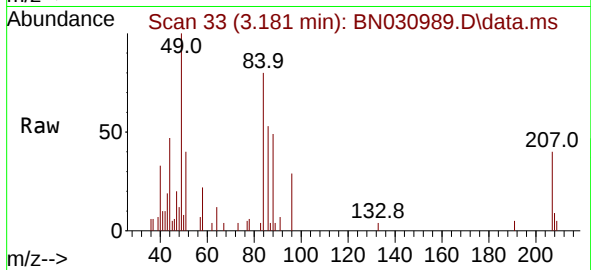

Tgt Ion:	88	Resp:	2768
Ion	Ratio	Lower	Upper
88	100		
43	38.0	23.8	35.8#
58	44.8	56.6	84.8#

