

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030979.D
 Acq On : 17 Apr 2024 16:07
 Operator : MA/JU
 Sample : P2036-04DL 20X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSX1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030979.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	17	22	31	rBV	2531389	4243734	100.00%	29.404%
2	3.646	106	112	115	rBV7	3926	7990	0.19%	0.055%
3	3.870	146	150	154	rBV4	4230	6718	0.16%	0.047%
4	3.981	164	169	177	rVB8	7346	15830	0.37%	0.110%
5	4.387	232	238	251	rVV	180308	298814	7.04%	2.070%
6	4.493	251	256	261	rVB7	2875	6220	0.15%	0.043%
7	5.664	452	455	461	rBV7	4897	7290	0.17%	0.051%
8	6.987	674	680	689	rVB	13949	24865	0.59%	0.172%
9	7.181	706	713	719	rBV4	10696	18791	0.44%	0.130%
10	7.640	785	791	803	rBV	350270	547761	12.91%	3.795%
11	8.346	906	911	916	rBV6	5497	9738	0.23%	0.067%
12	8.799	982	988	997	rBV2	12522	22027	0.52%	0.153%
13	9.510	1106	1109	1117	rVB3	6963	13030	0.31%	0.090%
14	10.052	1195	1201	1208	rBV4	9626	18832	0.44%	0.130%
15	10.422	1257	1264	1273	rBV	513584	840264	19.80%	5.822%
16	10.569	1284	1289	1299	rVB3	11724	22081	0.52%	0.153%
17	13.187	1727	1734	1738	rBV6	4994	8701	0.21%	0.060%
18	13.704	1814	1822	1828	rBV	49321	71824	1.69%	0.498%
19	13.975	1863	1868	1875	rBV	39762	61657	1.45%	0.427%
20	14.287	1913	1921	1931	rBV	911229	1284886	30.28%	8.903%
21	15.281	2085	2090	2100	rVB	70636	107080	2.52%	0.742%
22	15.404	2105	2111	2119	rBV6	10138	16591	0.39%	0.115%
23	17.034	2382	2388	2400	rBV	1214647	1691197	39.85%	11.718%
24	17.134	2400	2405	2413	rBV	76915	110846	2.61%	0.768%
25	17.939	2537	2542	2548	rBV4	20595	37471	0.88%	0.260%
26	19.228	2757	2761	2769	rBV8	18544	35374	0.83%	0.245%
27	19.433	2792	2796	2803	rBV	112154	160947	3.79%	1.115%
28	21.269	3103	3108	3119	rBV	1563003	2179608	51.36%	15.102%
29	24.168	3593	3601	3619	rVB2	1013251	2562094	60.37%	17.753%




Sum of corrected areas: 14432261

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030979.D
Acq On : 17 Apr 2024 16:07
Operator : MA/JU
Sample : P2036-04DL 20X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

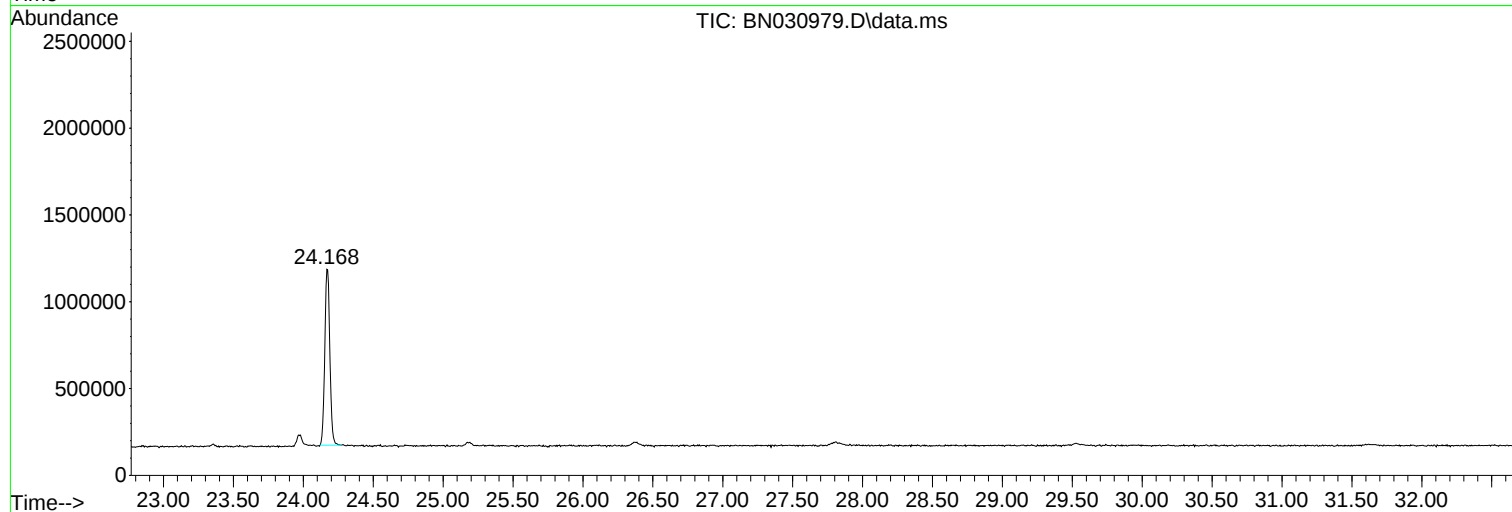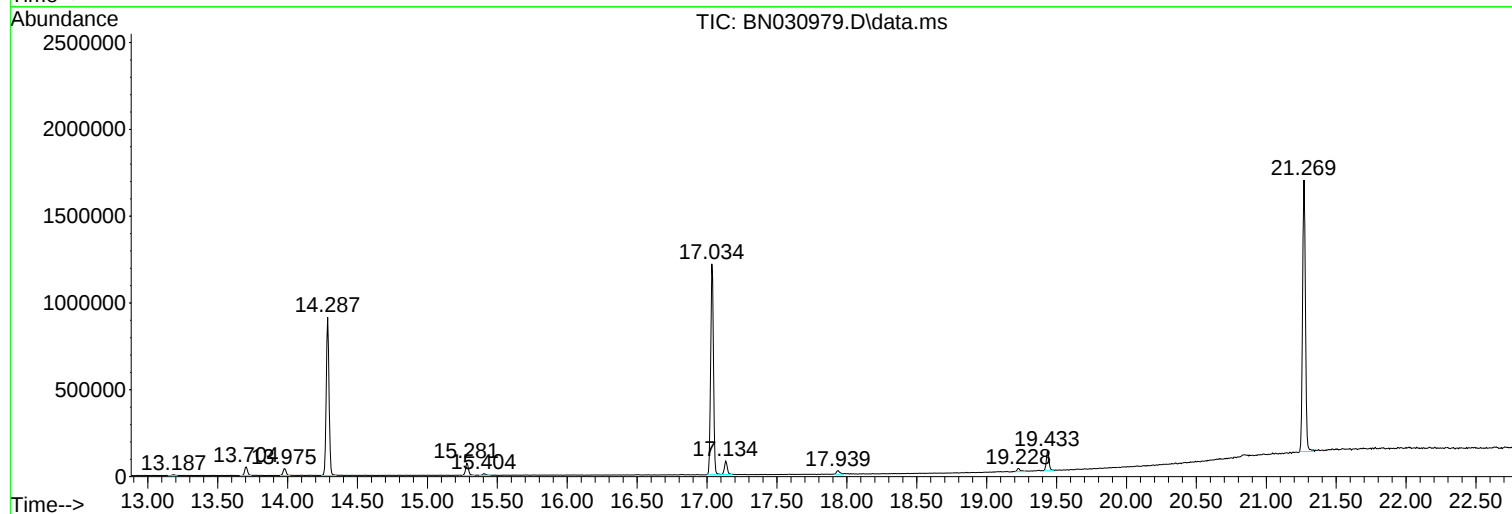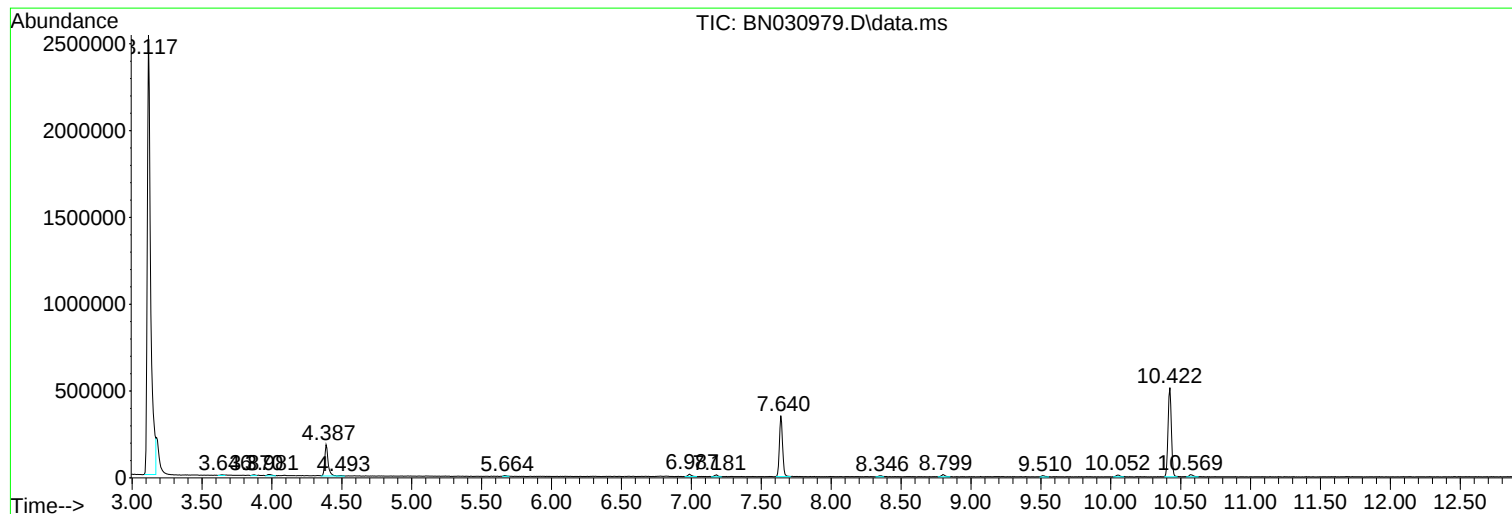

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030979.D
Acq On : 17 Apr 2024 16:07
Operator : MA/JU
Sample : P2036-04DL 20X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX1DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.387	10.91 ng/ul	298814	1,4-Dichlorobenzene-d4	7.640

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	32

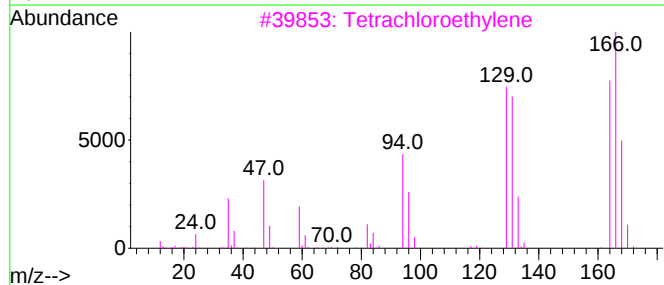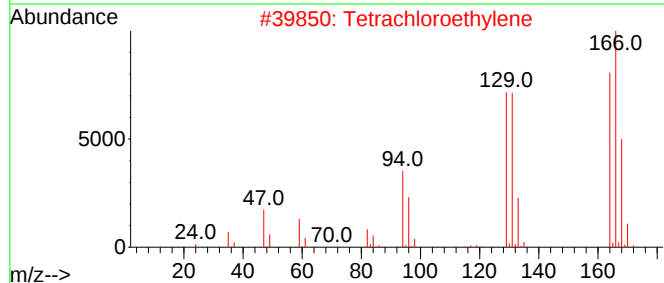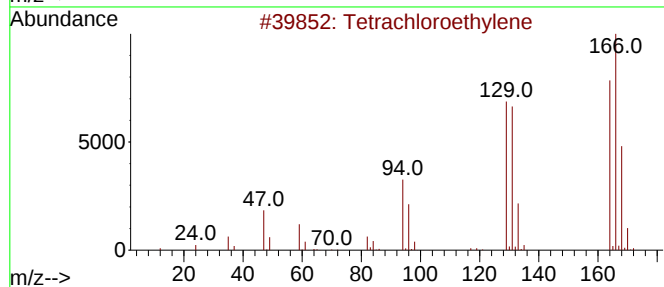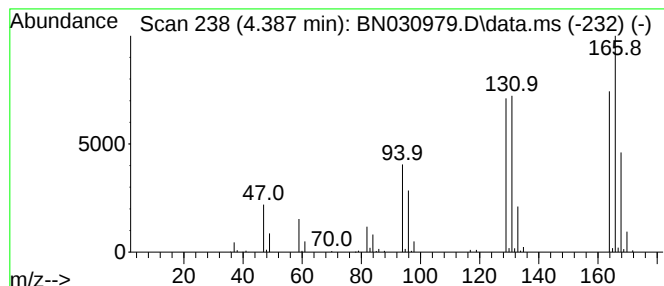

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030979.D
Acq On : 17 Apr 2024 16:07
Operator : MA/JU
Sample : P2036-04DL 20X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSX1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.387	10.9	ng/ul	298814	1	7.640	547761	20.0