

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030986.D
 Acq On : 17 Apr 2024 22:05
 Operator : MA/JU
 Sample : P2100-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	18	22	40	rVB2	174069	342905	4.71%	0.656%
2	3.428	72	75	78	rBV3	5940	8106	0.11%	0.016%
3	3.564	96	98	115	rBV	92067	189856	2.61%	0.363%
4	4.387	233	238	244	rBV2	18474	30221	0.42%	0.058%
5	4.793	300	307	310	rBV5	4339	8096	0.11%	0.015%
6	5.346	396	401	405	rBV	18180	29893	0.41%	0.057%
7	6.811	645	650	661	rVB	116055	196959	2.71%	0.377%
8	6.981	672	679	692	rBV	572652	905178	12.44%	1.731%
9	7.175	705	712	722	rBV	503885	820111	11.27%	1.569%
10	7.640	784	791	800	rBV	472870	748616	10.29%	1.432%
11	8.346	904	911	926	rBV	417140	658980	9.06%	1.261%
12	8.793	980	987	999	rBV	675297	1097750	15.09%	2.100%
13	9.193	1049	1055	1064	rVB2	38185	59267	0.81%	0.113%
14	9.510	1098	1109	1118	rBV	496734	795140	10.93%	1.521%
15	10.040	1193	1199	1215	rBV	782254	1327373	18.24%	2.539%
16	10.422	1256	1264	1273	rVB	718224	1200644	16.50%	2.297%
17	10.563	1280	1288	1306	rBV	695878	1232429	16.94%	2.357%
18	11.169	1385	1391	1396	rBV2	12083	23095	0.32%	0.044%
19	11.681	1474	1478	1484	rVB3	6321	9876	0.14%	0.019%
20	11.963	1519	1526	1531	rBV	30325	59492	0.82%	0.114%
21	12.010	1531	1534	1542	rVB2	15272	26852	0.37%	0.051%
22	13.181	1728	1733	1741	rVB2	12552	20548	0.28%	0.039%
23	13.704	1815	1822	1829	rBV	1892931	2672663	36.73%	5.112%
24	13.975	1861	1868	1883	rBV	2046161	3001476	41.25%	5.741%
25	14.287	1914	1921	1930	rBV	1244108	1789723	24.60%	3.423%
26	14.510	1950	1959	1978	rBV	1282652	2805393	38.56%	5.366%
27	15.281	2083	2090	2097	rBV	2784210	3954137	54.35%	7.564%
28	15.404	2103	2111	2125	rBV	797793	1071390	14.73%	2.049%
29	15.522	2127	2131	2136	rVB2	12764	16744	0.23%	0.032%
30	16.010	2210	2214	2220	rBV6	5373	9020	0.12%	0.017%
31	16.063	2220	2223	2229	rVB4	9200	13625	0.19%	0.026%
32	16.804	2344	2349	2352	rBV6	5663	10806	0.15%	0.021%
33	17.034	2382	2388	2398	rBV	1655007	2341856	32.19%	4.480%
34	17.134	2398	2405	2417	rBV2	3211957	4590240	63.09%	8.780%
35	17.710	2497	2503	2509	rBV6	22604	37363	0.51%	0.071%
36	17.934	2536	2541	2547	rBV2	65030	94192	1.29%	0.180%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030986.D
Acq On : 17 Apr 2024 22:05
Operator : MA/JU
Sample : P2100-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	18.234	2588	2592	2595	rBV6	5905	9122	0.13%	0.017%
38	18.269	2595	2598	2606	rVB9	7798	13454	0.18%	0.026%
39	18.810	2687	2690	2696	rBV6	10153	14491	0.20%	0.028%
40	18.898	2701	2705	2712	rVB4	38326	52302	0.72%	0.100%
41	18.998	2717	2722	2725	rBV	47149	62435	0.86%	0.119%
42	19.034	2725	2728	2730	rVV3	11790	14166	0.19%	0.027%
43	19.069	2730	2734	2739	rVV	43558	65172	0.90%	0.125%
44	19.128	2742	2744	2750	rVB5	15958	20142	0.28%	0.039%
45	19.222	2757	2760	2770	rBV	37465	56098	0.77%	0.107%
46	19.439	2790	2797	2811	rBV	4099547	5800388	79.72%	11.095%
47	21.269	3102	3108	3116	rBV2	2180401	3037215	41.74%	5.810%
48	23.974	3559	3568	3581	rBV2	3028952	7275715	100.00%	13.917%
49	24.169	3593	3601	3617	rVB2	1504701	3657053	50.26%	6.995%




Sum of corrected areas: 52277768

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030986.D
Acq On : 17 Apr 2024 22:05
Operator : MA/JU
Sample : P2100-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

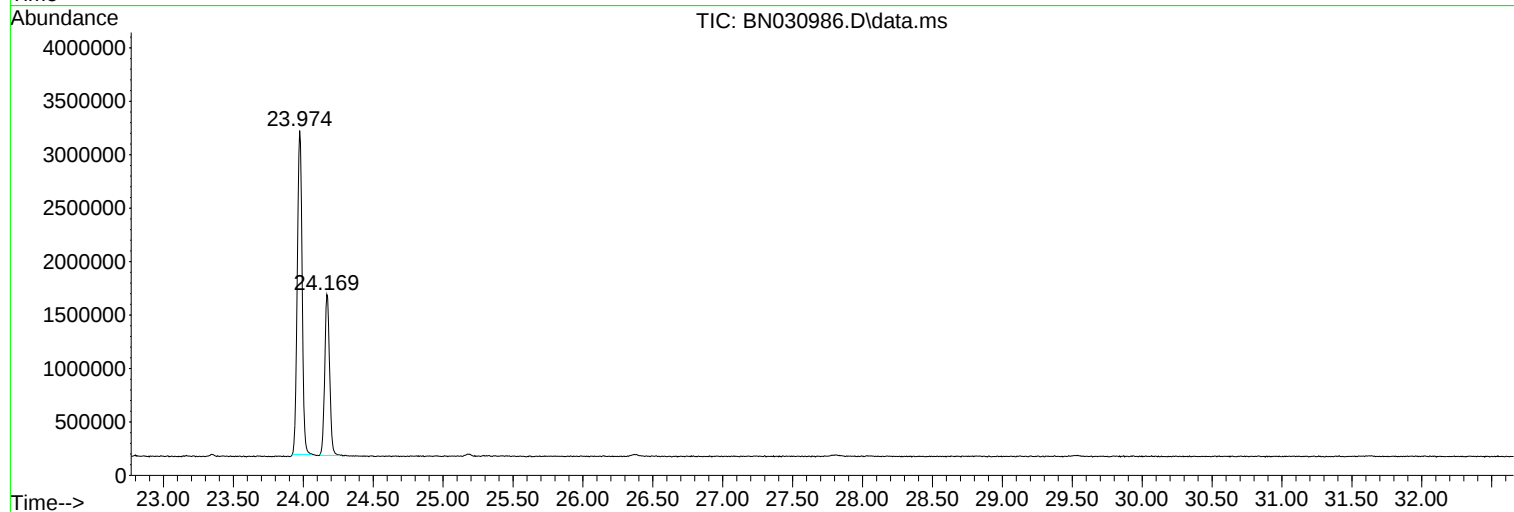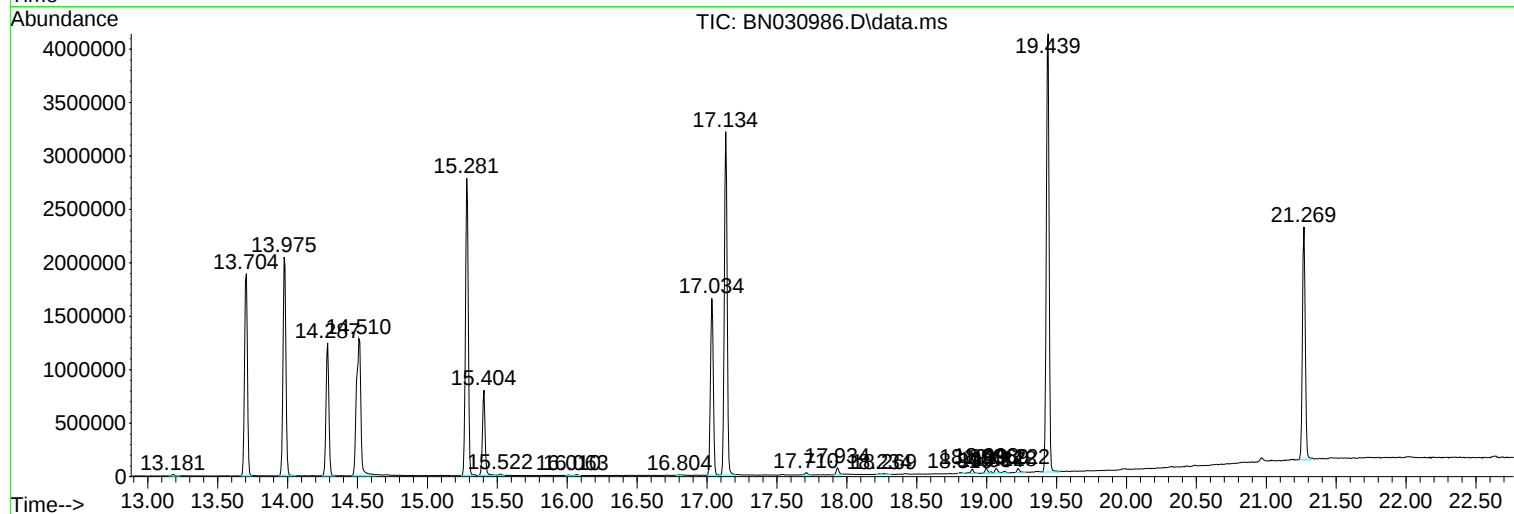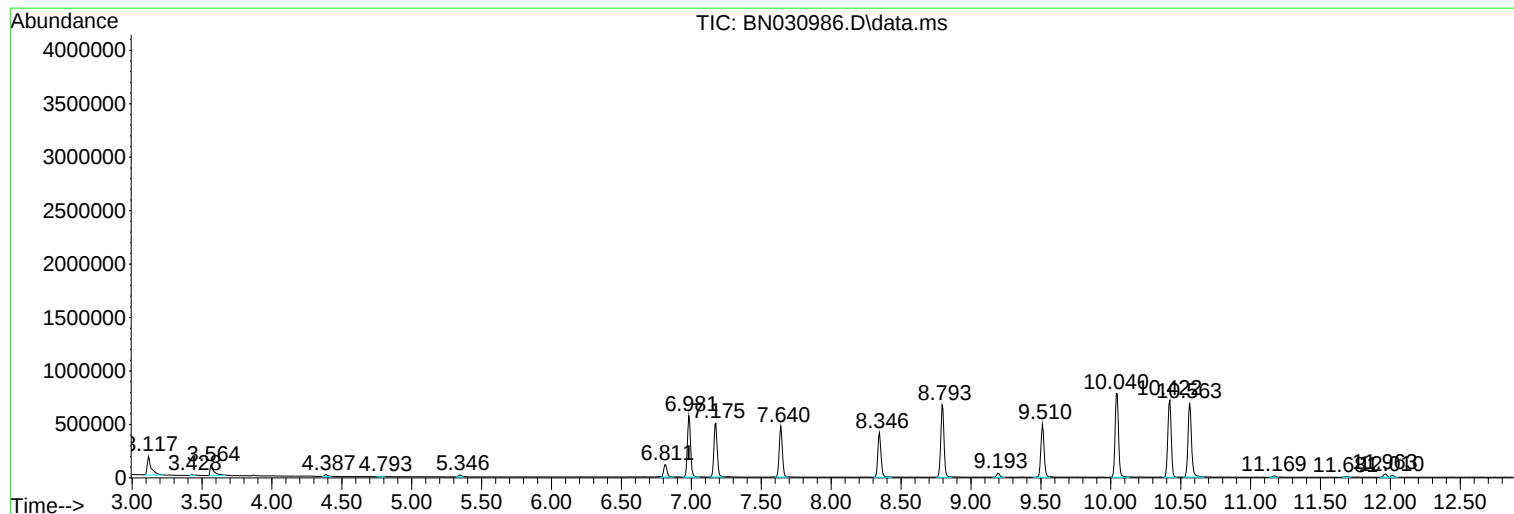

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030986.D
Acq On : 17 Apr 2024 22:05
Operator : MA/JU
Sample : P2100-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030986.D
Acq On : 17 Apr 2024 22:05
Operator : MA/JU
Sample : P2100-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------