

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030987.D
 Acq On : 17 Apr 2024 22:44
 Operator : MA/JU
 Sample : P2100-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	17	22	43	rVB2	201900	402779	4.86%	0.709%
2	3.564	96	98	117	rBV	105579	223239	2.69%	0.393%
3	3.875	147	151	156	rVB2	7345	10180	0.12%	0.018%
4	4.387	234	238	247	rVB2	21162	36429	0.44%	0.064%
5	4.787	302	306	311	rVB6	4132	8501	0.10%	0.015%
6	5.346	395	401	405	rBV	6956	12907	0.16%	0.023%
7	6.816	645	651	658	rVB	138685	220897	2.67%	0.389%
8	6.981	672	679	690	rBV	672250	1056487	12.75%	1.860%
9	7.169	704	711	722	rBV	606103	991854	11.97%	1.746%
10	7.581	777	781	784	rBV3	5688	9115	0.11%	0.016%
11	7.640	784	791	801	rVV	552935	892360	10.77%	1.571%
12	8.346	904	911	922	rBV	479108	771261	9.31%	1.358%
13	8.793	980	987	1002	rBV	794784	1295877	15.64%	2.282%
14	9.193	1050	1055	1061	rVB	25358	39213	0.47%	0.069%
15	9.510	1101	1109	1122	rBV	606945	969984	11.70%	1.708%
16	10.040	1192	1199	1213	rBV	936894	1538649	18.57%	2.709%
17	10.422	1256	1264	1277	rVB	851516	1412201	17.04%	2.487%
18	10.563	1280	1288	1308	rBV	715746	1235282	14.91%	2.175%
19	11.687	1473	1479	1484	rVB3	6626	10331	0.12%	0.018%
20	11.963	1517	1526	1531	rBV	44025	80595	0.97%	0.142%
21	12.016	1531	1535	1541	rVB	18986	32595	0.39%	0.057%
22	13.181	1727	1733	1739	rBV2	14974	25616	0.31%	0.045%
23	13.704	1815	1822	1835	rBV	2191158	3018011	36.42%	5.314%
24	13.975	1861	1868	1878	rBV	2294914	3454162	41.68%	6.082%
25	14.287	1913	1921	1933	rBV	1460005	2100653	25.35%	3.699%
26	14.498	1951	1957	1970	rBV	134645	248876	3.00%	0.438%
27	15.281	2083	2090	2097	rBV	3137787	4486218	54.13%	7.899%
28	15.404	2104	2111	2125	rBV	952591	1264726	15.26%	2.227%
29	15.522	2127	2131	2137	rVB2	13561	18959	0.23%	0.033%
30	16.069	2220	2224	2228	rBV4	12307	17537	0.21%	0.031%
31	16.822	2349	2352	2360	rVB4	4906	8877	0.11%	0.016%
32	17.034	2382	2388	2398	rBV	2009942	2752820	33.22%	4.847%
33	17.134	2399	2405	2417	rBV2	3745959	5189587	62.62%	9.138%
34	17.710	2498	2503	2509	rBV3	23844	33648	0.41%	0.059%
35	17.934	2537	2541	2547	rBV2	34830	49356	0.60%	0.087%
36	18.263	2594	2597	2601	rVB3	6845	9478	0.11%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030987.D
Acq On : 17 Apr 2024 22:44
Operator : MA/JU
Sample : P2100-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	18.422	2621	2624	2629	rBV5	8462	13376	0.16%	0.024%
38	18.998	2717	2722	2726	rBV	54849	72696	0.88%	0.128%
39	19.069	2730	2734	2738	rBV	49396	65820	0.79%	0.116%
40	19.222	2756	2760	2767	rBV4	38640	58938	0.71%	0.104%
41	19.433	2790	2796	2804	rBV	4605394	6604482	79.69%	11.629%
42	21.269	3102	3108	3118	rBV2	2458766	3495675	42.18%	6.155%
43	23.974	3558	3568	3586	rBV2	3337376	8287426	100.00%	14.593%
44	24.168	3592	3601	3615	rBV	1776459	4263633	51.45%	7.508%




Sum of corrected areas: 56791306

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030987.D
Acq On : 17 Apr 2024 22:44
Operator : MA/JU
Sample : P2100-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

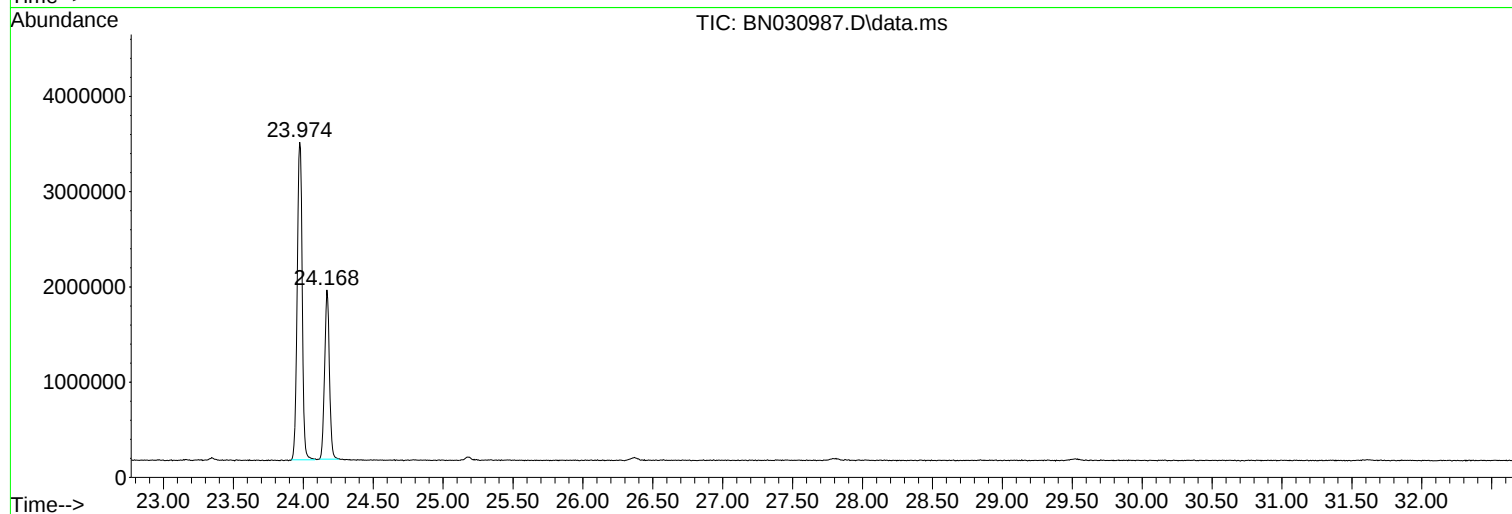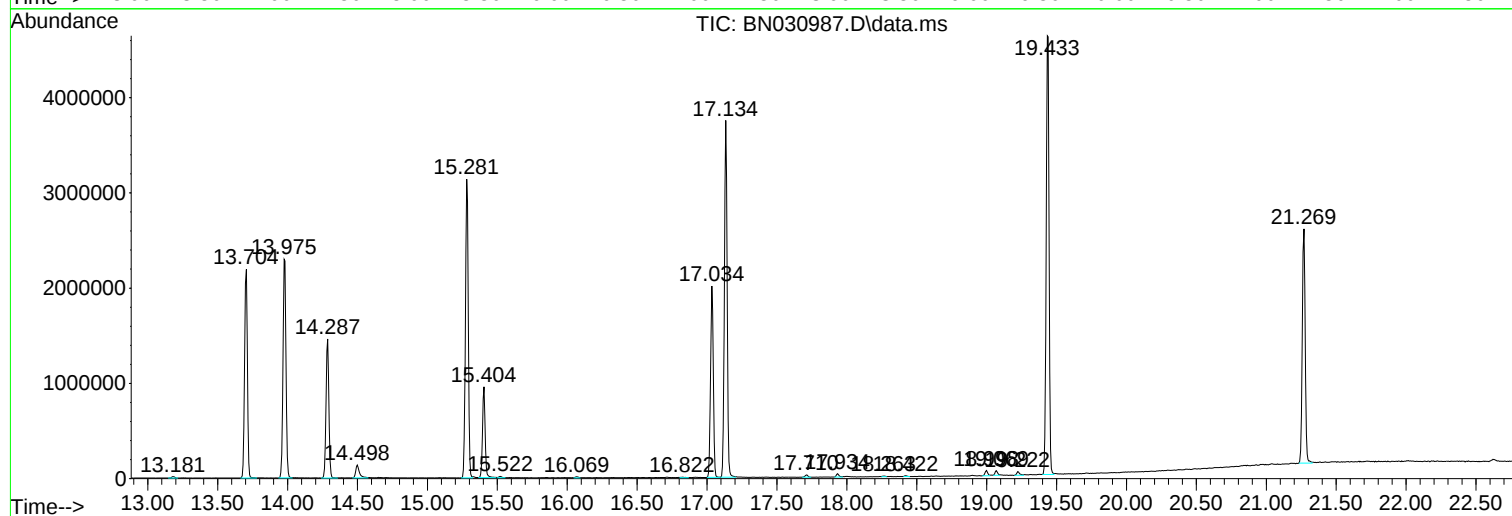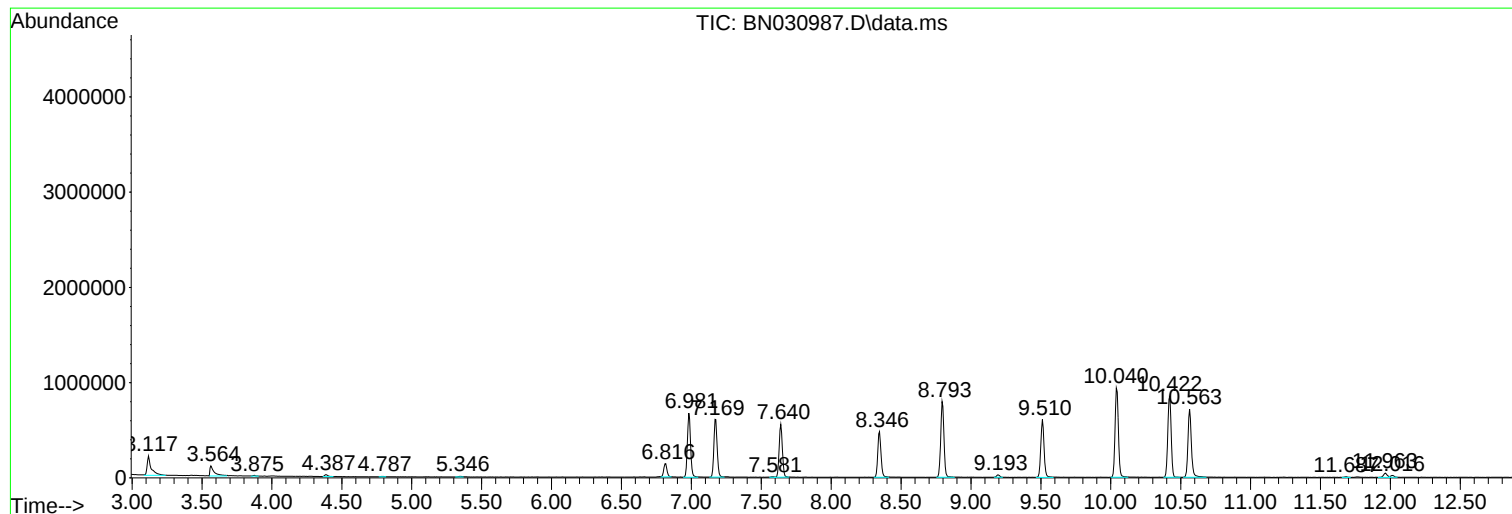

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030987.D
Acq On : 17 Apr 2024 22:44
Operator : MA/JU
Sample : P2100-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030987.D
Acq On : 17 Apr 2024 22:44
Operator : MA/JU
Sample : P2100-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc