

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030989.D
 Acq On : 18 Apr 2024 00:04
 Operator : MA/JU
 Sample : P2100-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	31	rBV	18747	25614	0.33%	0.053%
2	3.181	31	33	40	rVB3	8790	11320	0.15%	0.023%
3	3.428	71	75	78	rBV4	8137	11499	0.15%	0.024%
4	3.563	96	98	114	rBV	78517	158062	2.06%	0.326%
5	3.863	147	149	155	rVB5	5005	8935	0.12%	0.018%
6	6.816	644	651	660	rBV	114466	193170	2.52%	0.399%
7	6.981	673	679	689	rBV	538005	840561	10.98%	1.735%
8	7.169	704	711	721	rBV	461031	752351	9.83%	1.553%
9	7.640	783	791	798	rBV	452825	710145	9.27%	1.466%
10	7.699	798	801	807	rVB4	4877	8620	0.11%	0.018%
11	8.346	904	911	924	rBV	391374	625470	8.17%	1.291%
12	8.793	980	987	999	rVV	623911	1018462	13.30%	2.102%
13	9.193	1050	1055	1062	rBV2	8418	12430	0.16%	0.026%
14	9.510	1101	1109	1119	rBV	466797	750762	9.80%	1.550%
15	10.040	1193	1199	1214	rBV	744450	1245596	16.27%	2.571%
16	10.210	1225	1228	1234	rVB6	4357	8307	0.11%	0.017%
17	10.416	1256	1263	1273	rBV	687756	1149881	15.02%	2.374%
18	10.563	1280	1288	1303	rBV	619468	1072258	14.00%	2.213%
19	11.169	1385	1391	1397	rBV3	11279	22848	0.30%	0.047%
20	11.687	1471	1479	1482	rVB5	4844	10236	0.13%	0.021%
21	12.010	1527	1534	1540	rBV2	13321	24786	0.32%	0.051%
22	13.181	1725	1733	1738	rBV2	15321	24511	0.32%	0.051%
23	13.704	1815	1822	1833	rBV	1801264	2521865	32.93%	5.206%
24	13.975	1858	1868	1879	rBV	1917480	2833058	37.00%	5.848%
25	14.286	1914	1921	1933	rBV	1186817	1727344	22.56%	3.566%
26	14.498	1950	1957	1969	rBV2	161252	332703	4.34%	0.687%
27	15.281	2083	2090	2101	rBV	2754730	3824017	49.94%	7.894%
28	15.404	2105	2111	2122	rBV	803198	1060744	13.85%	2.190%
29	15.522	2127	2131	2138	rVB2	14368	23561	0.31%	0.049%
30	16.069	2220	2224	2229	rVB4	9196	13605	0.18%	0.028%
31	17.033	2382	2388	2398	rBV	1614544	2279914	29.77%	4.706%
32	17.133	2398	2405	2423	rVV2	3203048	4527679	59.13%	9.346%
33	17.710	2499	2503	2509	rVB	31129	43109	0.56%	0.089%
34	17.933	2537	2541	2551	rVV2	60734	86398	1.13%	0.178%
35	18.269	2594	2598	2602	rBV6	8163	12900	0.17%	0.027%
36	18.422	2621	2624	2629	rBV5	5558	8048	0.11%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030989.D
Acq On : 18 Apr 2024 00:04
Operator : MA/JU
Sample : P2100-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	18.898	2701	2705	2711	rVB2	51757	64555	0.84%	0.133%
38	18.998	2718	2722	2725	rBV2	46145	53778	0.70%	0.111%
39	19.069	2729	2734	2742	rBV	47881	74987	0.98%	0.155%
40	19.221	2756	2760	2768	rBV3	46716	68936	0.90%	0.142%
41	19.433	2790	2796	2804	rBV	4226152	5898047	77.03%	12.175%
42	21.268	3102	3108	3121	rBV2	2061013	3002795	39.21%	6.199%
43	23.974	3559	3568	3581	rBV2	3293147	7657303	100.00%	15.807%
44	24.168	3592	3601	3613	rBV	1535562	3642332	47.57%	7.519%




Sum of corrected areas: 48443502

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030989.D
Acq On : 18 Apr 2024 00:04
Operator : MA/JU
Sample : P2100-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

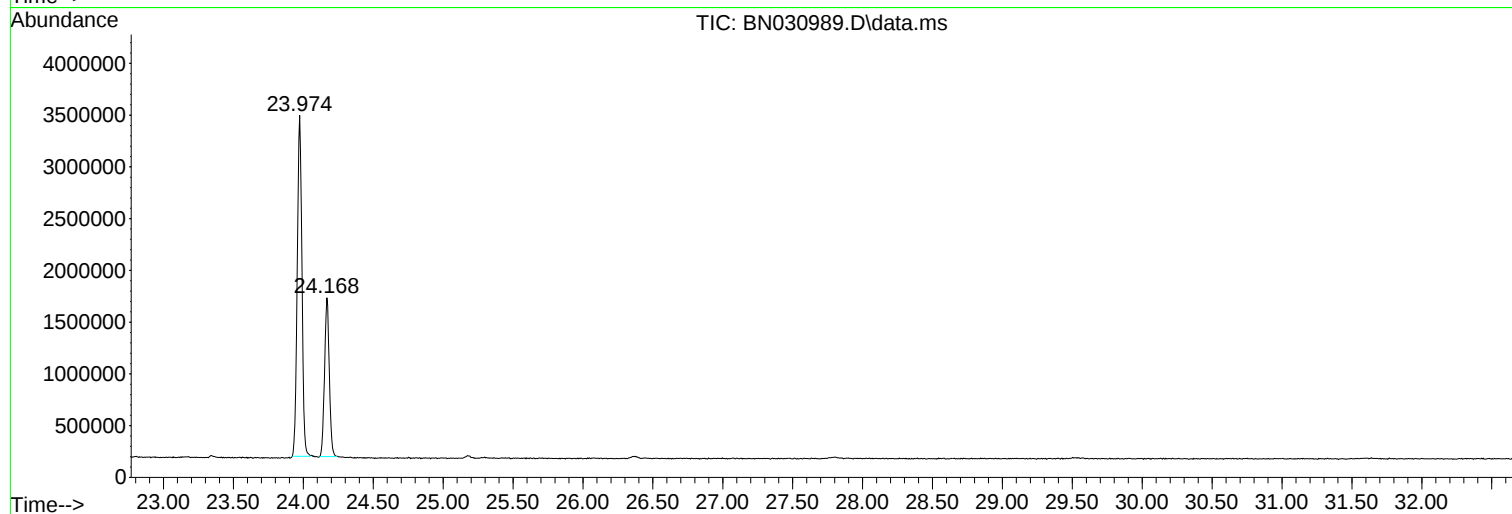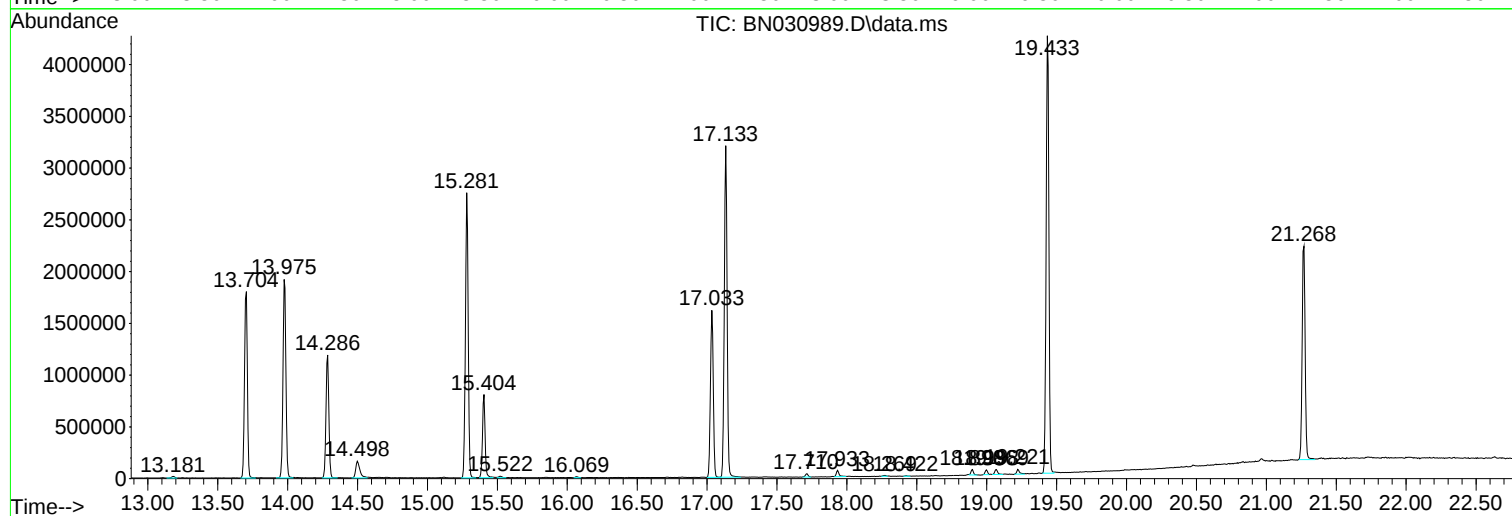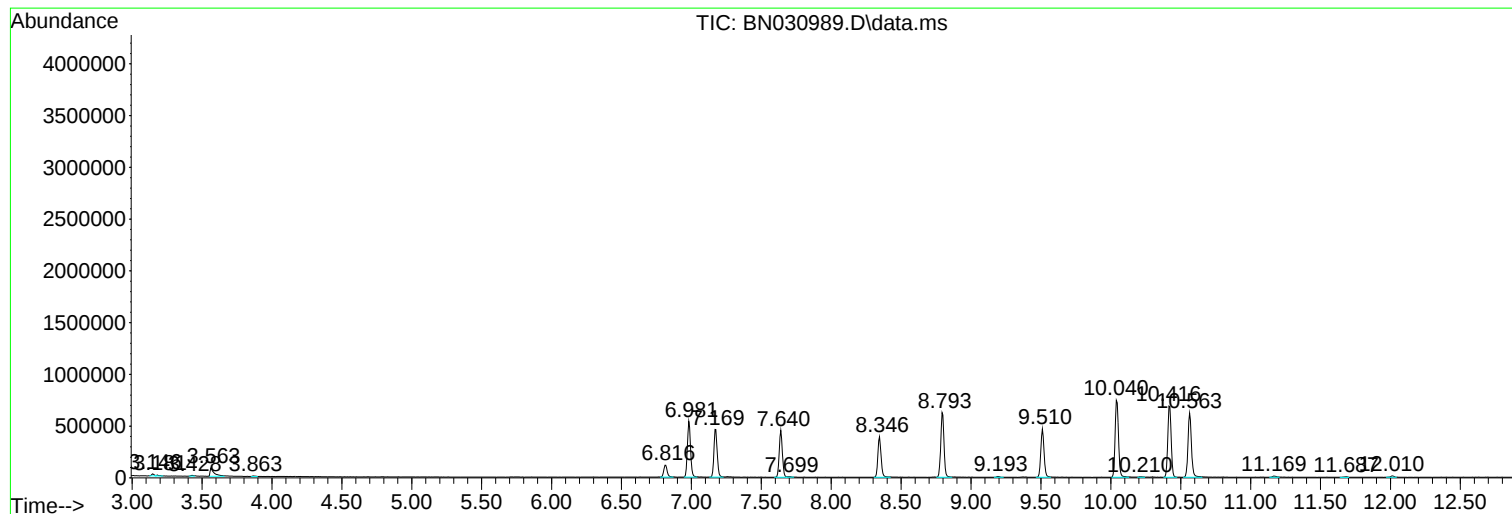

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030989.D
Acq On : 18 Apr 2024 00:04
Operator : MA/JU
Sample : P2100-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030989.D
Acq On : 18 Apr 2024 00:04
Operator : MA/JU
Sample : P2100-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc