

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030990.D
 Acq On : 18 Apr 2024 00:43
 Operator : MA/JU
 Sample : P2100-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	35	rVB	23115	30809	0.36%	0.054%
2	3.428	71	75	85	rVB2	14844	29088	0.34%	0.051%
3	3.564	95	98	119	rBV	121947	238375	2.80%	0.420%
4	3.869	147	150	155	rVB3	6833	8578	0.10%	0.015%
5	6.816	643	651	665	rVB	125661	211083	2.48%	0.372%
6	6.981	673	679	694	rBV	640955	1012735	11.89%	1.783%
7	7.175	705	712	721	rBV	519003	842540	9.89%	1.483%
8	7.640	784	791	800	rBV	580946	906110	10.64%	1.595%
9	8.346	905	911	920	rBV	414453	648888	7.62%	1.142%
10	8.793	980	987	998	rBV	764581	1245473	14.62%	2.193%
11	9.193	1050	1055	1061	rVB	13405	21859	0.26%	0.038%
12	9.363	1080	1084	1093	rVB2	13580	23920	0.28%	0.042%
13	9.510	1101	1109	1124	rBV	546084	877672	10.30%	1.545%
14	10.040	1192	1199	1211	rBV	822003	1356597	15.93%	2.388%
15	10.210	1221	1228	1239	rBV4	16292	30354	0.36%	0.053%
16	10.422	1256	1264	1277	rBV	849792	1437724	16.88%	2.531%
17	10.563	1279	1288	1306	rBV	844331	1399405	16.43%	2.464%
18	11.169	1384	1391	1398	rBV	29286	57833	0.68%	0.102%
19	11.234	1398	1402	1409	rVB7	6971	15248	0.18%	0.027%
20	11.675	1470	1477	1485	rBV5	5038	10370	0.12%	0.018%
21	12.016	1530	1535	1541	rVB3	17145	29007	0.34%	0.051%
22	13.181	1727	1733	1740	rBV2	17960	29106	0.34%	0.051%
23	13.704	1814	1822	1837	rBV	2134852	2930665	34.41%	5.160%
24	13.975	1858	1868	1883	rBV	2327463	3398750	39.90%	5.984%
25	14.287	1914	1921	1933	rBV	1500508	2146245	25.20%	3.779%
26	14.498	1951	1957	1974	rBV	124673	236291	2.77%	0.416%
27	15.281	2084	2090	2097	rBV	3157009	4510332	52.95%	7.941%
28	15.328	2097	2098	2105	rVV5	11167	11811	0.14%	0.021%
29	15.404	2105	2111	2127	rVV	941392	1223585	14.36%	2.154%
30	15.522	2127	2131	2136	rVB	12912	19100	0.22%	0.034%
31	16.063	2220	2223	2229	rVB3	10794	16066	0.19%	0.028%
32	17.034	2382	2388	2398	rVV	2031018	2792220	32.78%	4.916%
33	17.133	2398	2405	2417	rVV2	3880505	5477457	64.30%	9.644%
34	17.233	2420	2422	2428	rVB5	8471	10808	0.13%	0.019%
35	17.539	2469	2474	2479	rBV9	4710	9962	0.12%	0.018%
36	17.716	2499	2504	2507	rVB2	14394	19200	0.23%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030990.D
Acq On : 18 Apr 2024 00:43
Operator : MA/JU
Sample : P2100-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.933	2536	2541	2548	rBV2	76110	110278	1.29%	0.194%
38	17.986	2548	2550	2558	rVB7	4238	10385	0.12%	0.018%
39	18.269	2594	2598	2606	rVB5	11123	18489	0.22%	0.033%
40	18.369	2611	2615	2620	rBV4	7863	10641	0.12%	0.019%
41	18.998	2717	2722	2726	rBV	52861	70008	0.82%	0.123%
42	19.069	2729	2734	2738	rBV	49267	70803	0.83%	0.125%
43	19.222	2756	2760	2765	rBV2	47822	63292	0.74%	0.111%
44	19.433	2790	2796	2804	rBV	4930802	6831829	80.20%	12.028%
45	20.957	3052	3055	3060	rBV4	46188	74802	0.88%	0.132%
46	21.269	3102	3108	3117	rBV	2532231	3542094	41.58%	6.236%
47	23.974	3558	3568	3584	rBV2	3564006	8517983	100.00%	14.997%
48	24.168	3593	3601	3613	rVB	1793177	4212356	49.45%	7.416%




Sum of corrected areas: 56798226

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030990.D
Acq On : 18 Apr 2024 00:43
Operator : MA/JU
Sample : P2100-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

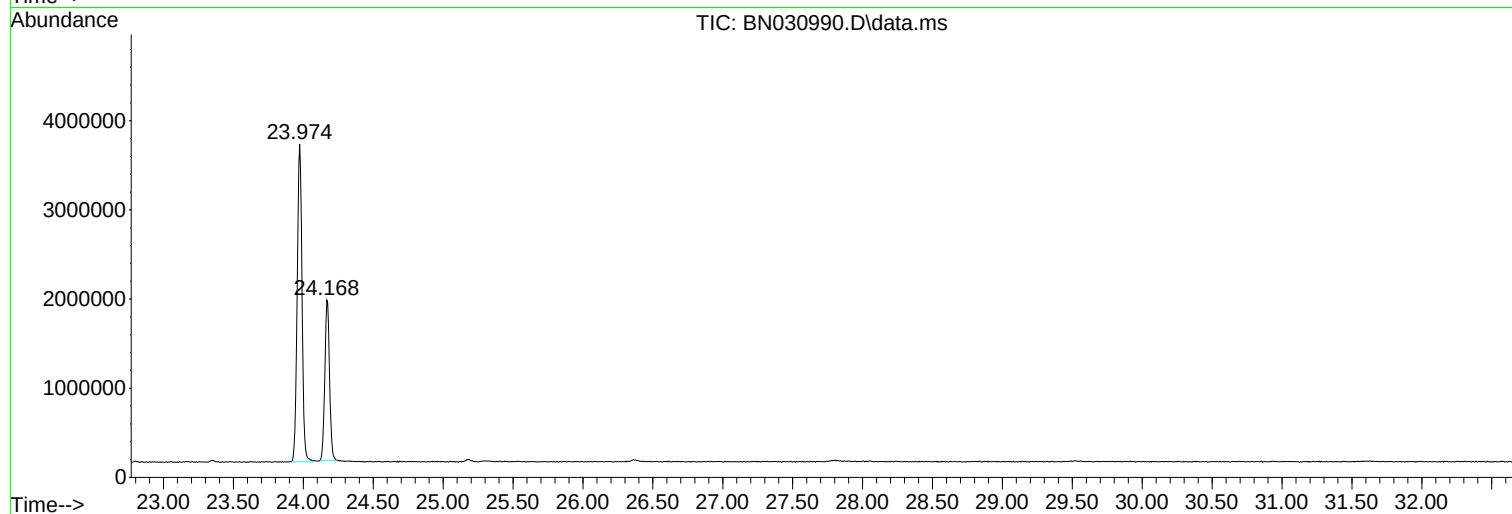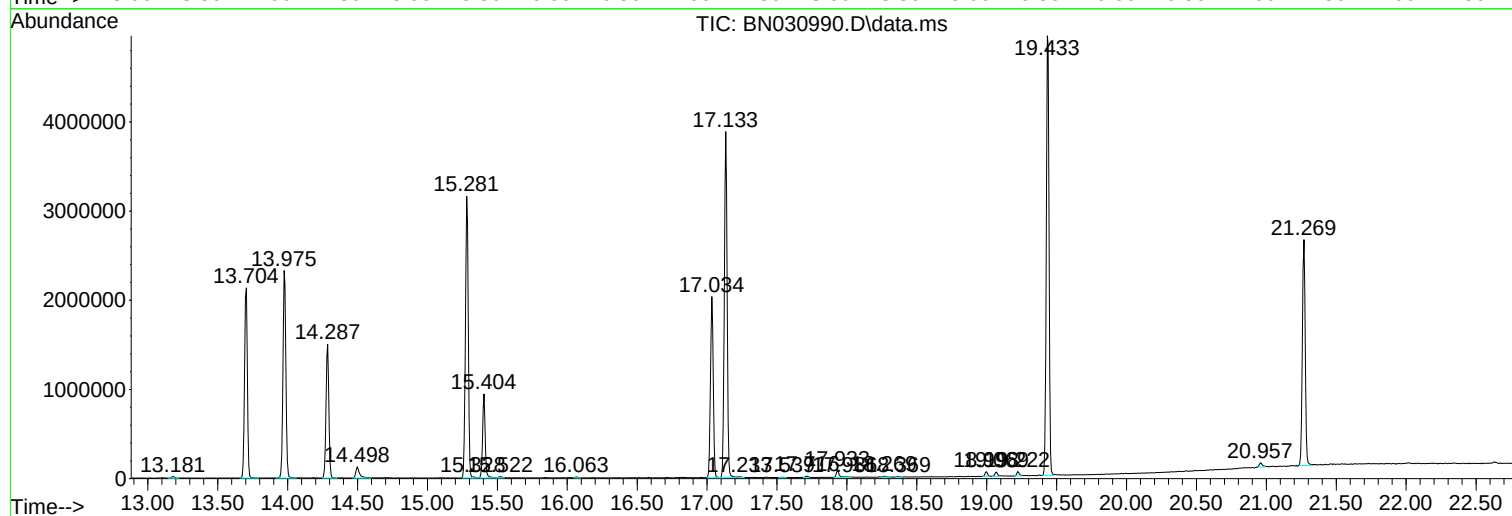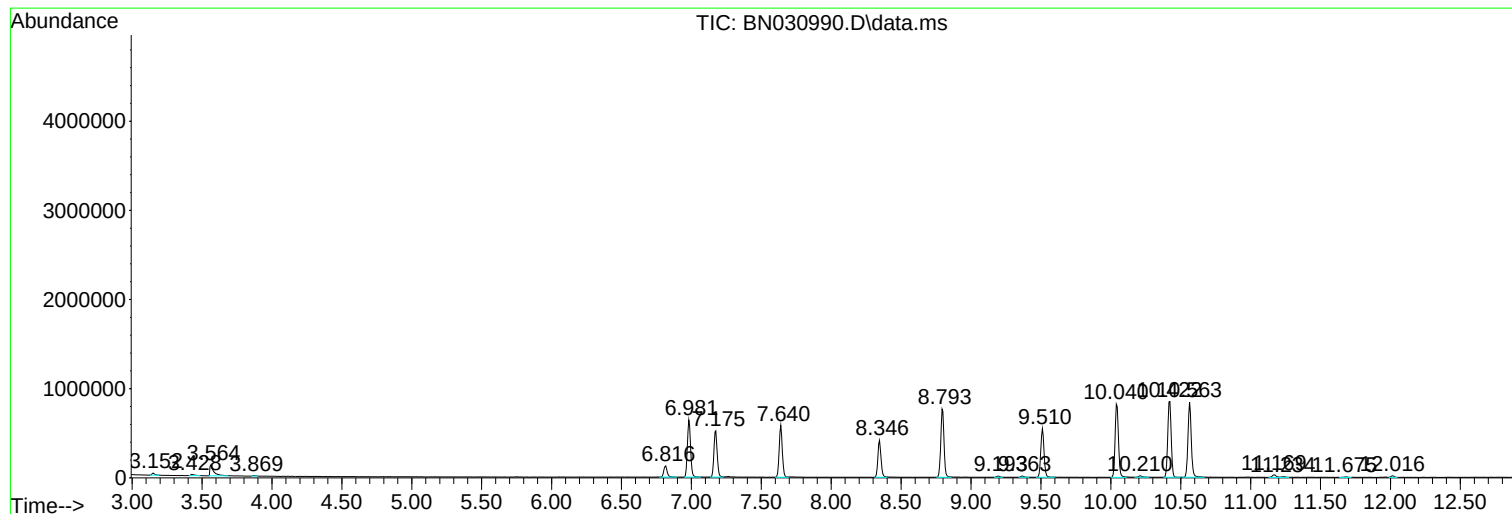

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030990.D
Acq On : 18 Apr 2024 00:43
Operator : MA/JU
Sample : P2100-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030990.D
Acq On : 18 Apr 2024 00:43
Operator : MA/JU
Sample : P2100-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc